

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010523\
 Data File : P0091851.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2023 15:25
 Operator : YP/AJ
 Sample : 01027-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-1-1-4-2023

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/06/2023
 Supervised By :Ankita Jodhani 01/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 20:41:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 05 01:51:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.292	3.469	73038843	32249056	22.728	23.360
2) SA Decachlor...	10.033	8.465	48988826	11289242	20.638	8.970m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010523\
Data File : PO091851.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2023 15:25
Operator : YP/AJ
Sample : 01027-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-1-1-4-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/06/2023
Supervised By :Ankita Jodhani 01/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 20:41:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010423.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 05 01:51:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

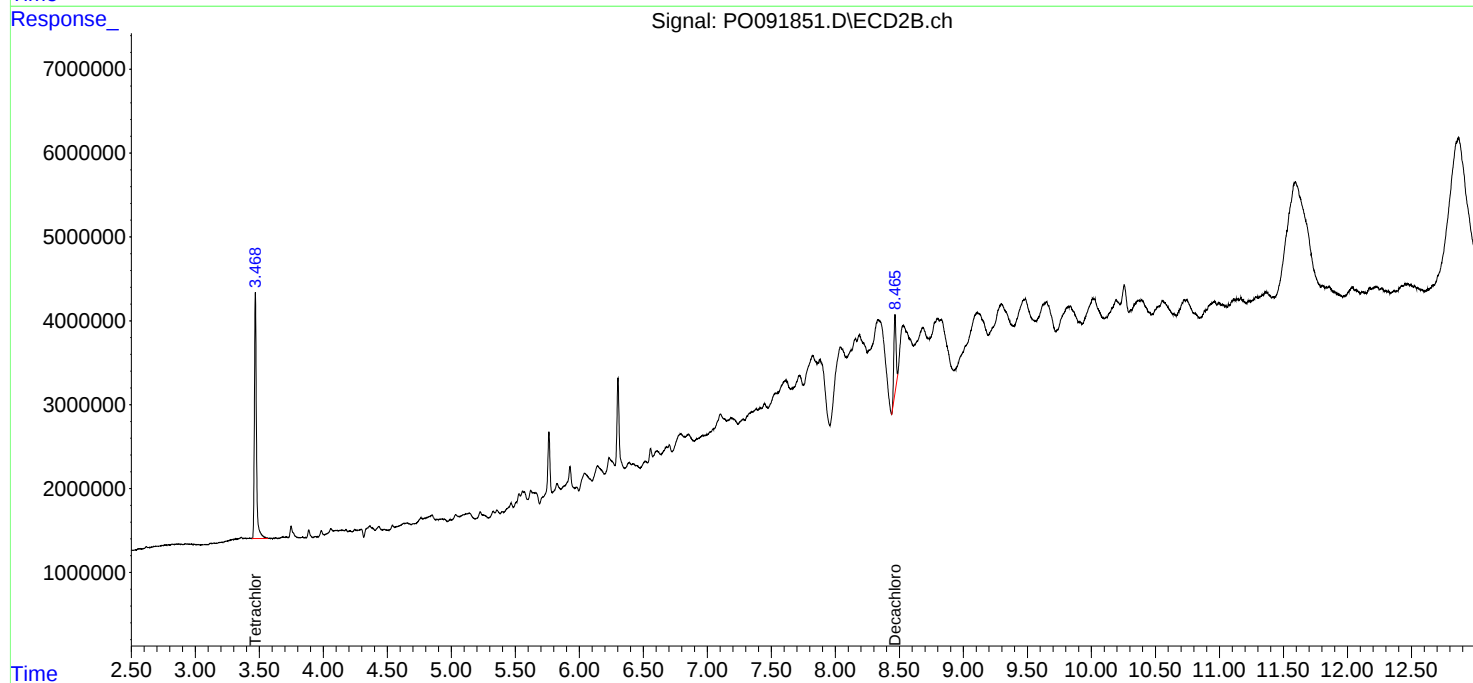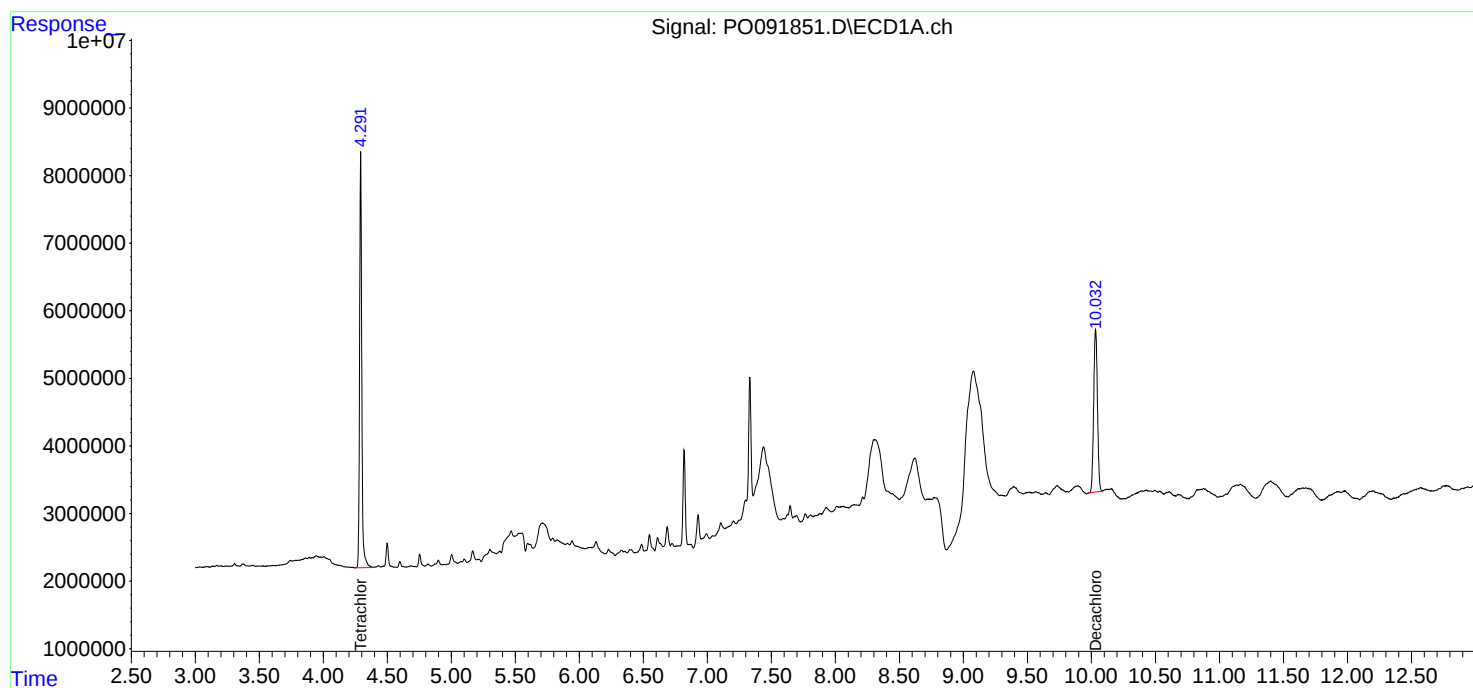

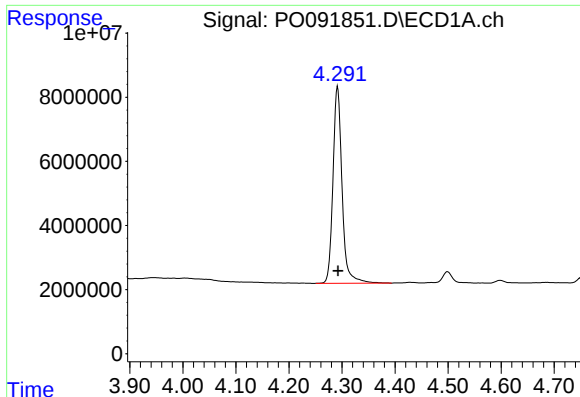


#1 Tetrachloro-m-xylene

R.T.: 4.292 min
Delta R.T.: -0.001 min
Response: 73038843
Conc: 22.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1-1-4-2023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/06/2023
Supervised By :Ankita Jodhani 01/06/2023

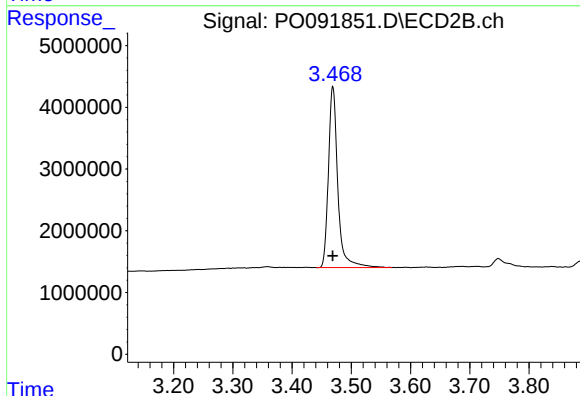


#1 Tetrachloro-m-xylene

R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 32249056
Conc: 23.36 ng/ml

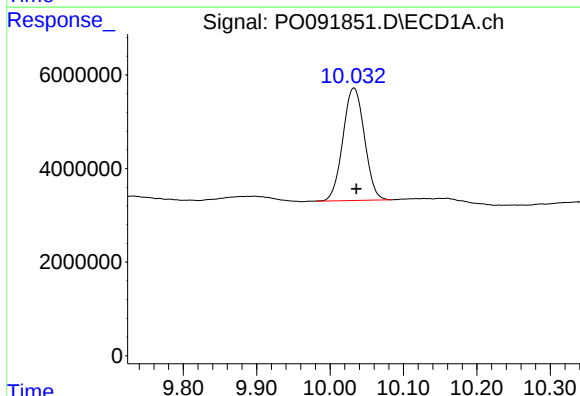

#2 Decachlorobiphenyl

R.T.: 10.033 min
Delta R.T.: -0.003 min
Response: 48988826
Conc: 20.64 ng/ml

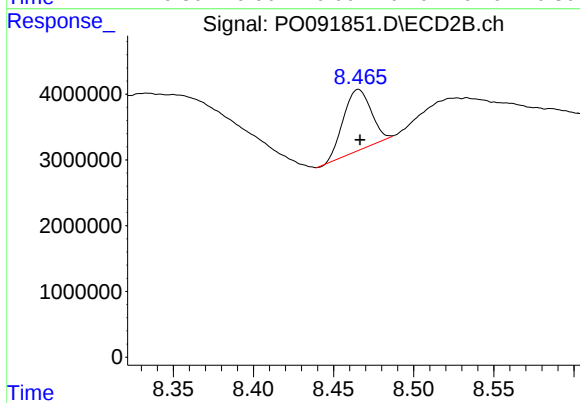

#2 Decachlorobiphenyl

R.T.: 8.465 min
Delta R.T.: -0.001 min
Response: 11289242
Conc: 8.97 ng/ml m