

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010523\
 Data File : P0091852.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2023 15:42
 Operator : YP/AJ
 Sample : 01029-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-205

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/06/2023
 Supervised By :Ankita Jodhani 01/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 20:42:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010423.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 05 01:51:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.292	3.469	94725022	33086752	29.476	23.967
2) SA Decachlor...	10.031	8.466	46085562	31864737	19.414	25.318m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010523\
Data File : PO091852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2023 15:42
Operator : YP/AJ
Sample : 01029-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-205


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/06/2023
Supervised By :Ankita Jodhani 01/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 20:42:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010423.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 05 01:51:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

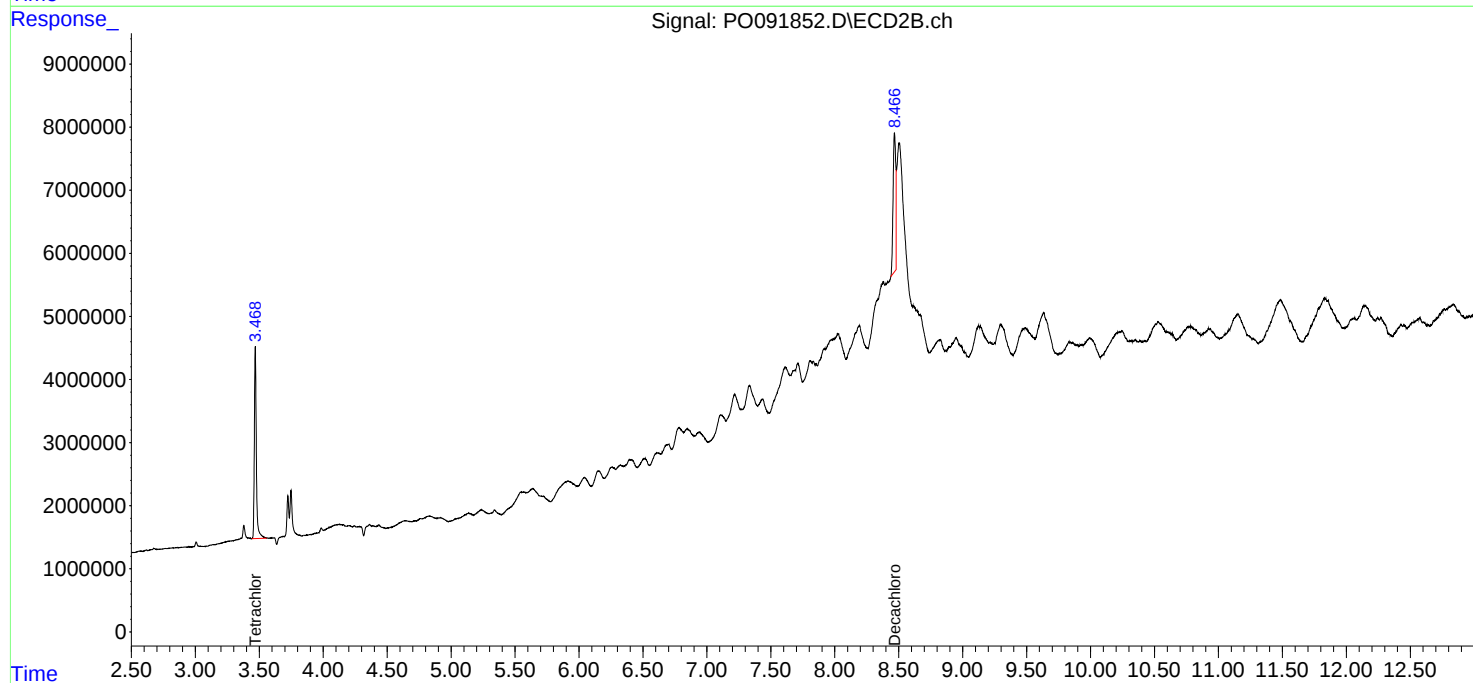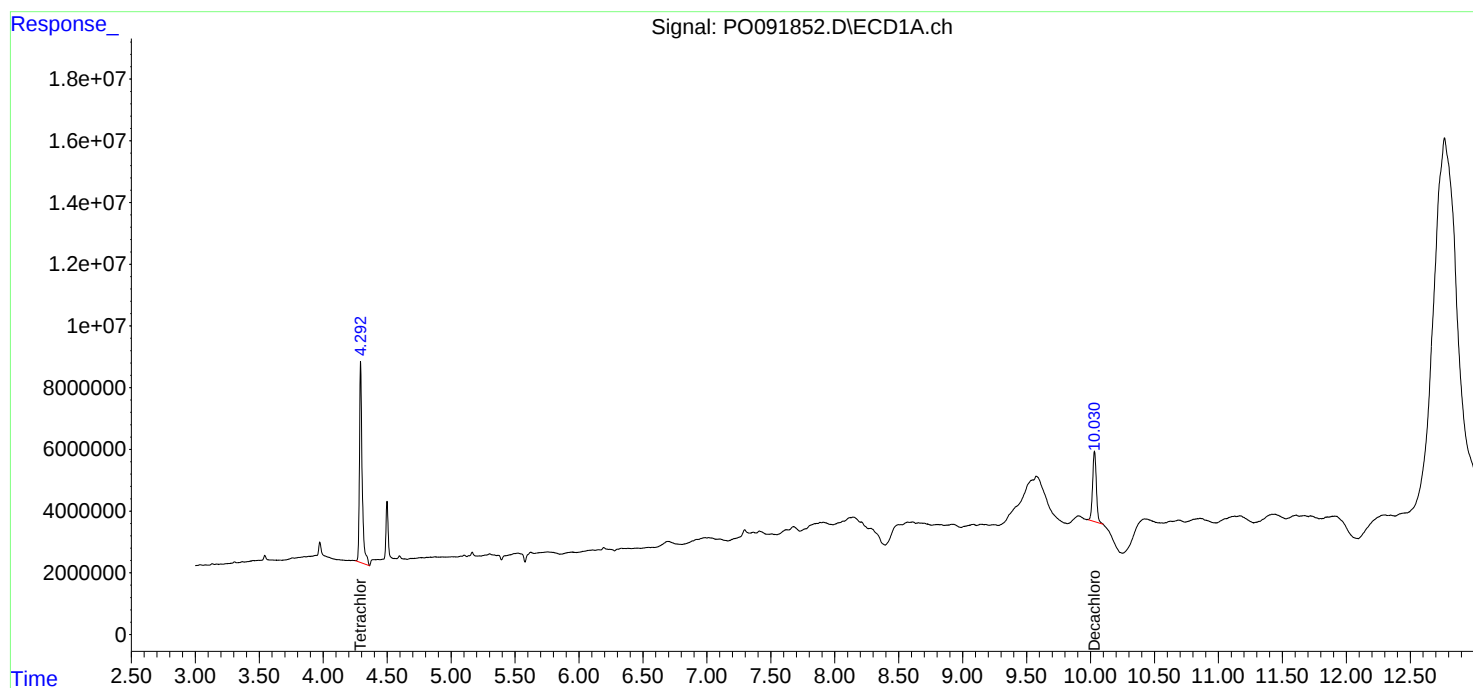

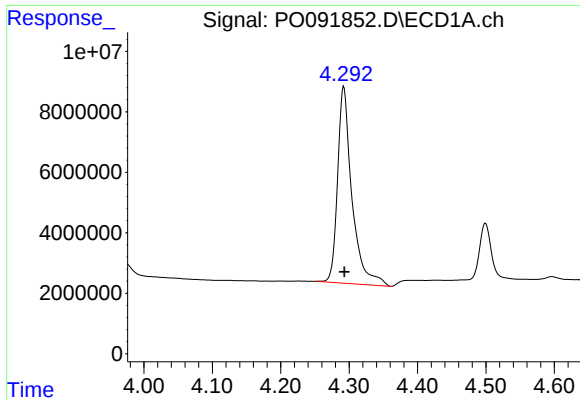


#1 Tetrachloro-m-xylene

R.T.: 4.292 min
Delta R.T.: 0.000 min
Response: 94725022
Conc: 29.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-205


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/06/2023
Supervised By :Ankita Jodhani 01/06/2023

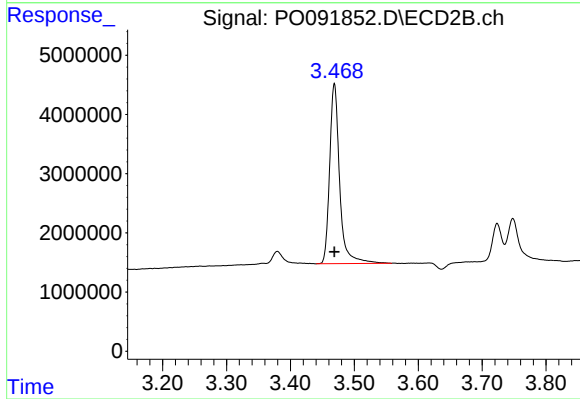


#1 Tetrachloro-m-xylene

R.T.: 3.469 min
Delta R.T.: 0.000 min
Response: 33086752
Conc: 23.97 ng/ml

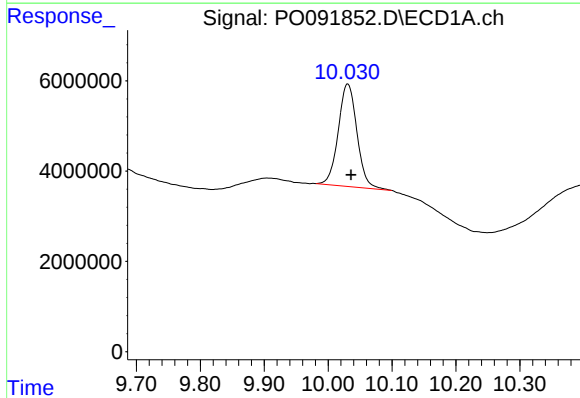

#2 Decachlorobiphenyl

R.T.: 10.031 min
Delta R.T.: -0.005 min
Response: 46085562
Conc: 19.41 ng/ml

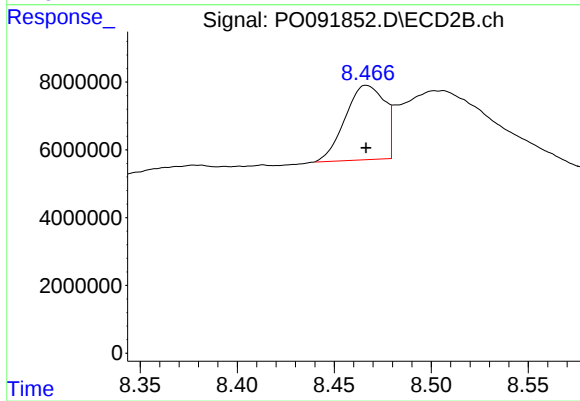

#2 Decachlorobiphenyl

R.T.: 8.466 min
Delta R.T.: 0.000 min
Response: 31864737
Conc: 25.32 ng/ml m