

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010524\
 Data File : P0100925.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2024 13:01
 Operator : YP/AJ
 Sample : PB158259BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB158259BL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/08/2024
 Supervised By :Ankita Jodhani 01/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 23:26:34 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.346	3.640	75564789	47299206	24.217	23.147m
2) SA Decachlor...	10.087	8.700	48147514	35463357	23.047	23.496

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010524\
Data File : PO100925.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2024 13:01
Operator : YP/AJ
Sample : PB158259BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB158259BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2024
Supervised By :Ankita Jodhani 01/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 23:26:34 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

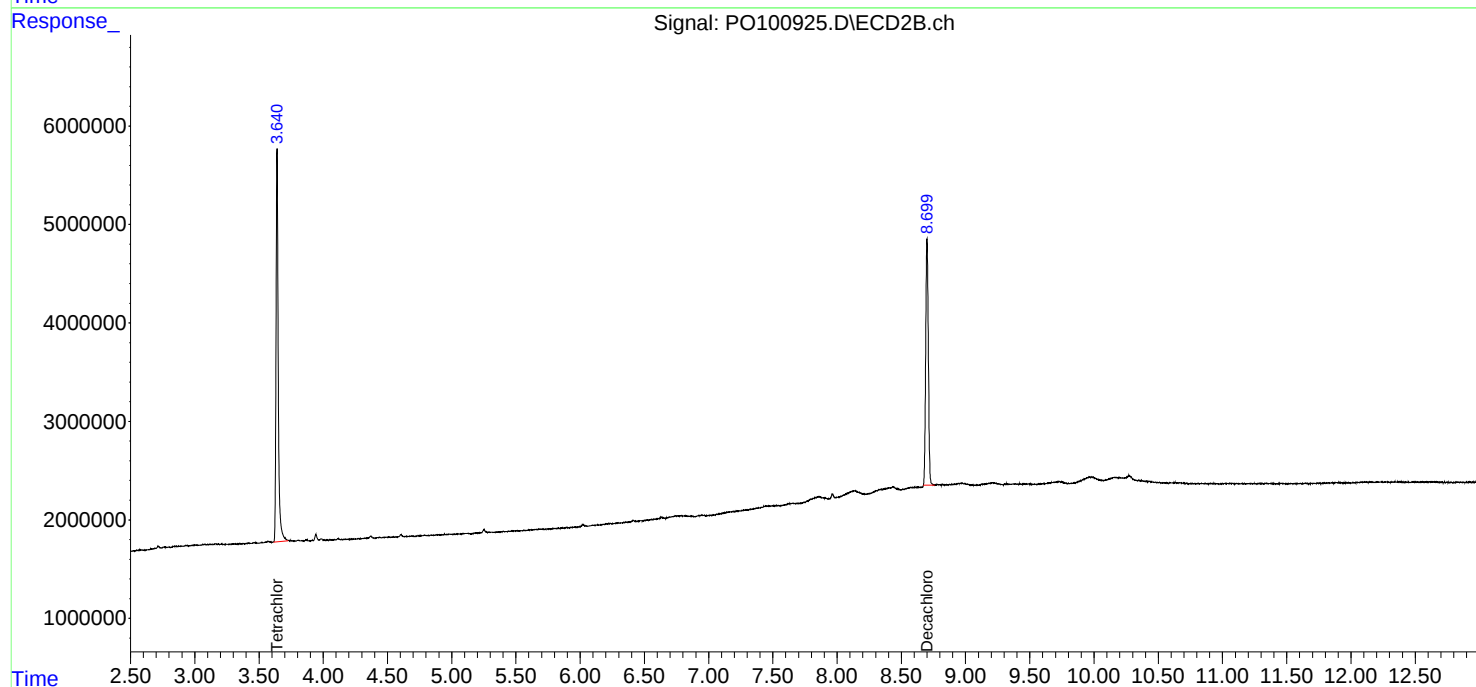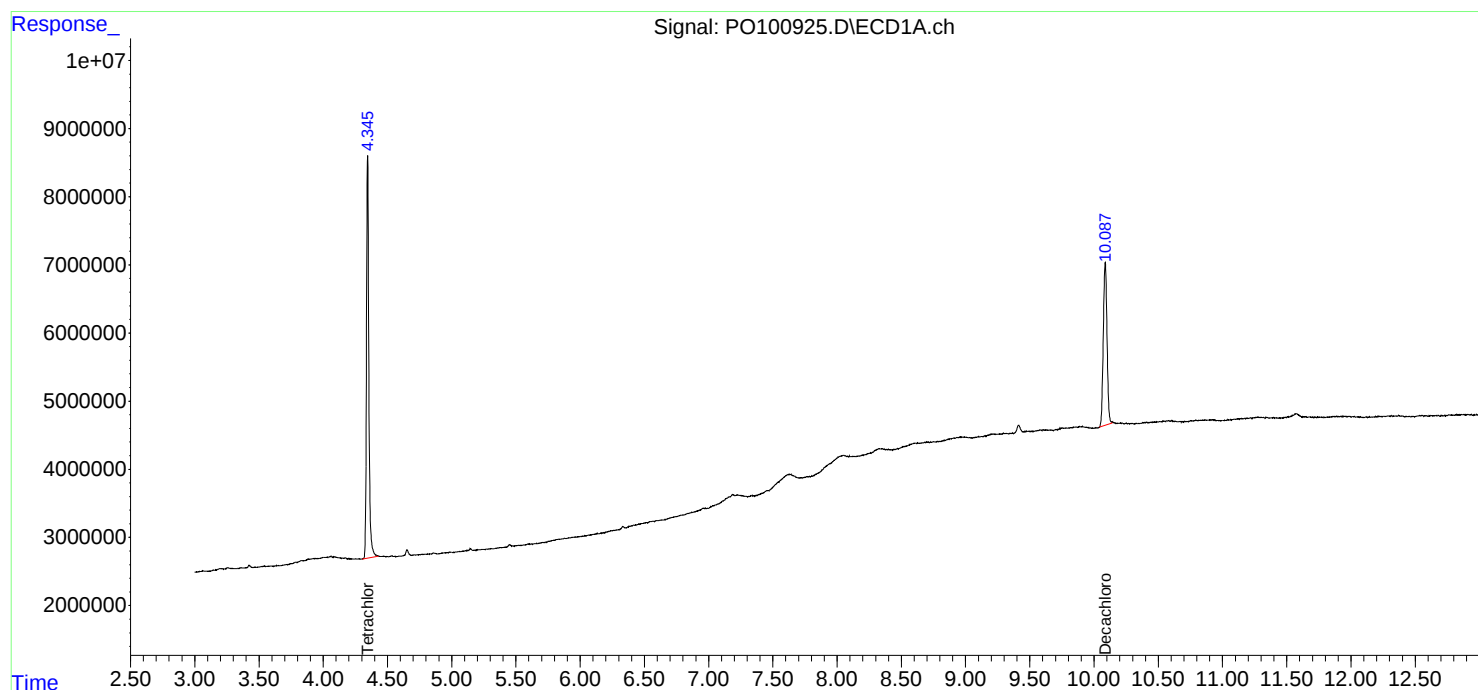

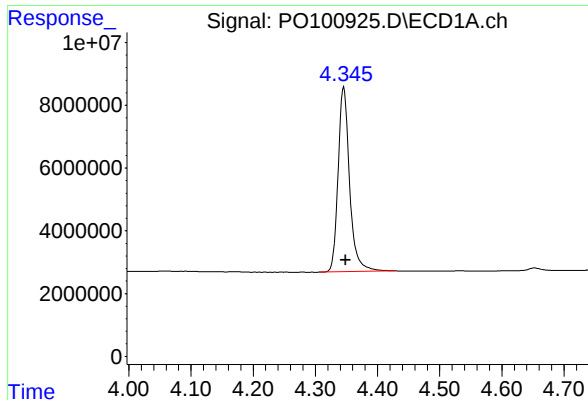


#1 Tetrachloro-m-xylene

R.T.: 4.346 min
Delta R.T.: -0.003 min
Response: 75564789
Conc: 24.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB158259BL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2024
Supervised By :Ankita Jodhani 01/08/2024

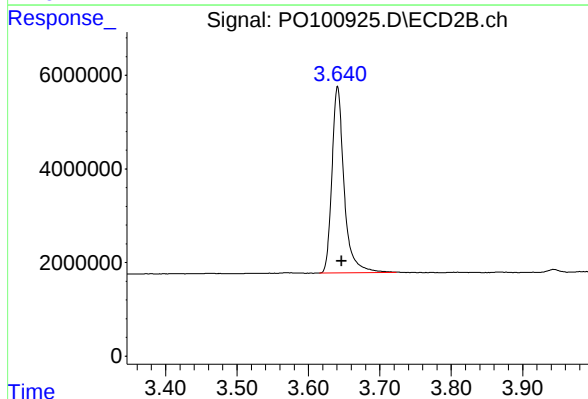


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: -0.006 min
Response: 47299206
Conc: 23.15 ng/ml

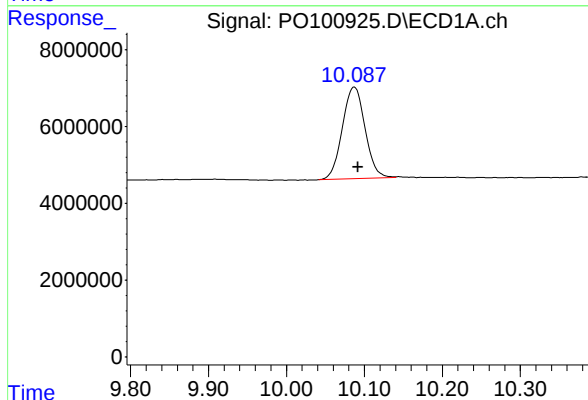

#2 Decachlorobiphenyl

R.T.: 10.087 min
Delta R.T.: -0.005 min
Response: 48147514
Conc: 23.05 ng/ml

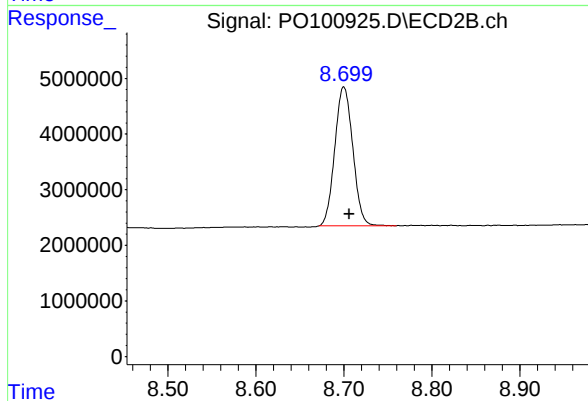

#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.006 min
Response: 35463357
Conc: 23.50 ng/ml