

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010524\
 Data File : P0100933.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2024 15:14
 Operator : YP/AJ
 Sample : P1031-03 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC270896-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/08/2024
 Supervised By :Ankita Jodhani 01/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 23:30:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.345	3.642	4331823	3073141	1.388m	1.504m
2) SA Decachlor...	10.085	8.700	3116801	2681146	1.492m	1.776

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010524\
Data File : PO100933.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2024 15:14
Operator : YP/AJ
Sample : P1031-03 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC270896-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2024
Supervised By :Ankita Jodhani 01/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 23:30:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

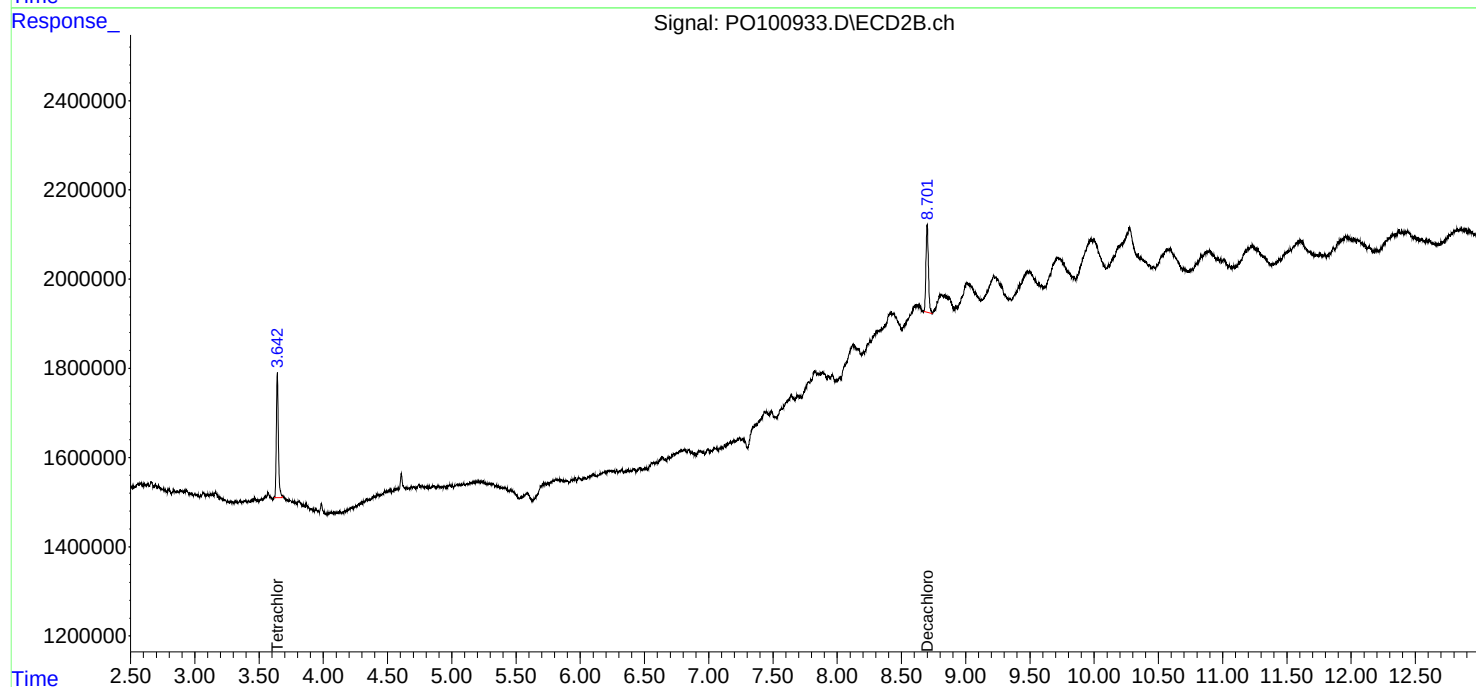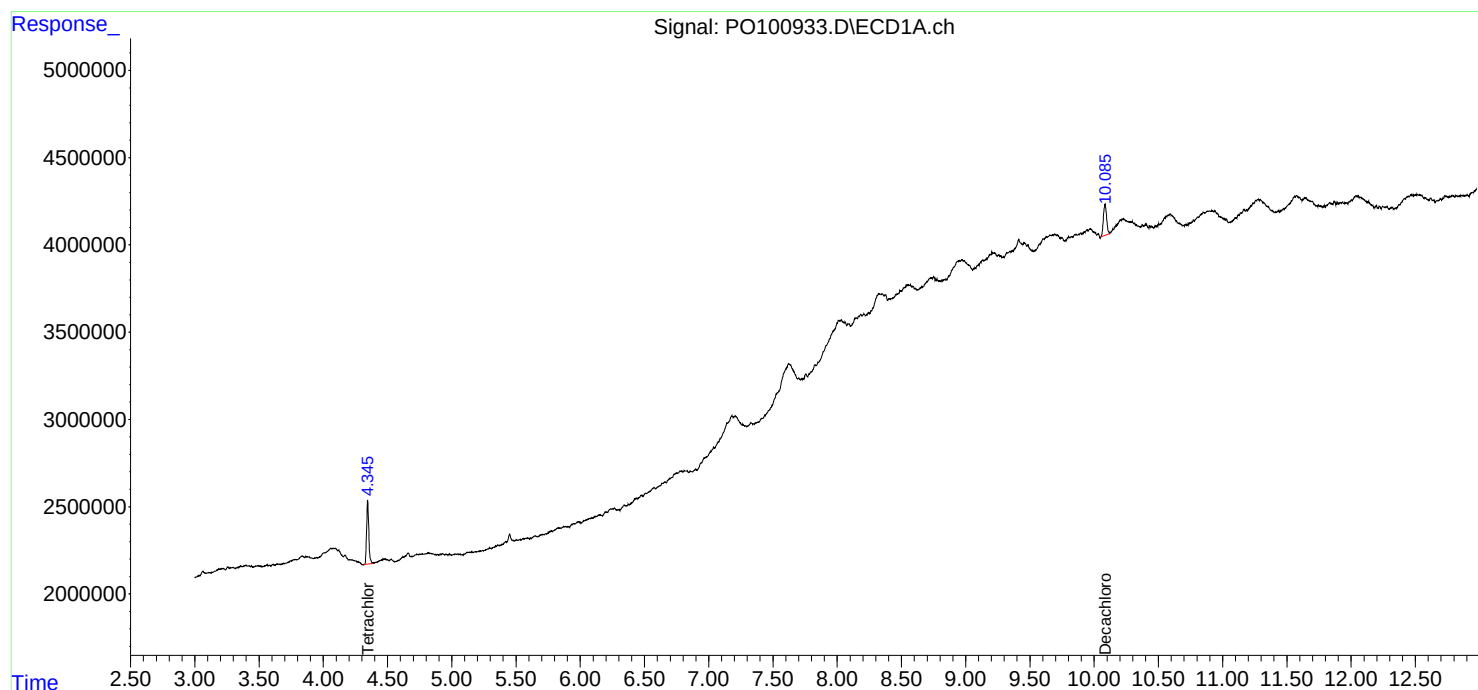

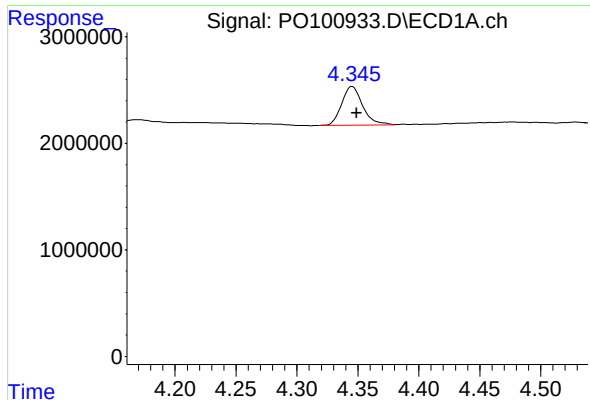


#1 Tetrachloro-m-xylene

R.T.: 4.345 min
Delta R.T.: -0.004 min
Response: 4331823
Conc: 1.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC270896-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2024
Supervised By :Ankita Jodhani 01/08/2024

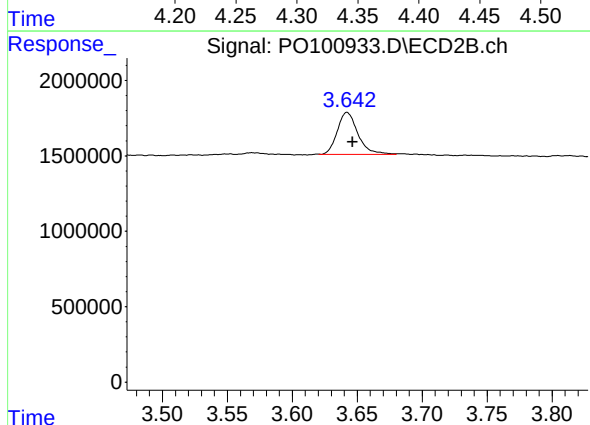


#1 Tetrachloro-m-xylene

R.T.: 3.642 min
Delta R.T.: -0.005 min
Response: 3073141
Conc: 1.50 ng/ml

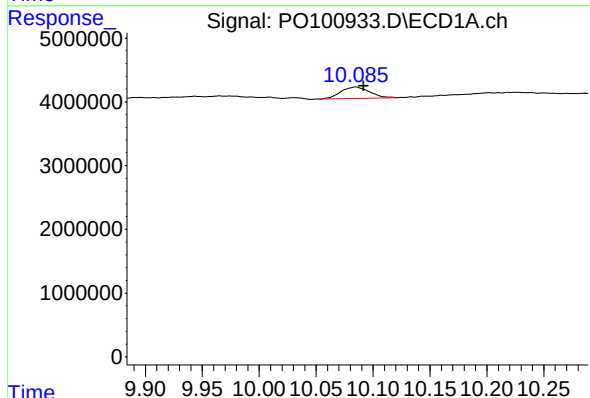

#2 Decachlorobiphenyl

R.T.: 10.085 min
Delta R.T.: -0.007 min
Response: 3116801
Conc: 1.49 ng/ml

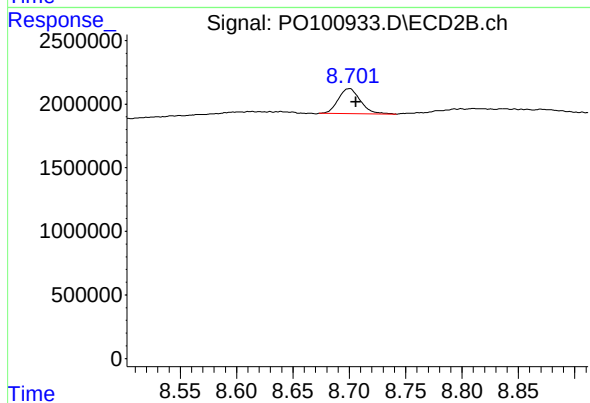

#2 Decachlorobiphenyl

R.T.: 8.700 min
Delta R.T.: -0.006 min
Response: 2681146
Conc: 1.78 ng/ml