

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010524\
 Data File : P0100947.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Jan 2024 19:42
 Operator : YP/AJ
 Sample : P1033-04 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 W029022-B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/08/2024
 Supervised By :Ankita Jodhani 01/08/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 05 23:34:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.641	3813200	3190665	1.222m	1.561m#
2) SA Decachlor...	10.085	8.699	3256529	2518699	1.559	1.669

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010524\
Data File : PO100947.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Jan 2024 19:42
Operator : YP/AJ
Sample : P1033-04 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
W029022-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2024
Supervised By :Ankita Jodhani 01/08/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 05 23:34:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

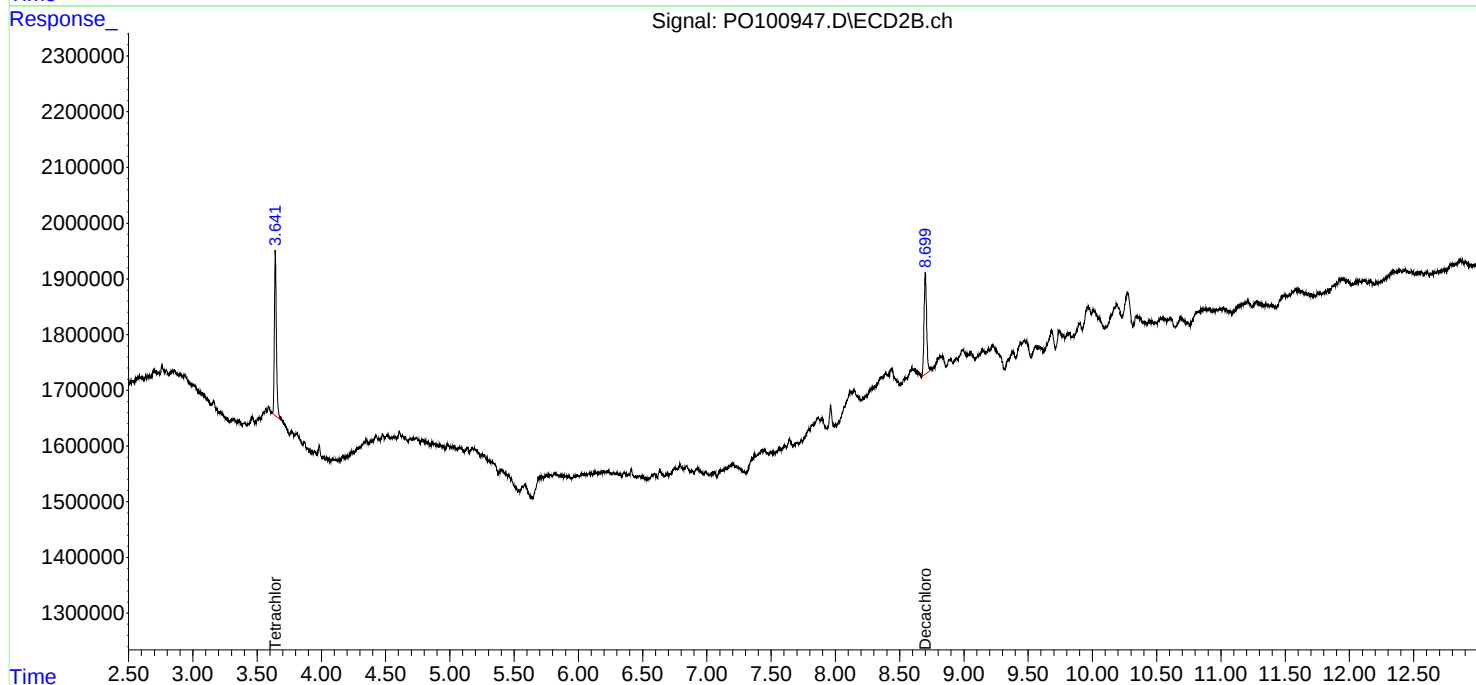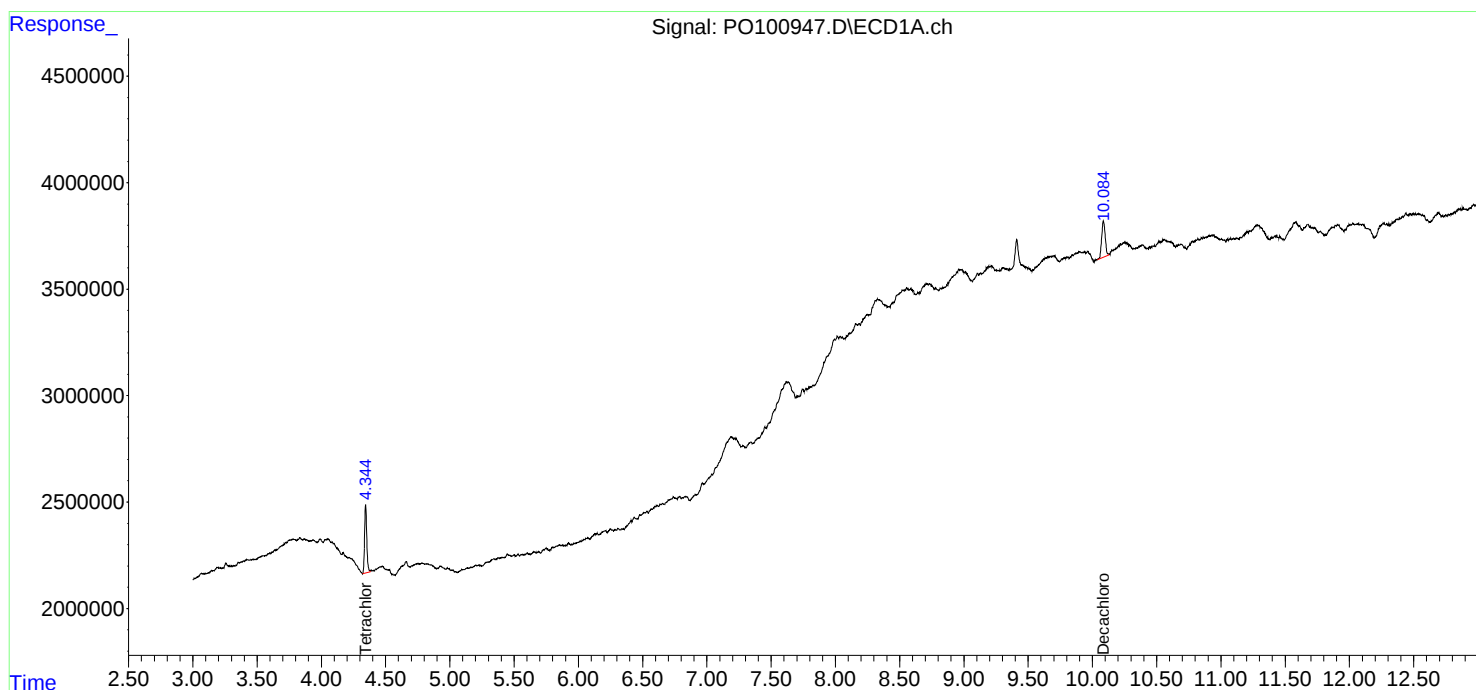

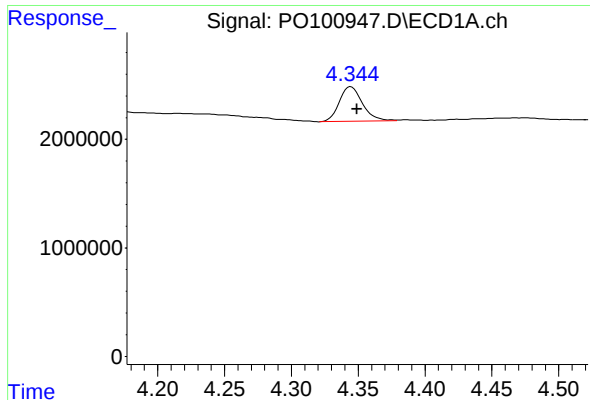


#1 Tetrachloro-m-xylene

R.T.: 4.344 min
Delta R.T.: -0.005 min
Response: 3813200
Conc: 1.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
W029022-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2024
Supervised By :Ankita Jodhani 01/08/2024

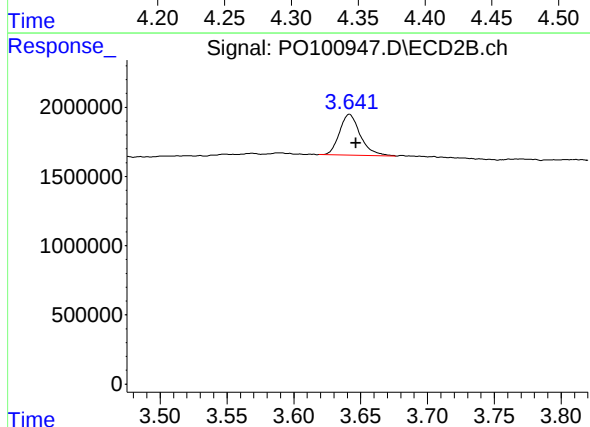


#1 Tetrachloro-m-xylene

R.T.: 3.641 min
Delta R.T.: -0.005 min
Response: 3190665
Conc: 1.56 ng/ml

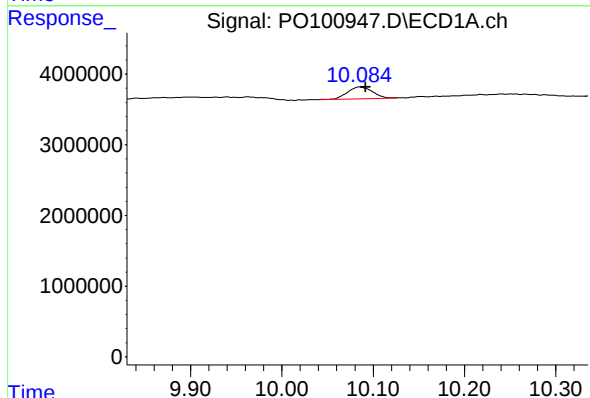

#2 Decachlorobiphenyl

R.T.: 10.085 min
Delta R.T.: -0.006 min
Response: 3256529
Conc: 1.56 ng/ml

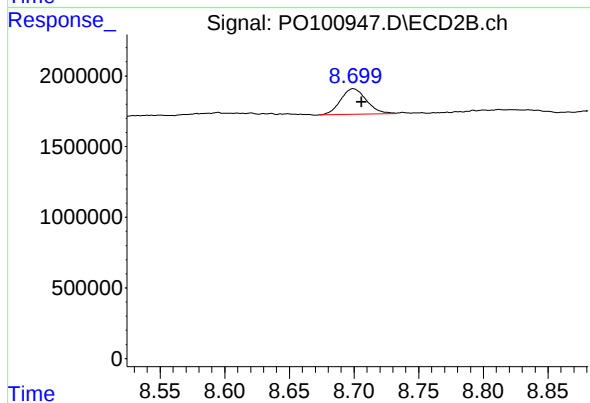

#2 Decachlorobiphenyl

R.T.: 8.699 min
Delta R.T.: -0.007 min
Response: 2518699
Conc: 1.67 ng/ml