

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010620\
 Data File : P0065315.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jan 2020 11:18
 Operator : AJ/MA
 Sample : L1008-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-010220

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 11:32:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.167	3.441	488886	576911	26.773	26.226
2) SA Decachlor...	9.677	8.350	497532	536171	14.684	12.929

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010620\
Data File : PO065315.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jan 2020 11:18
Operator : AJ/MA
Sample : L1008-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-02-010220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 11:32:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

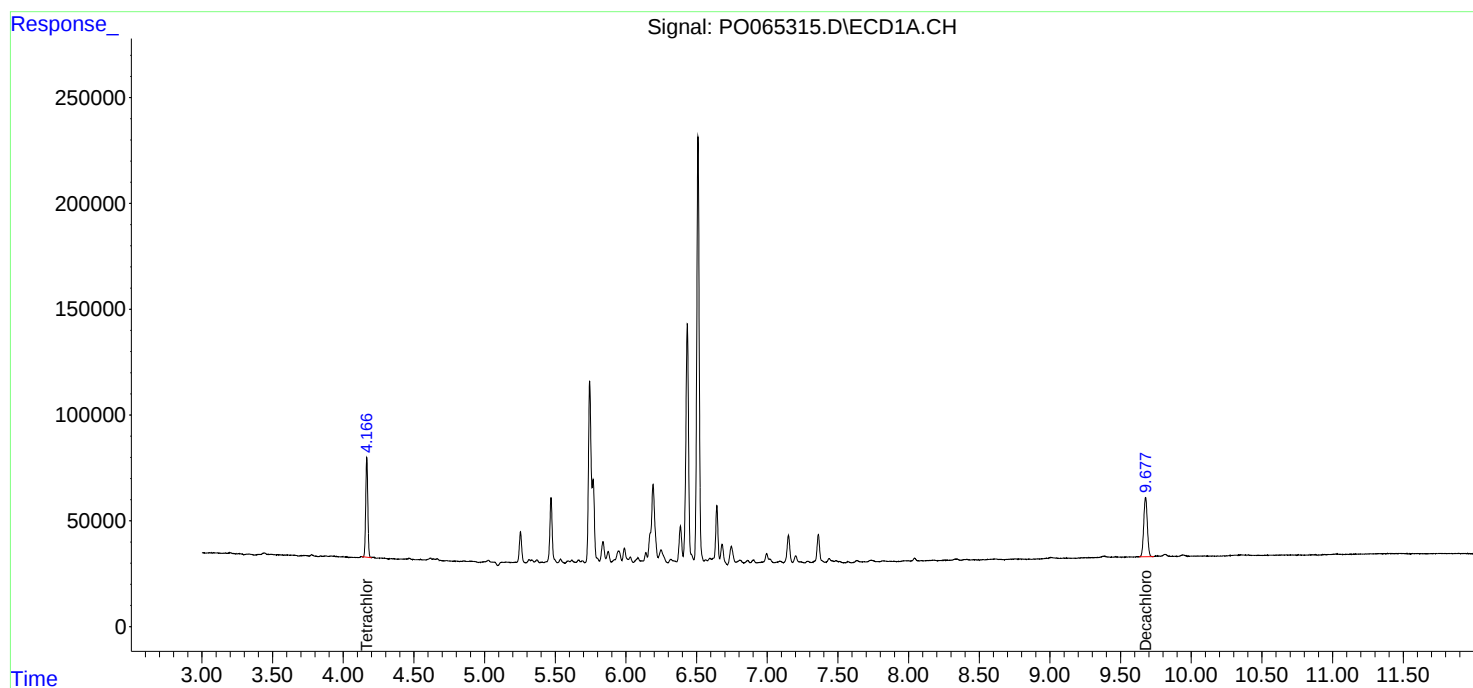


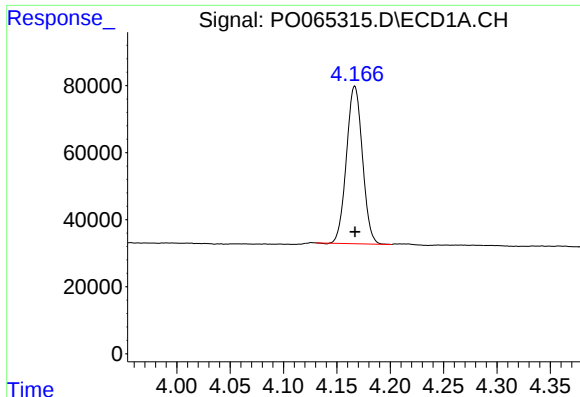

#1 Tetrachloro-m-xylene


R.T.: 4.167 min
Delta R.T.: 0.000 min
Response: 488886
Conc: 26.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-010220

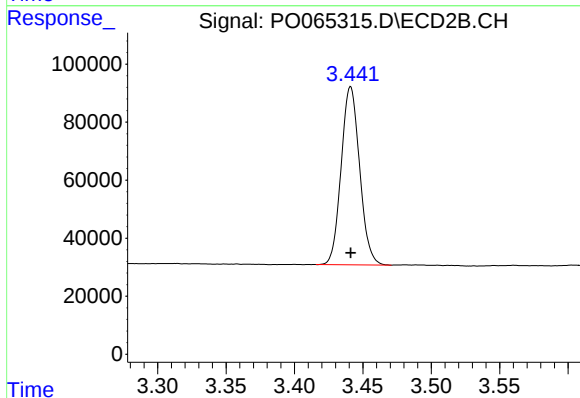


#1 Tetrachloro-m-xylene

R.T.: 3.441 min
Delta R.T.: 0.000 min
Response: 576911
Conc: 26.23 ng/ml

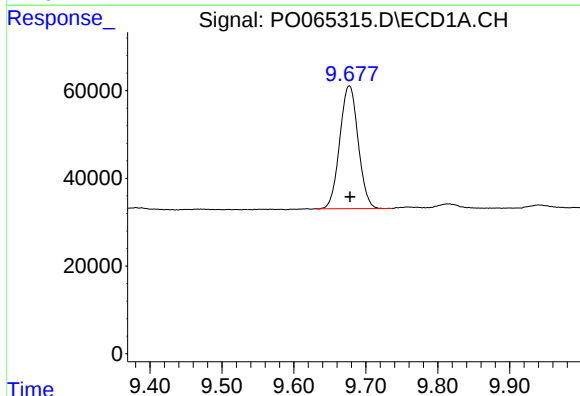

#2 Decachlorobiphenyl

R.T.: 9.677 min
Delta R.T.: -0.001 min
Response: 497532
Conc: 14.68 ng/ml

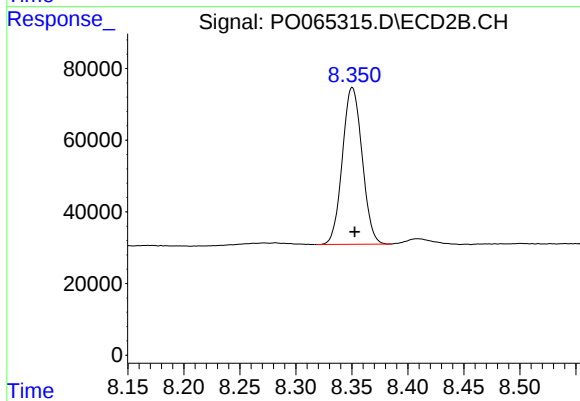

#2 Decachlorobiphenyl

R.T.: 8.350 min
Delta R.T.: -0.002 min
Response: 536171
Conc: 12.93 ng/ml