

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010621\
 Data File : P0074409.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jan 2021 14:00
 Operator : DD\AJ
 Sample : M1012-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KKA091Y-END-2

Manual Integrations
 APPROVED

Ankita
 1/7/2021 11:14:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 16:01:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 05:03:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	3.990	1778111	1038070	18.505m	19.488
2) SA Decachlor...	10.966	9.263	1585128	780389	17.051	14.991

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010621\
Data File : P0074409.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jan 2021 14:00
Operator : DD\AJ
Sample : M1012-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KKA091Y-END-2


Manual Integrations
APPROVED

Ankita
1/7/2021 11:14:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 16:01:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

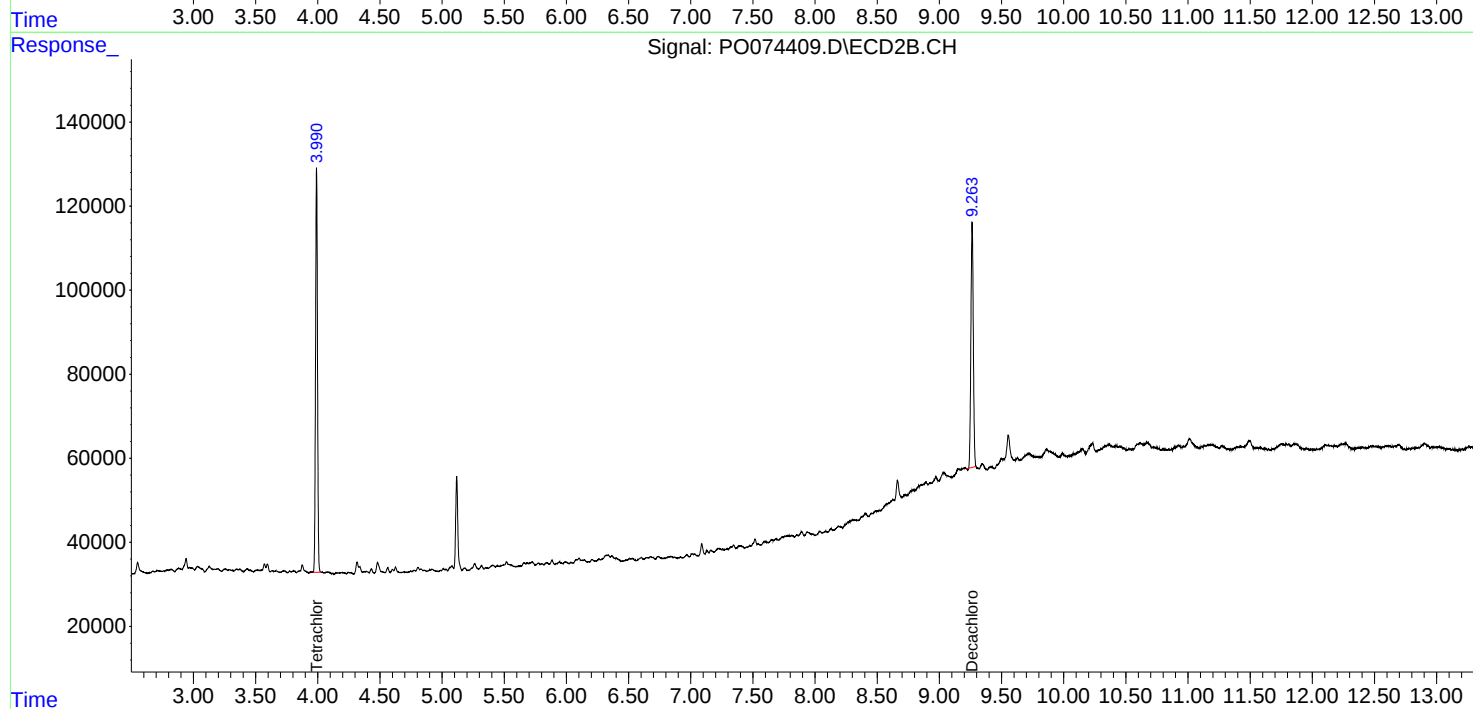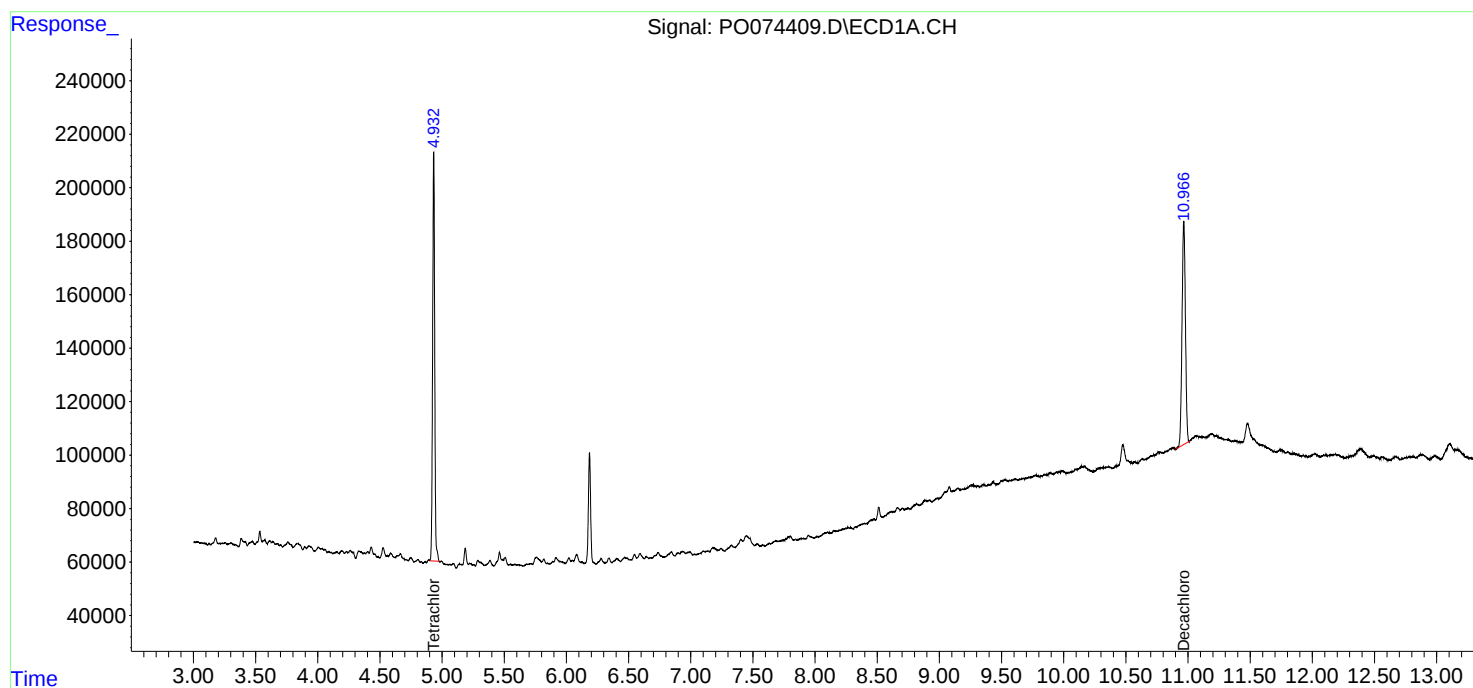

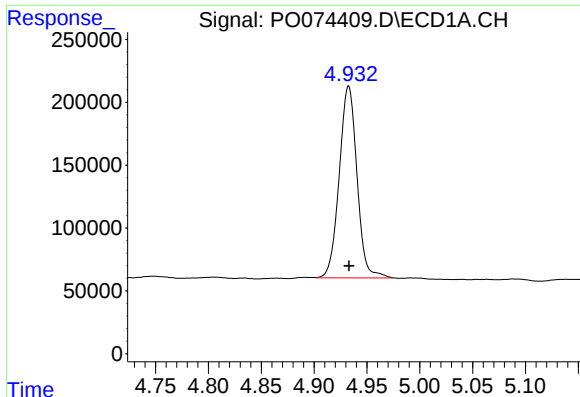


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 1778111
Conc: 18.51 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KKA091Y-END-2


Manual Integrations
APPROVED

Ankita
1/7/2021 11:14:21 AM

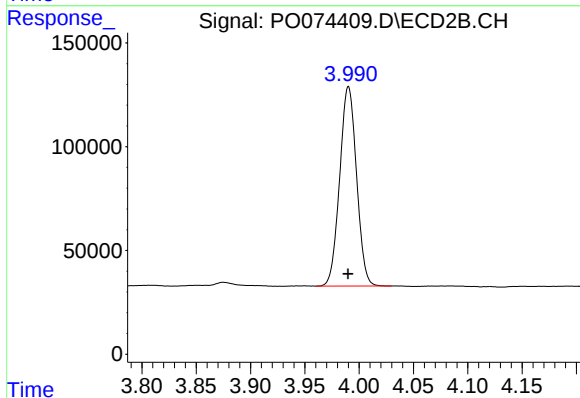


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: 0.000 min
Response: 1038070
Conc: 19.49 ng/ml

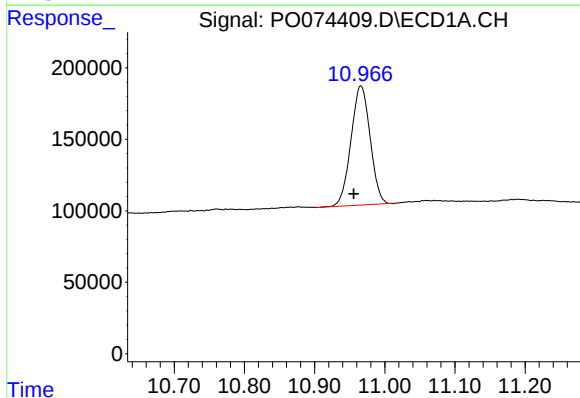

#2 Decachlorobiphenyl

R.T.: 10.966 min
Delta R.T.: 0.010 min
Response: 1585128
Conc: 17.05 ng/ml

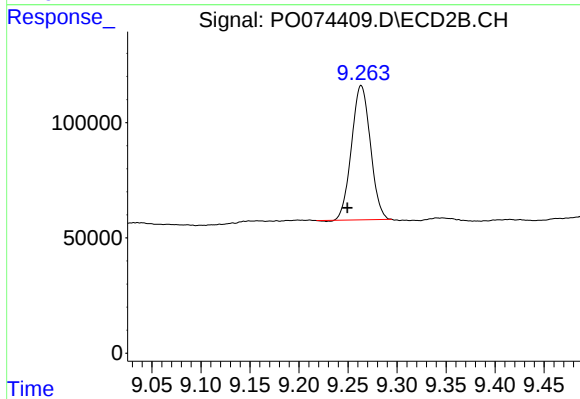

#2 Decachlorobiphenyl

R.T.: 9.263 min
Delta R.T.: 0.014 min
Response: 780389
Conc: 14.99 ng/ml