

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010719\
 Data File : P0053250.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2019 11:04
 Operator : SM/SJ
 Sample : K1034-05RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CONTROL-HOUSE-WALL-1-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 00:31:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.182	3.211	27683728	4554315	21.158	20.296
2)	SA Decachlor...	9.644	7.856	16554873	5067967	20.894	19.715
Target Compounds							
3)	L1 AR-1016-1	5.258	0.000	442374	0	11.540	N.D. #
7)	L1 AR-1016-5	0.000	4.655	0	4648151	N.D.	636.538 #
9)	L2 AR-1221-2	4.482	0.000	321517	0	37.225	N.D. #
10)	L2 AR-1221-3	4.482	3.605	321517	243024	11.501	42.696 #
11)	L3 AR-1232-1	4.482	3.605	321517	243024	14.140	51.672 #
12)	L3 AR-1232-2	5.135	0.000	591580	0	52.207	N.D. #
15)	L3 AR-1232-5	0.000	4.655	0	4648151	N.D.	1631.192 #
20)	L4 AR-1242-5	6.245	4.956	1053581	1484036	48.151	194.788 #
24)	L5 AR-1248-4	6.170	4.655	10051621	4648151	269.061	492.497 #
25)	L5 AR-1248-5	6.245	4.956	1053581	1484036	29.571	147.924 #
26)	L6 AR-1254-1	6.170	4.956	10051621	1484036	262.276	90.522 #
28)	L6 AR-1254-3	6.768	0.000	1675566	0	27.169	N.D. #
29)	L6 AR-1254-4	6.983	5.657	1474422	175976	32.087	11.609 #
30)	L6 AR-1254-5	7.436	0.000	352525	0	7.767	N.D. #
31)	L7 AR-1260-1	0.000	5.571	0	662806	N.D.	43.180 #
32)	L7 AR-1260-2	0.000	5.743	0	618952	N.D.	32.342 #
34)	L7 AR-1260-4	7.761	0.000	800539	0	20.591	N.D. #
35)	L7 AR-1260-5	0.000	6.539	0	375321	N.D.	13.028 #
37)	L8 AR-1262-2	0.000	6.539	0	375321	N.D.	11.302 #
38)	L8 AR-1262-3	0.000	6.920	0	359646	N.D.	27.774 #
39)	L8 AR-1262-4	0.000	6.920	0	359646	N.D.	14.813 #
41)	L9 AR-1268-1	0.000	6.920	0	359646	N.D.	8.278 #
42)	L9 AR-1268-2	0.000	6.920	0	359646	N.D.	8.745 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010719\
Data File : PO053250.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2019 11:04
Operator : SM/SJ
Sample : K1034-05RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 00:31:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

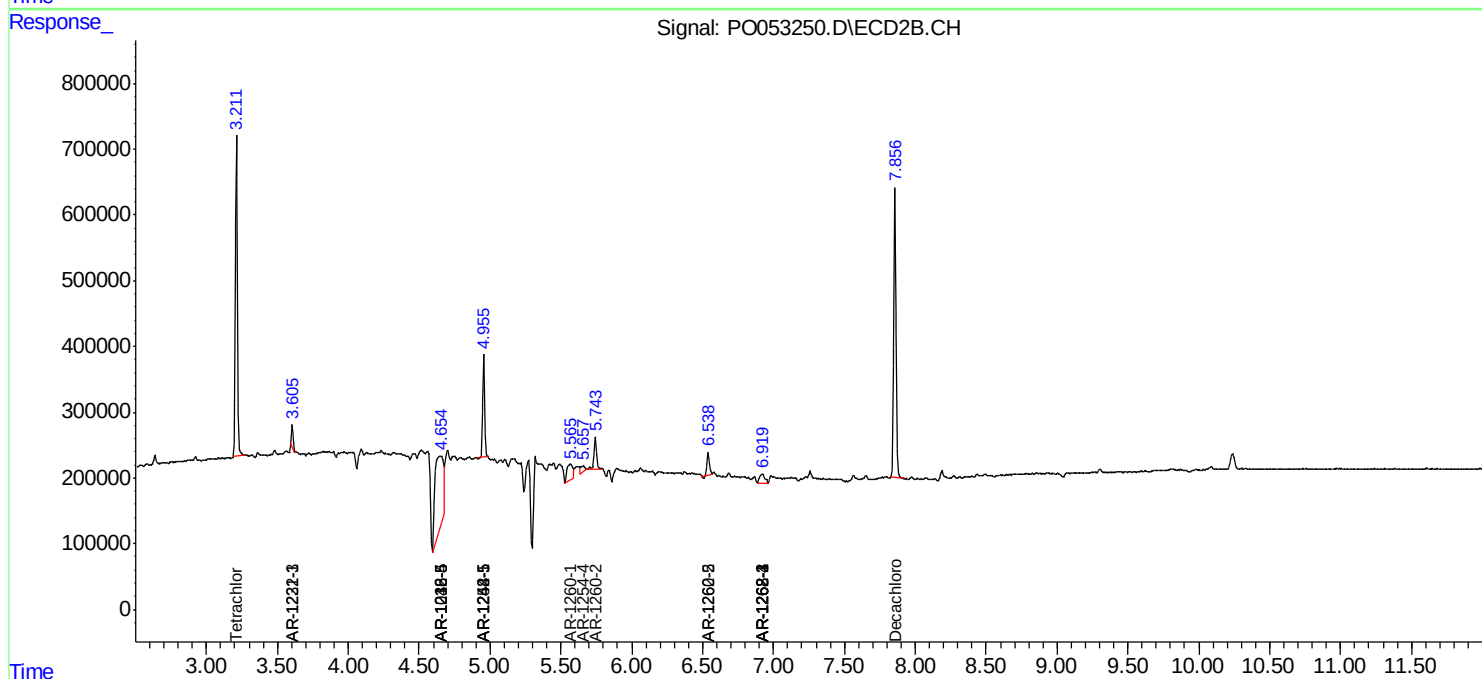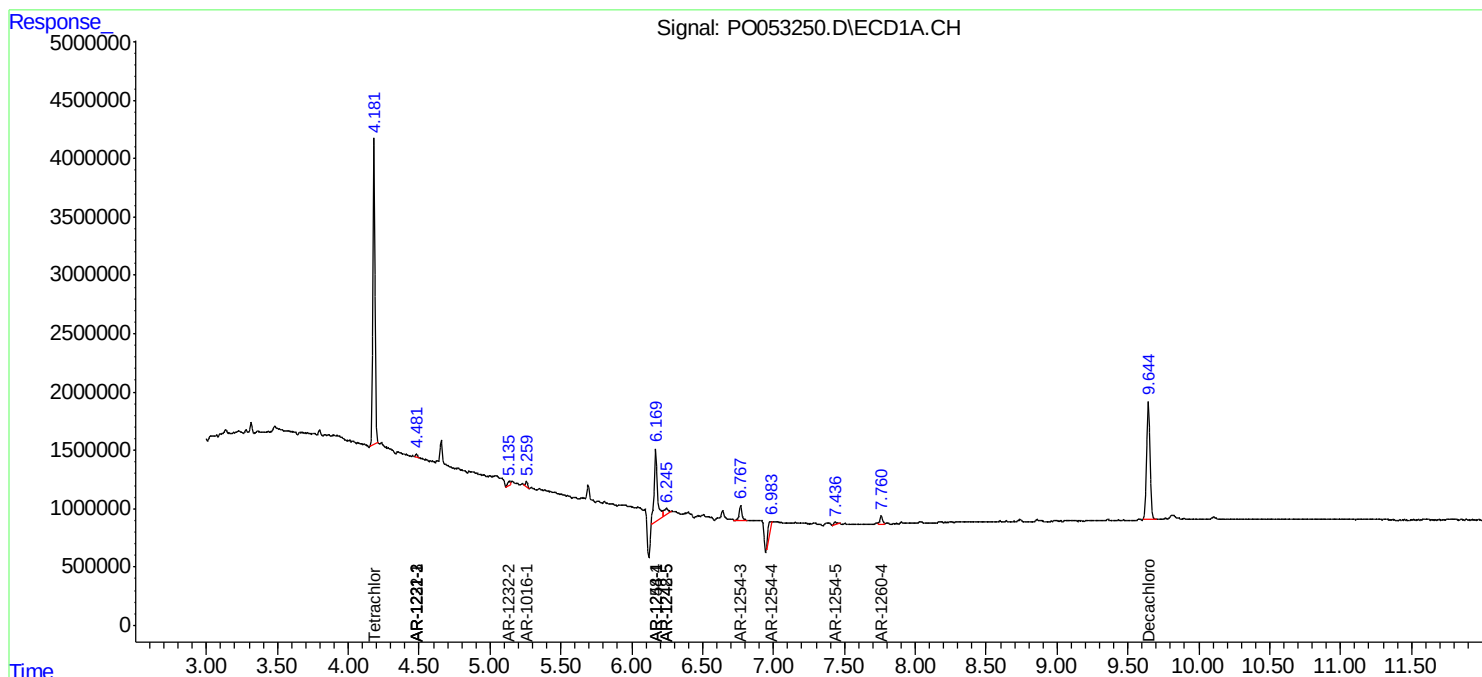


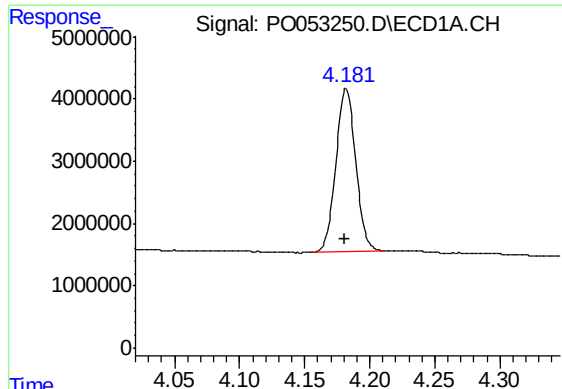

#1 Tetrachloro-m-xylene


R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 27683728
Conc: 21.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

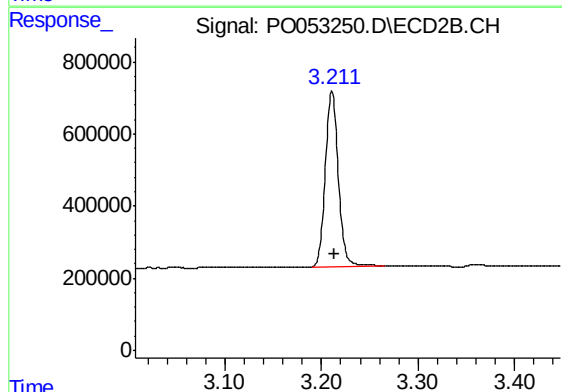


#1 Tetrachloro-m-xylene

R.T.: 3.211 min
Delta R.T.: -0.003 min
Response: 4554315
Conc: 20.30 ng/ml

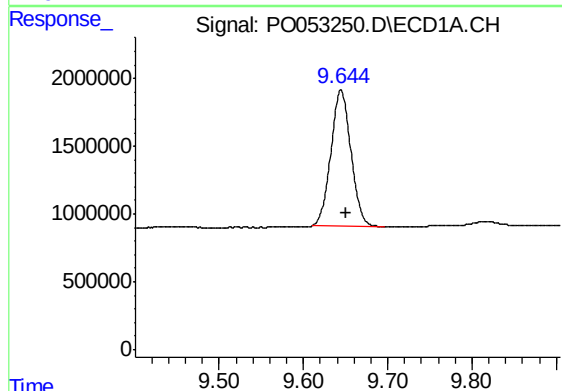


#2 Decachlorobiphenyl

R.T.: 9.644 min
Delta R.T.: -0.006 min
Response: 16554873
Conc: 20.89 ng/ml

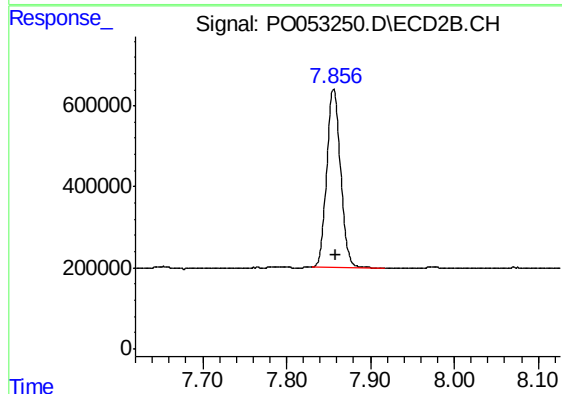

#2 Decachlorobiphenyl


R.T.: 7.856 min
Delta R.T.: -0.003 min
Response: 5067967
Conc: 19.72 ng/ml

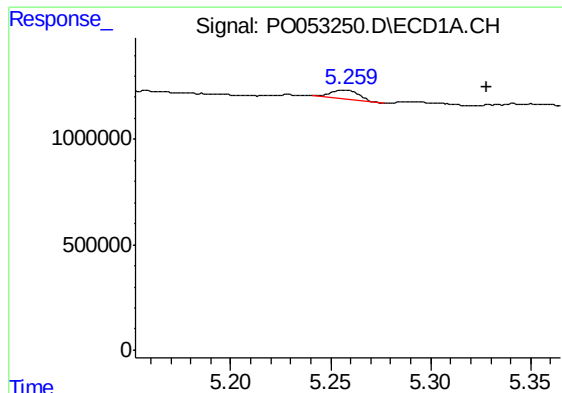

#3 AR-1016-1


R.T.: 5.258 min
Delta R.T.: -0.069 min
Response: 442374
Conc: 11.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

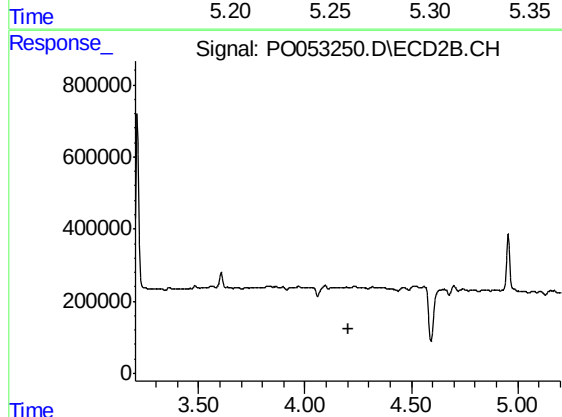


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.202 min
Response: 0
Conc: N.D.

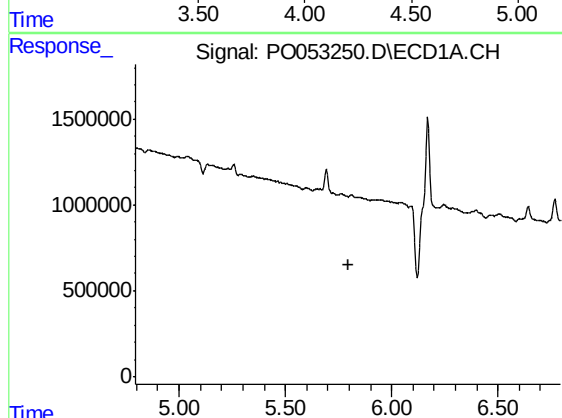


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.795 min
Response: 0
Conc: N.D.

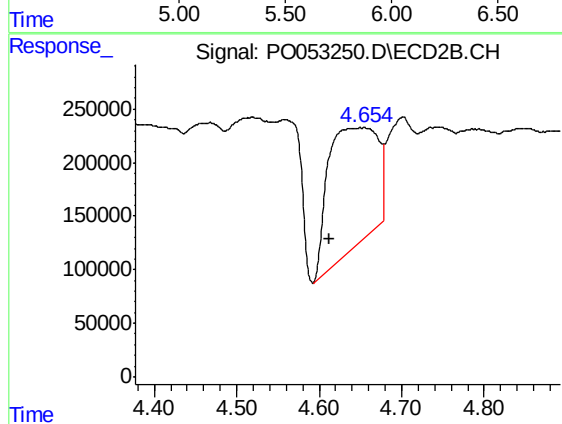

#7 AR-1016-5


R.T.: 4.655 min
Delta R.T.: 0.042 min
Response: 4648151
Conc: 636.54 ng/ml

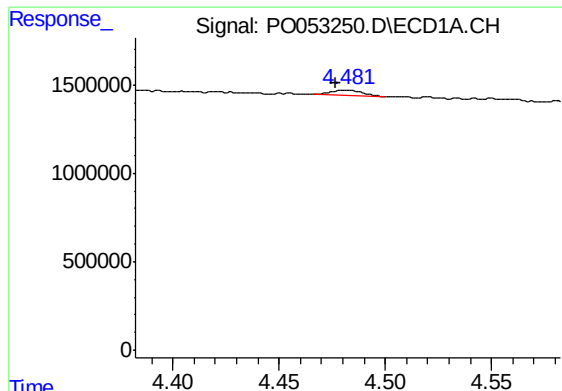

#9 AR-1221-2


R.T.: 4.482 min
Delta R.T.: 0.005 min
Response: 321517
Conc: 37.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

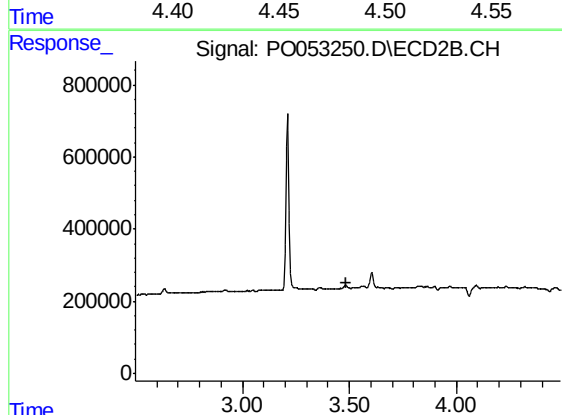


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.487 min
Response: 0
Conc: N.D.

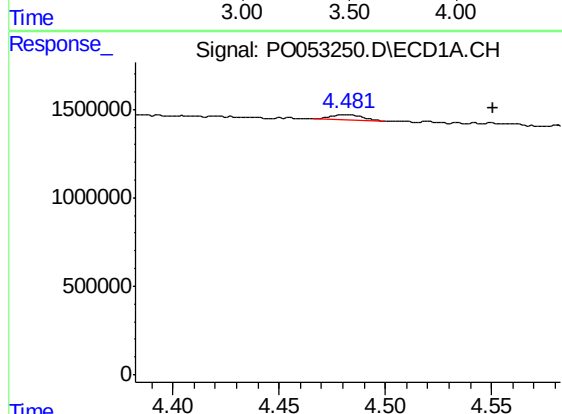


#10 AR-1221-3

R.T.: 4.482 min
Delta R.T.: -0.069 min
Response: 321517
Conc: 11.50 ng/ml

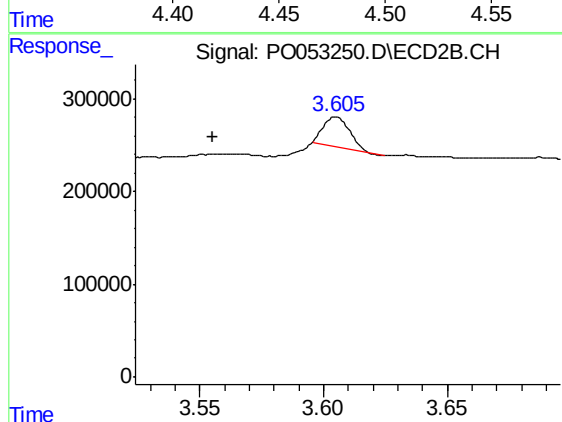

#10 AR-1221-3


R.T.: 3.605 min
Delta R.T.: 0.050 min
Response: 243024
Conc: 42.70 ng/ml

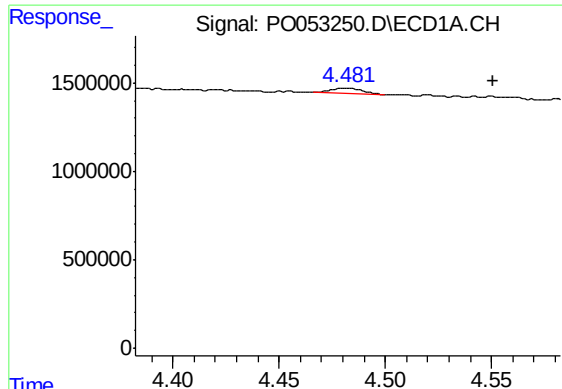

#11 AR-1232-1


R.T.: 4.482 min
Delta R.T.: -0.069 min
Response: 321517
Conc: 14.14 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

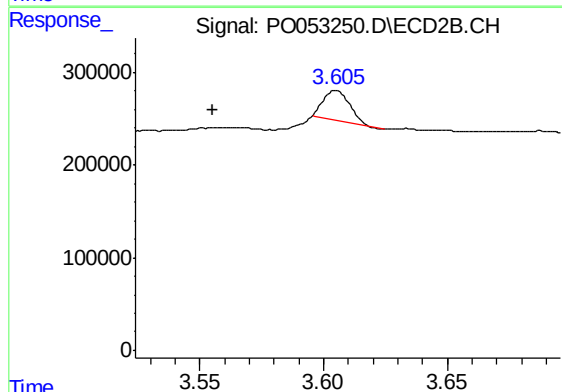


#11 AR-1232-1

R.T.: 3.605 min
Delta R.T.: 0.050 min
Response: 243024
Conc: 51.67 ng/ml

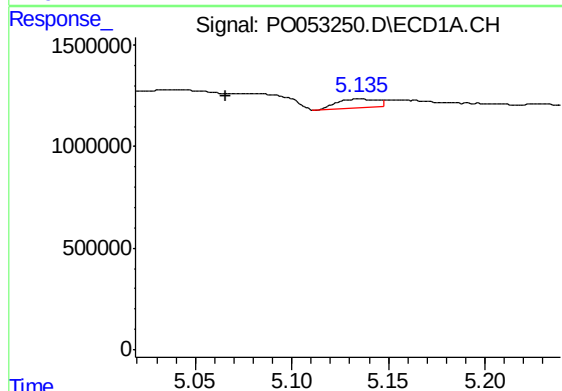


#12 AR-1232-2

R.T.: 5.135 min
Delta R.T.: 0.069 min
Response: 591580
Conc: 52.21 ng/ml

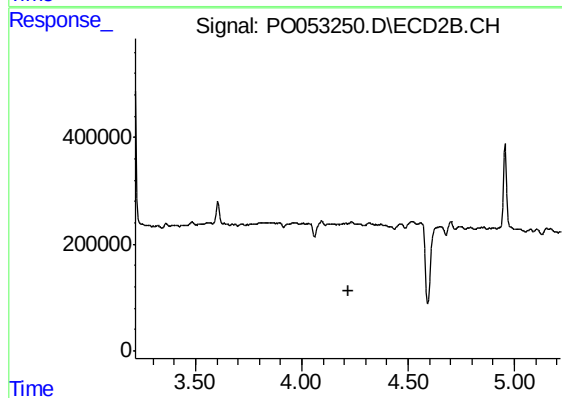

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.217 min
Response: 0
Conc: N.D.

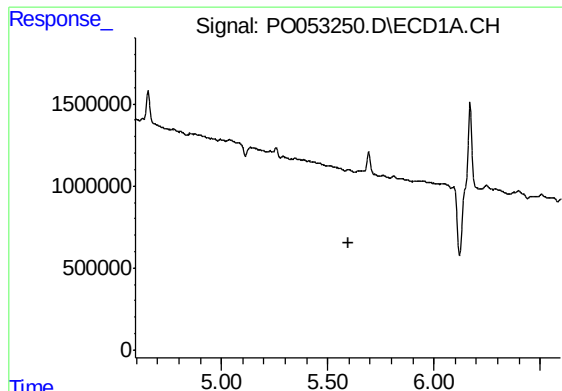

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 5.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

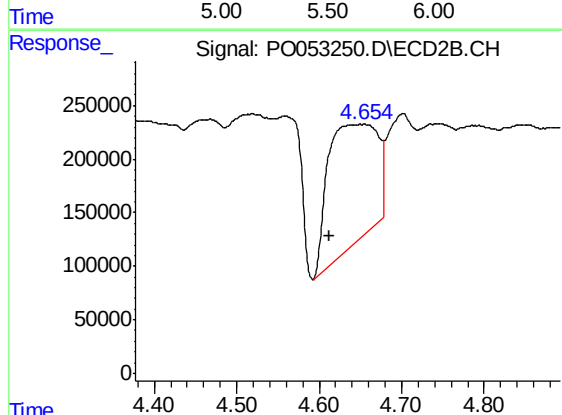


#15 AR-1232-5

R.T.: 4.655 min
Delta R.T.: 0.042 min
Response: 4648151
Conc: 1631.19 ng/ml

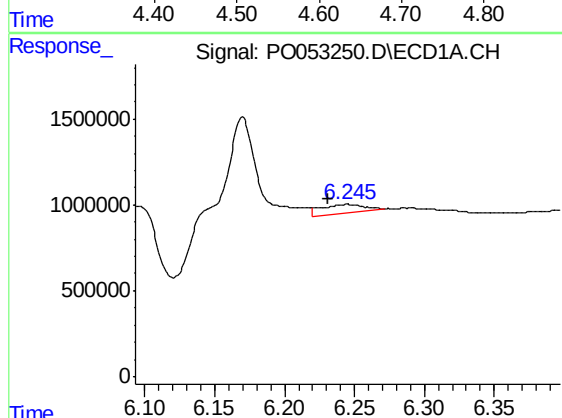


#20 AR-1242-5

R.T.: 6.245 min
Delta R.T.: 0.014 min
Response: 1053581
Conc: 48.15 ng/ml

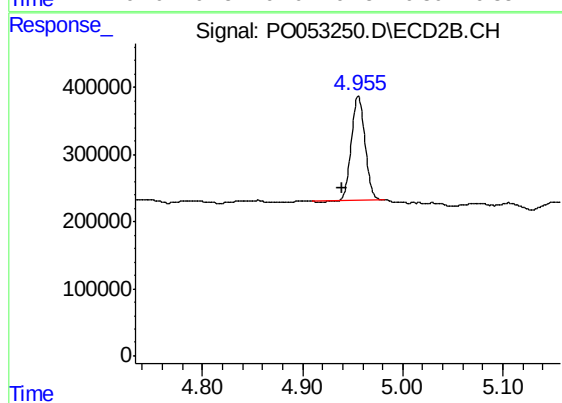

#20 AR-1242-5


R.T.: 4.956 min
Delta R.T.: 0.016 min
Response: 1484036
Conc: 194.79 ng/ml

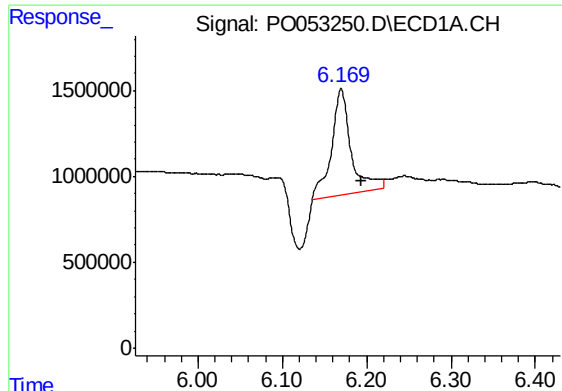

#24 AR-1248-4


R.T.: 6.170 min
Delta R.T.: -0.025 min
Response: 10051621
Conc: 269.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

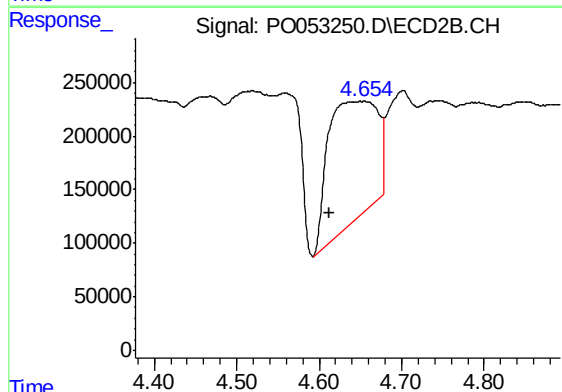


#24 AR-1248-4

R.T.: 4.655 min
Delta R.T.: 0.042 min
Response: 4648151
Conc: 492.50 ng/ml

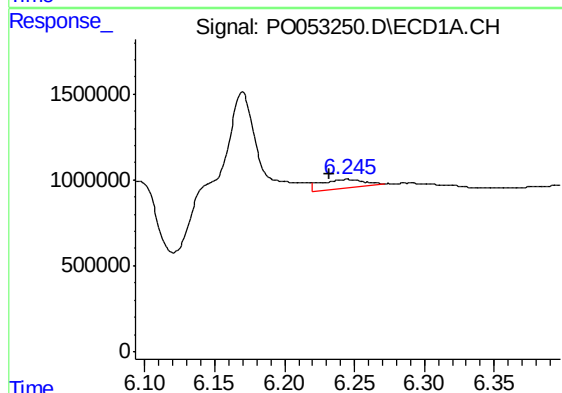


#25 AR-1248-5

R.T.: 6.245 min
Delta R.T.: 0.013 min
Response: 1053581
Conc: 29.57 ng/ml

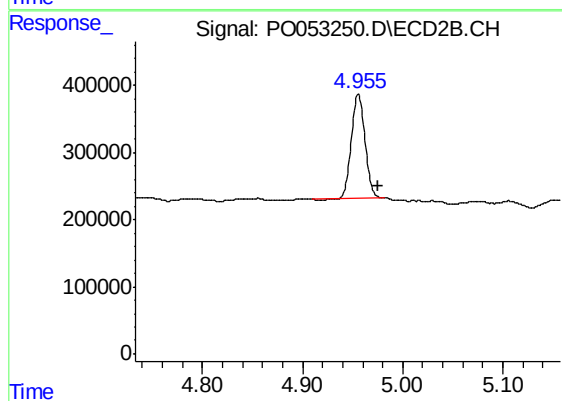

#25 AR-1248-5


R.T.: 4.956 min
Delta R.T.: -0.020 min
Response: 1484036
Conc: 147.92 ng/ml

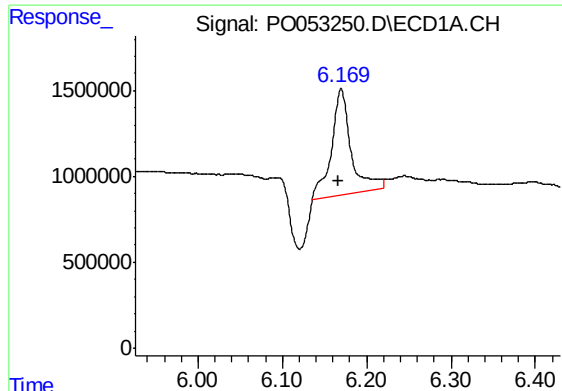

#26 AR-1254-1


R.T.: 6.170 min
Delta R.T.: 0.004 min
Response: 10051621
Conc: 262.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

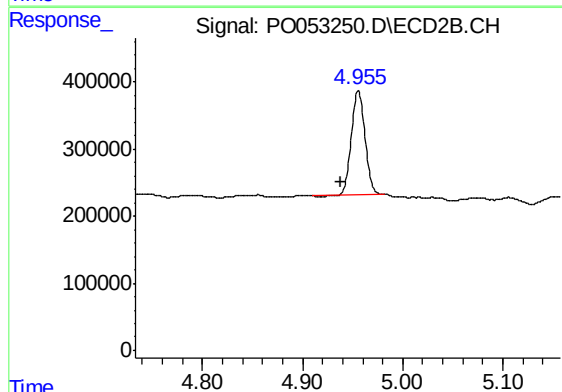


#26 AR-1254-1

R.T.: 4.956 min
Delta R.T.: 0.018 min
Response: 1484036
Conc: 90.52 ng/ml

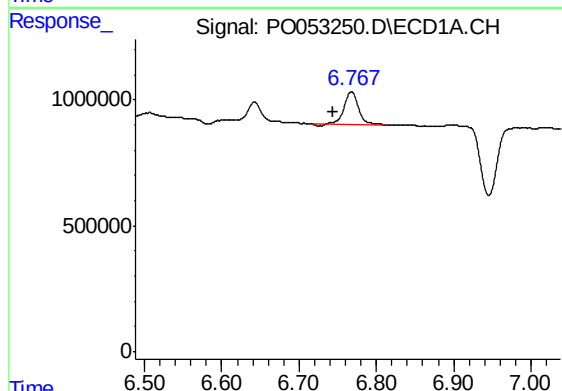


#28 AR-1254-3

R.T.: 6.768 min
Delta R.T.: 0.023 min
Response: 1675566
Conc: 27.17 ng/ml

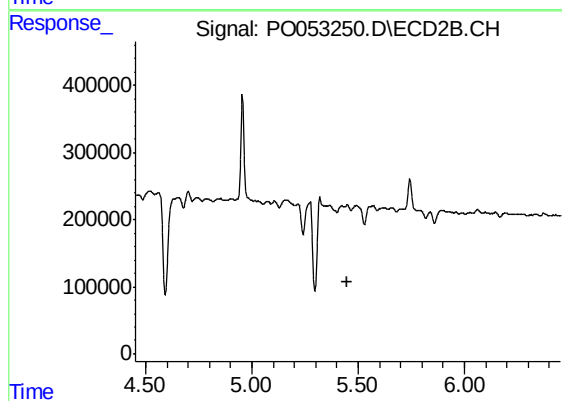

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 5.452 min
Response: 0
Conc: N.D.

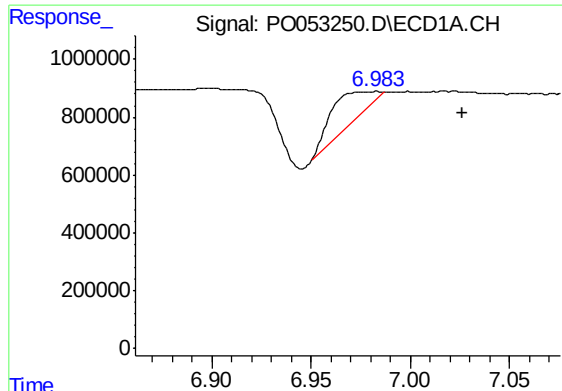

#29 AR-1254-4


R.T.: 6.983 min
Delta R.T.: -0.043 min
Response: 1474422
Conc: 32.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

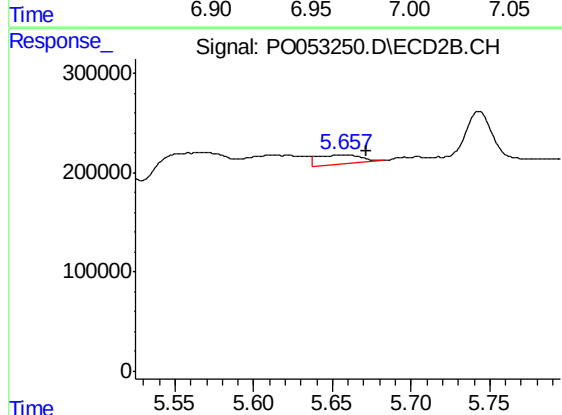


#29 AR-1254-4

R.T.: 5.657 min
Delta R.T.: -0.015 min
Response: 175976
Conc: 11.61 ng/ml

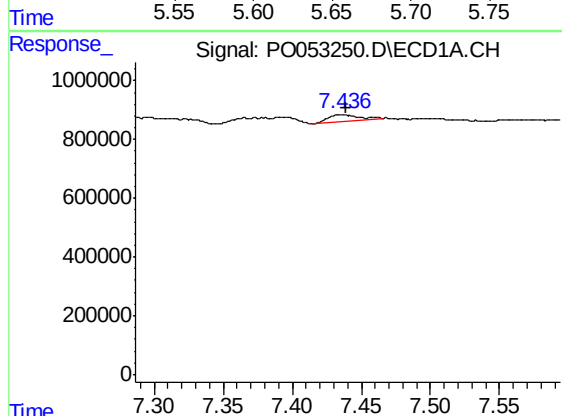


#30 AR-1254-5

R.T.: 7.436 min
Delta R.T.: -0.002 min
Response: 352525
Conc: 7.77 ng/ml

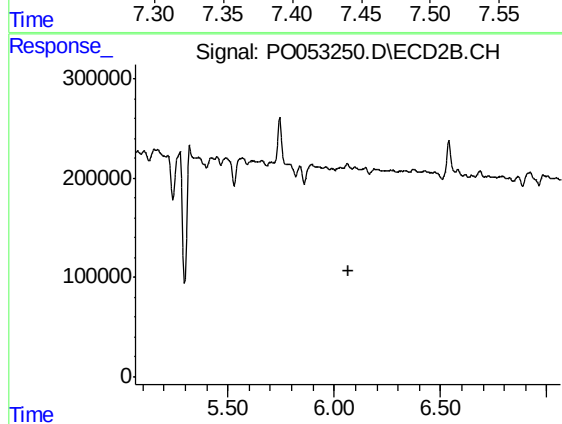

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T. : 6.065 min
Response: 0
Conc: N.D.

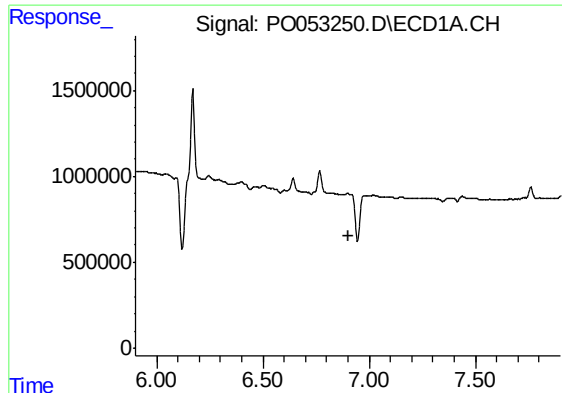

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.901 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

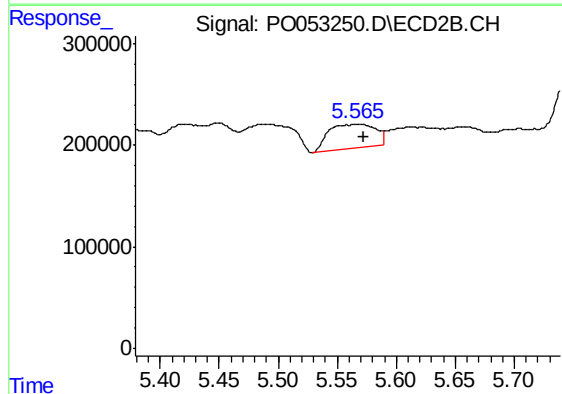


#31 AR-1260-1

R.T.: 5.571 min
Delta R.T.: -0.001 min
Response: 662806
Conc: 43.18 ng/ml

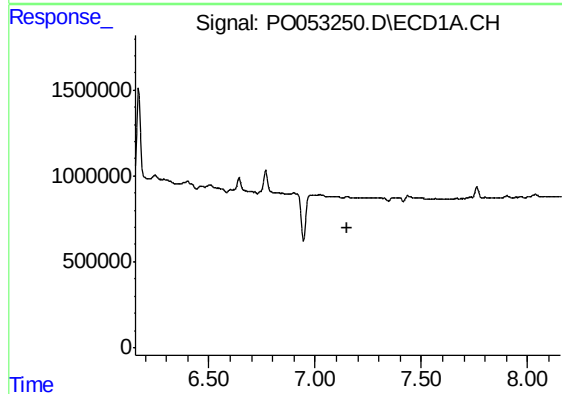


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.154 min
Response: 0
Conc: N.D.

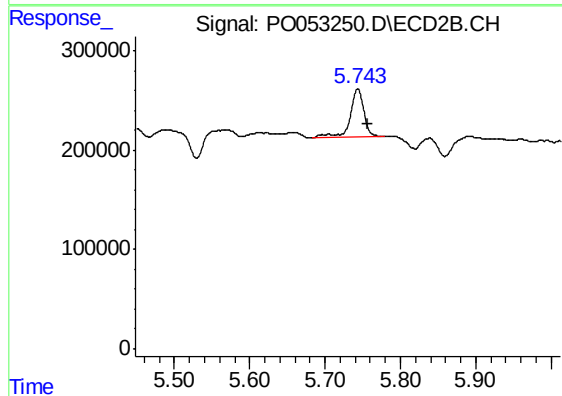

#32 AR-1260-2


R.T.: 5.743 min
Delta R.T.: -0.014 min
Response: 618952
Conc: 32.34 ng/ml

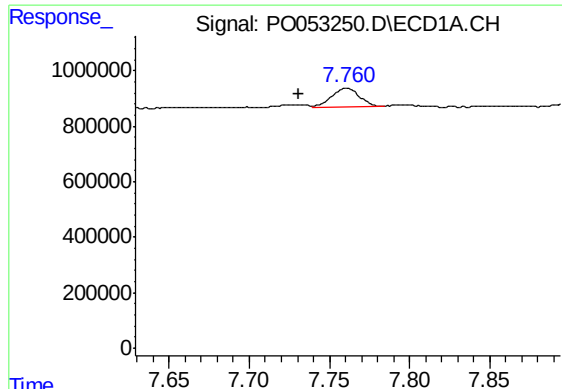

#34 AR-1260-4


R.T.: 7.761 min
Delta R.T.: 0.030 min
Response: 800539
Conc: 20.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

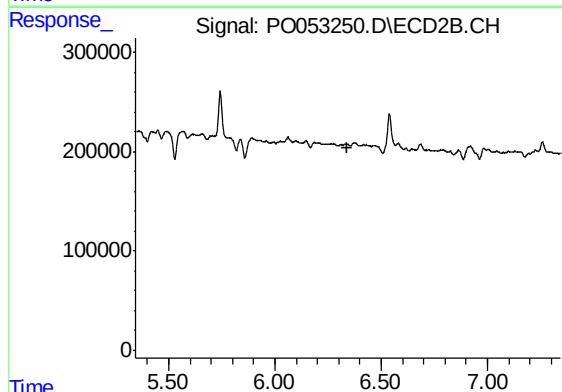


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 6.343 min
Response: 0
Conc: N.D.

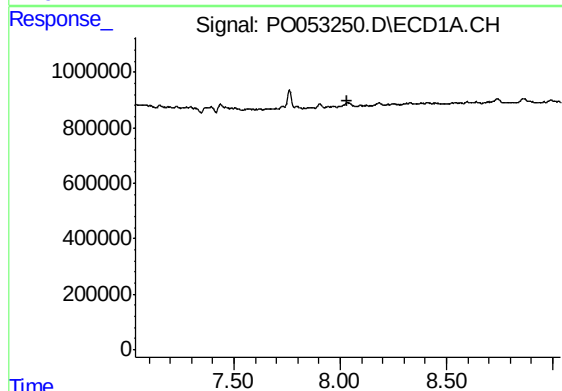


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.036 min
Response: 0
Conc: N.D.

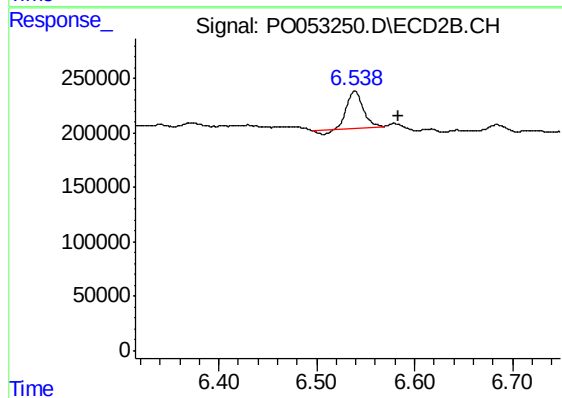

#35 AR-1260-5


R.T.: 6.539 min
Delta R.T.: -0.045 min
Response: 375321
Conc: 13.03 ng/ml

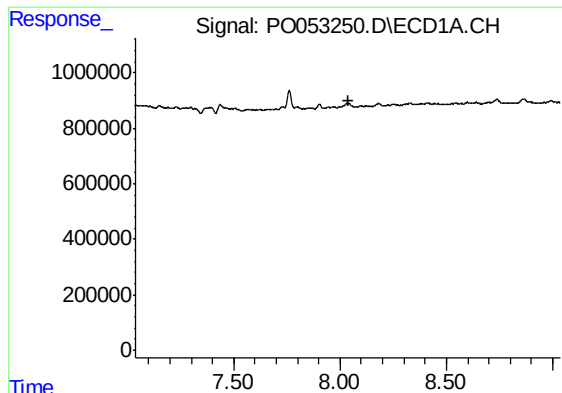

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

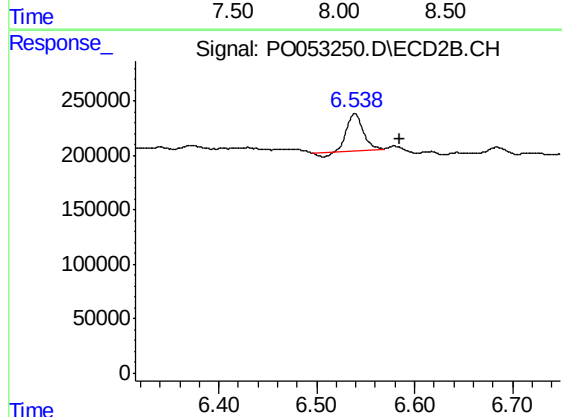


#37 AR-1262-2

R.T.: 6.539 min
Delta R.T.: -0.046 min
Response: 375321
Conc: 11.30 ng/ml

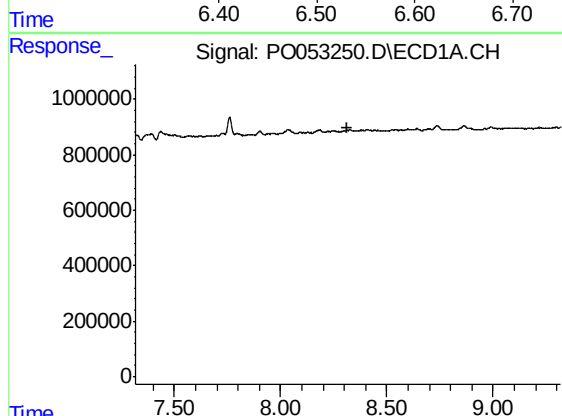


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.317 min
Response: 0
Conc: N.D.

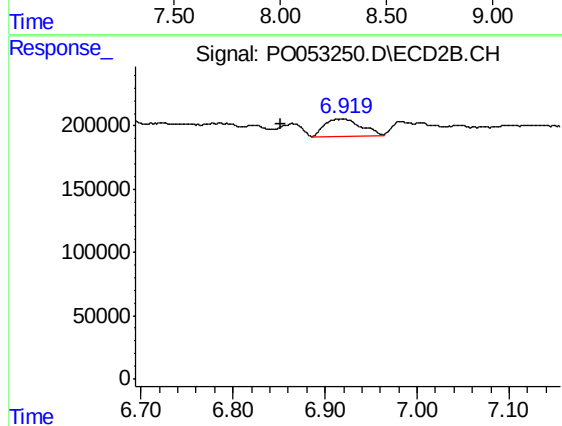

#38 AR-1262-3


R.T.: 6.920 min
Delta R.T.: 0.069 min
Response: 359646
Conc: 27.77 ng/ml

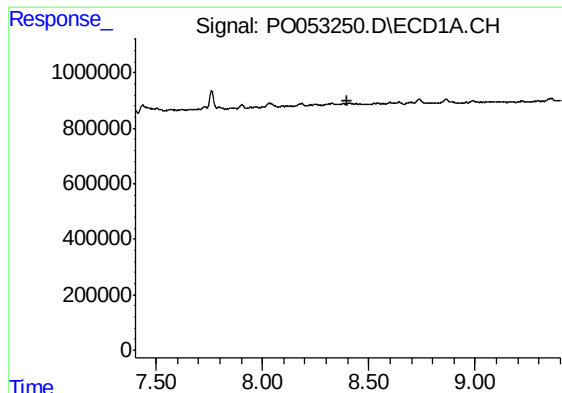

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 8.402 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

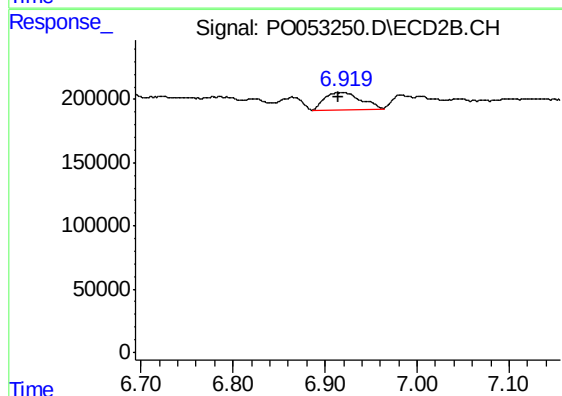


#39 AR-1262-4

R.T.: 6.920 min
Delta R.T.: 0.006 min
Response: 359646
Conc: 14.81 ng/ml

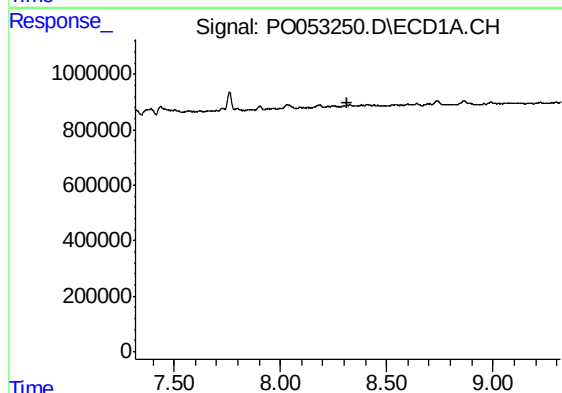


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.318 min
Response: 0
Conc: N.D.

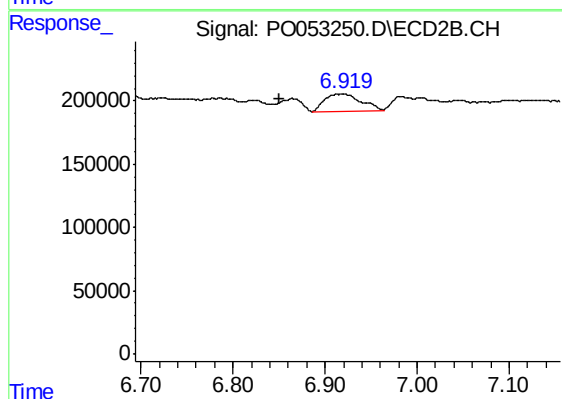

#41 AR-1268-1


R.T.: 6.920 min
Delta R.T.: 0.070 min
Response: 359646
Conc: 8.28 ng/ml

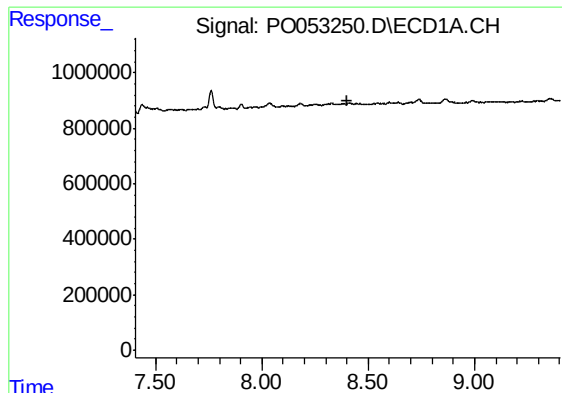

#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.404 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

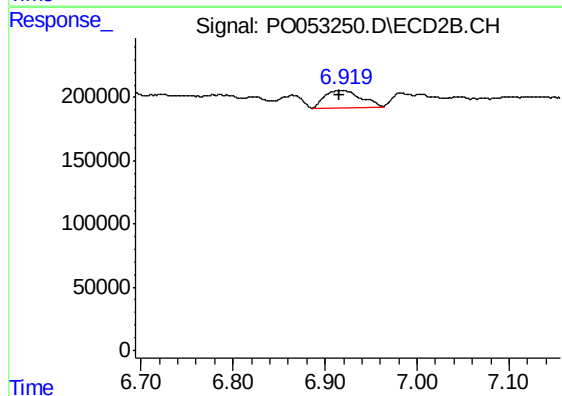

#42 AR-1268-2

R.T.: 6.920 min
Delta R.T.: 0.005 min
Response: 359646
Conc: 8.75 ng/ml