

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010719\
Data File : P0053250.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2019 11:04
Operator : SM/SJ
Sample : K1034-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 00:31:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.182	3.211	27683728	4554315	21.158	20.296
2)	SA Decachlor...	9.644	7.856	16554873	5067967	20.894	19.715

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010719\
Data File : P0053250.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2019 11:04
Operator : SM/SJ
Sample : K1034-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 00:31:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

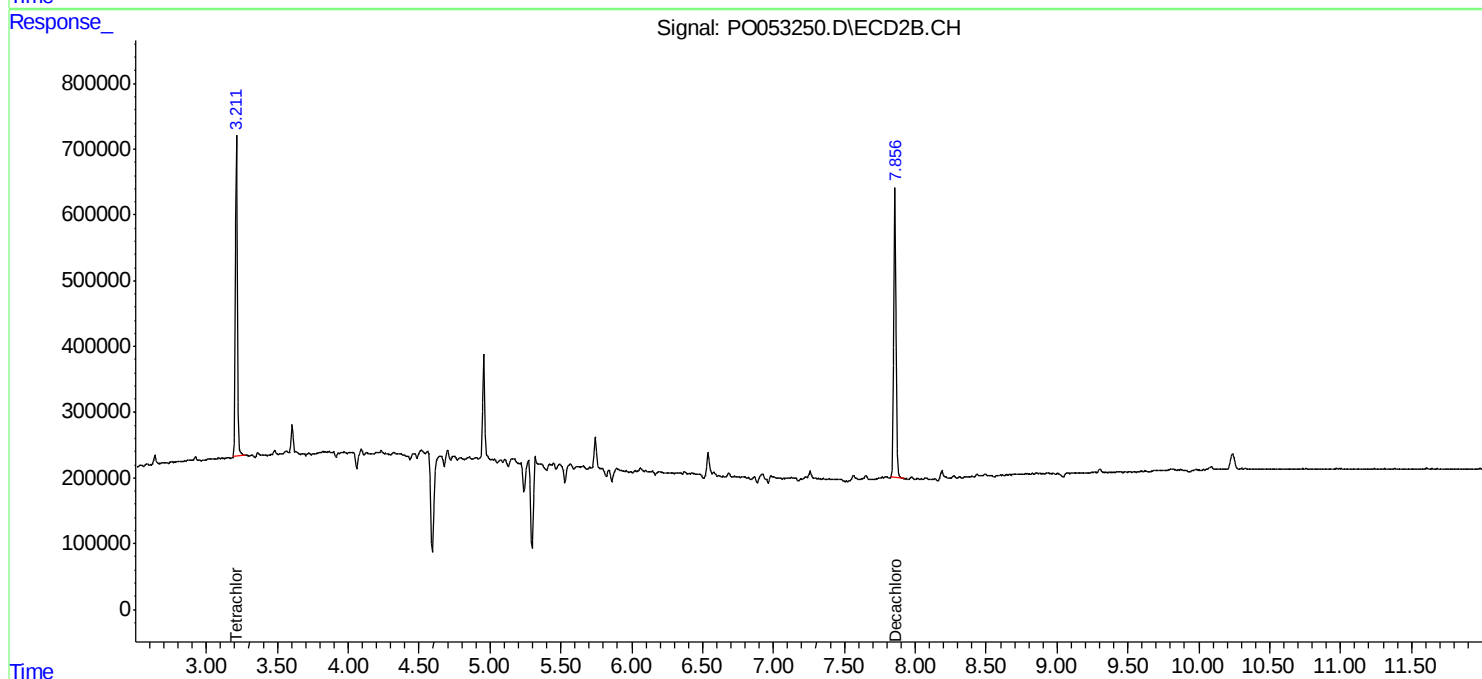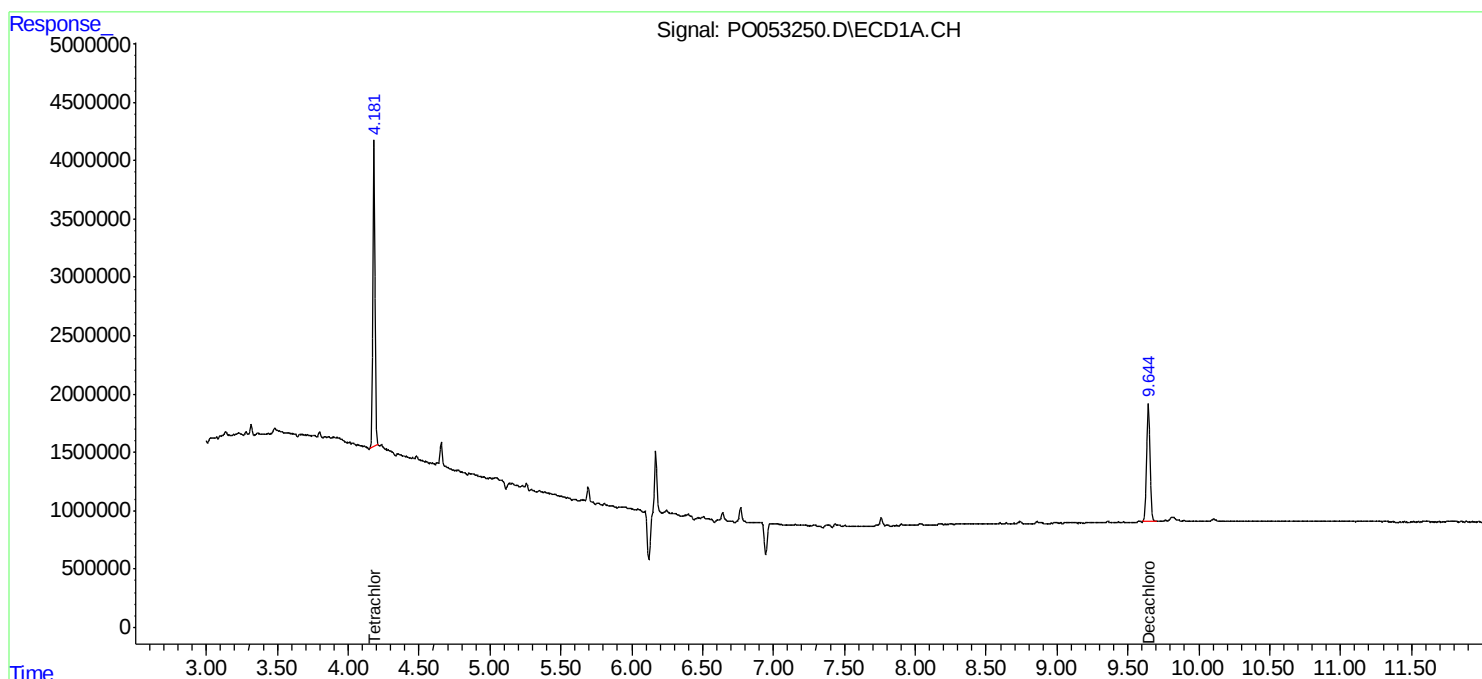


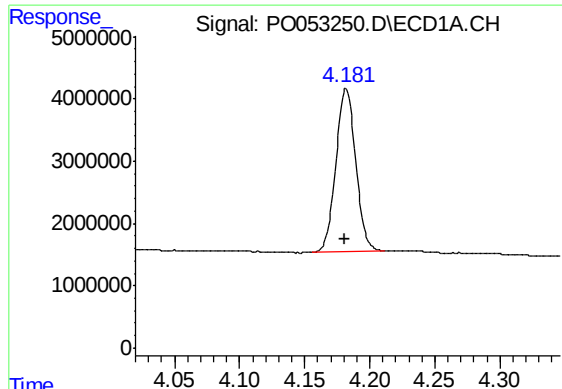

#1 Tetrachloro-m-xylene


R.T.: 4.182 min
Delta R.T.: 0.000 min
Response: 27683728
Conc: 21.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
CONTROL-HOUSE-WALL-1-5

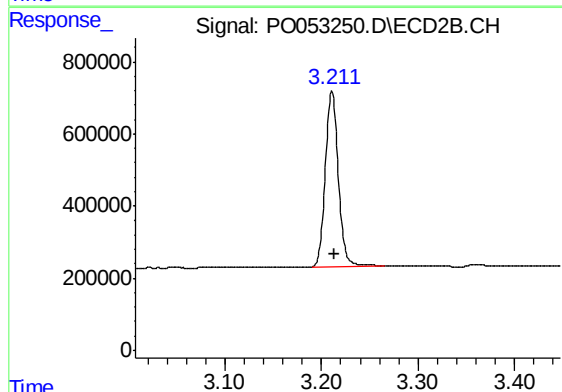


#1 Tetrachloro-m-xylene

R.T.: 3.211 min
Delta R.T.: -0.003 min
Response: 4554315
Conc: 20.30 ng/ml

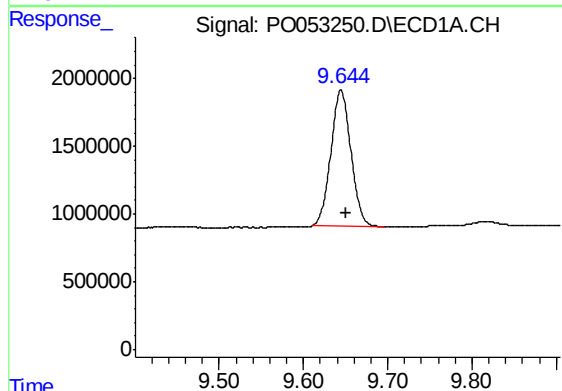

#2 Decachlorobiphenyl

R.T.: 9.644 min
Delta R.T.: -0.006 min
Response: 16554873
Conc: 20.89 ng/ml

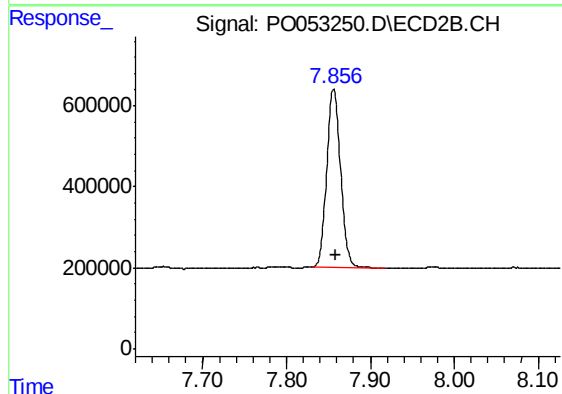

#2 Decachlorobiphenyl

R.T.: 7.856 min
Delta R.T.: -0.003 min
Response: 5067967
Conc: 19.72 ng/ml