

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010719\
 Data File : P0053251.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2019 11:21
 Operator : SM/SJ
 Sample : K1036-20
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 13-V

Manual Integrations
 APPROVED

Sohil
 1/8/2019 11:31:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 00:31:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.174	3.209	32638521	4847344	24.945m	21.602m
2) SA Decachlor...	9.633	7.853	17955401	5452236	22.662m	21.210m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010719\
Data File : P0053251.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2019 11:21
Operator : SM/SJ
Sample : K1036-20
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
13-V


Manual Integrations
APPROVED

Sohil
1/8/2019 11:31:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 00:31:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

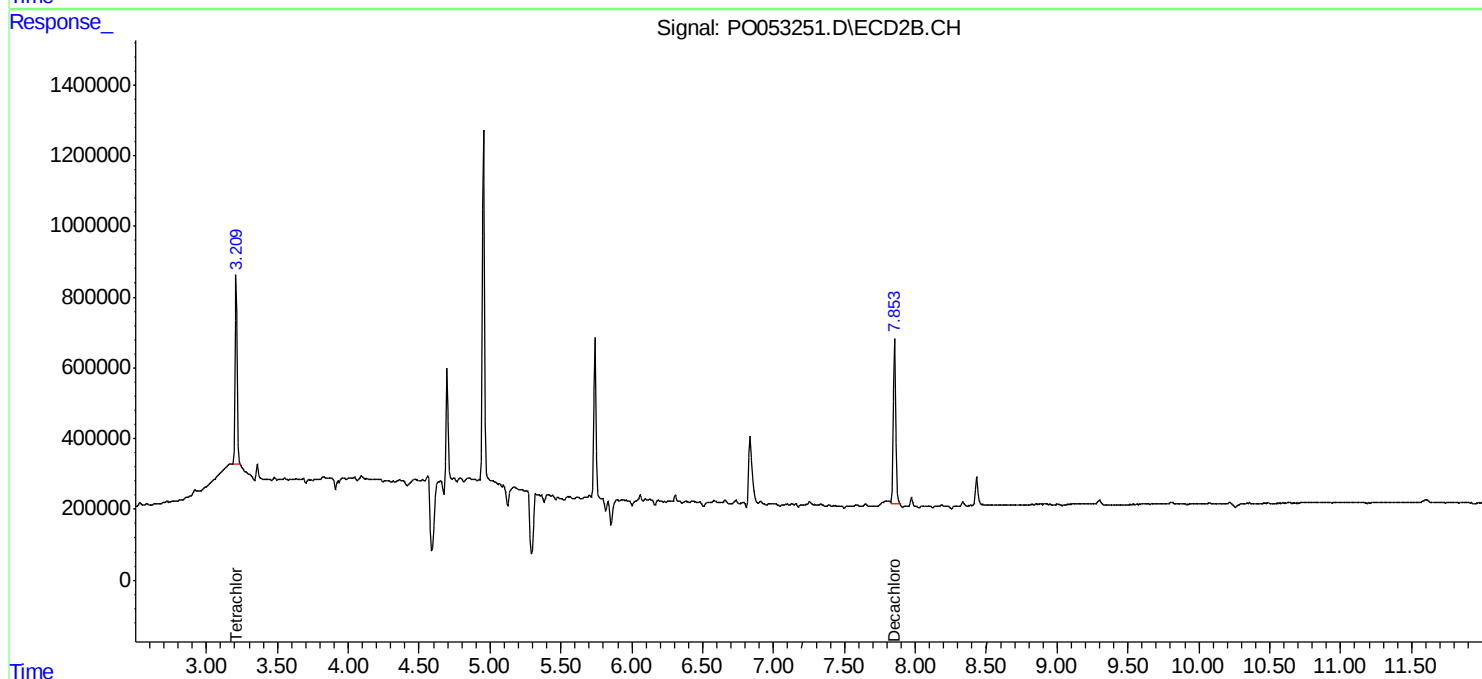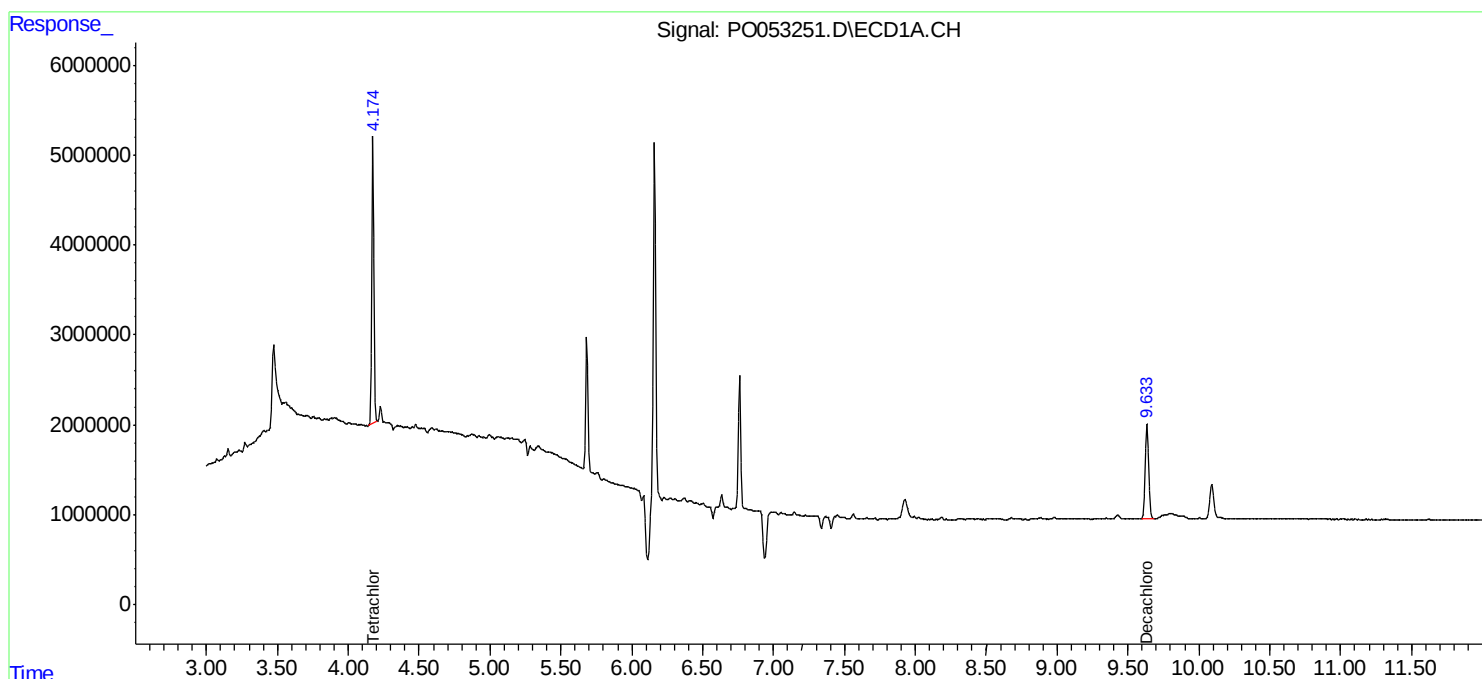

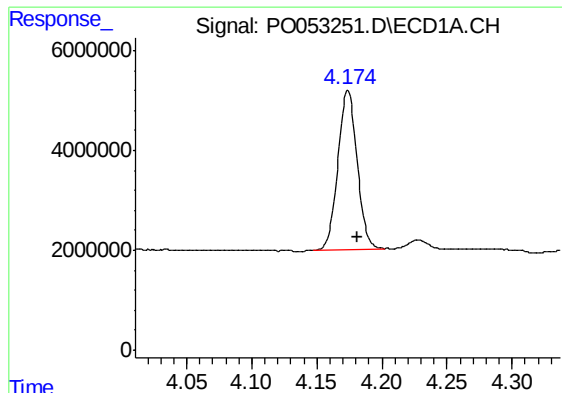


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.007 min
Response: 32638521
Conc: 24.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
13-V


Manual Integrations
APPROVED

Sohil
1/8/2019 11:31:38 AM

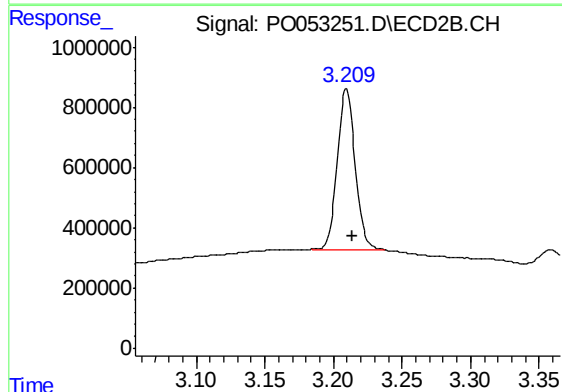


#1 Tetrachloro-m-xylene

R.T.: 3.209 min
Delta R.T.: -0.004 min
Response: 4847344
Conc: 21.60 ng/ml m

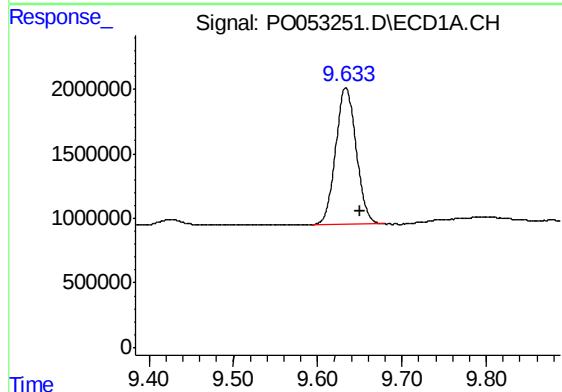

#2 Decachlorobiphenyl

R.T.: 9.633 min
Delta R.T.: -0.018 min
Response: 17955401
Conc: 22.66 ng/ml m

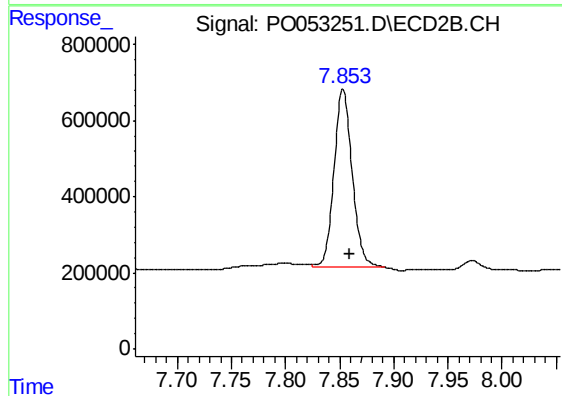

#2 Decachlorobiphenyl

R.T.: 7.853 min
Delta R.T.: -0.006 min
Response: 5452236
Conc: 21.21 ng/ml m