

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010719\
 Data File : P0053270.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2019 17:44
 Operator : SM/SJ
 Sample : K1052-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SSSI-0103-S-DH-8A

Manual Integrations
 APPROVED

Sohil
 1/8/2019 11:31:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 00:41:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010219.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 02 14:46:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.174	3.211	22790061	4742903	17.418m	21.137
2) SA Decachlor...	9.633	7.853	12827330	3431014	16.190m	13.347m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010719\
Data File : PO053270.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2019 17:44
Operator : SM/SJ
Sample : K1052-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SSSI-0103-S-DH-8A


Manual Integrations
APPROVED

Sohil
1/8/2019 11:31:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 00:41:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010219.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 02 14:46:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

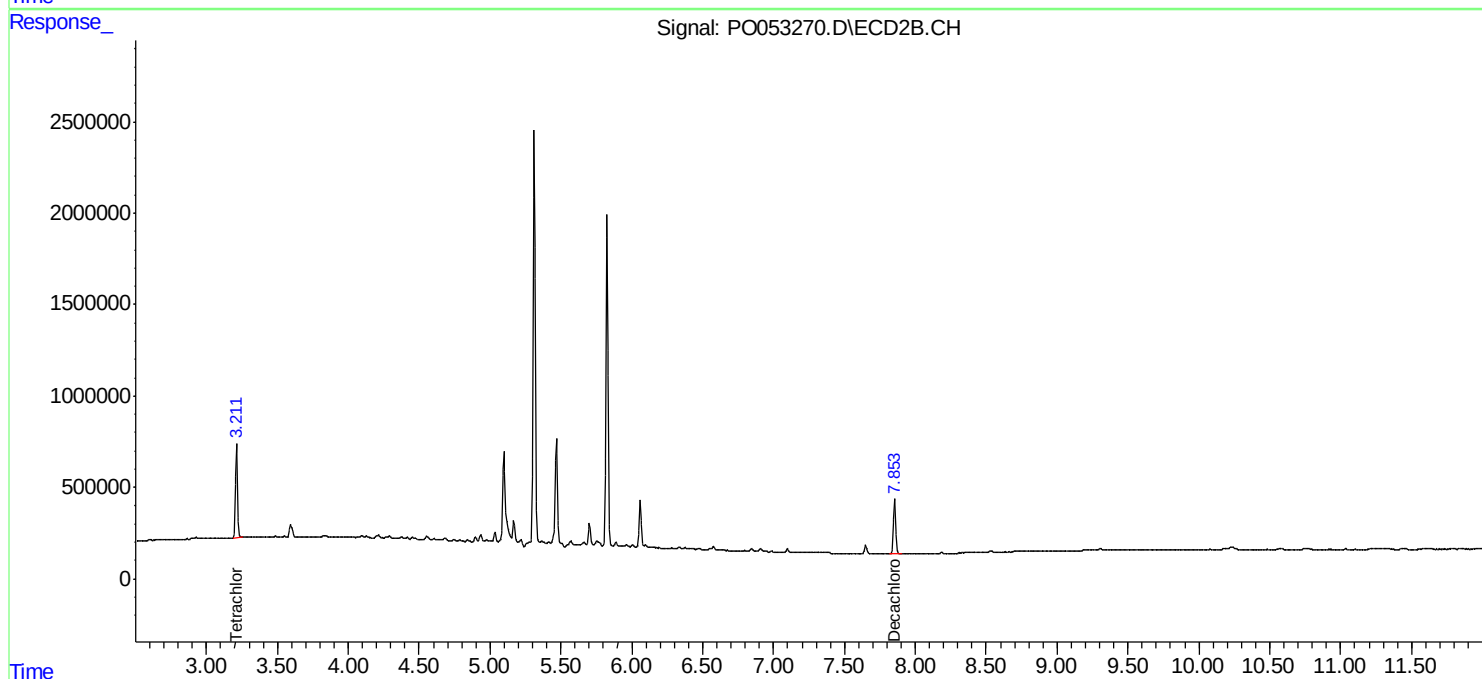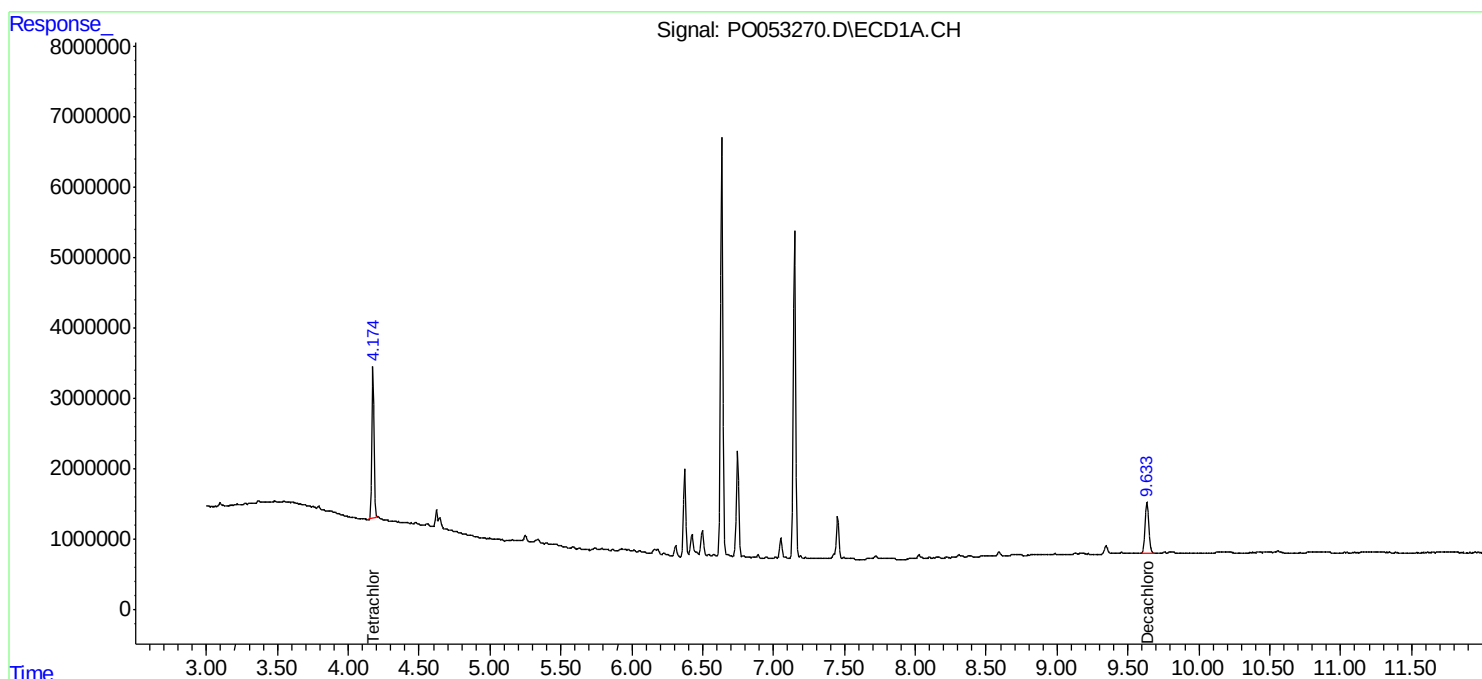

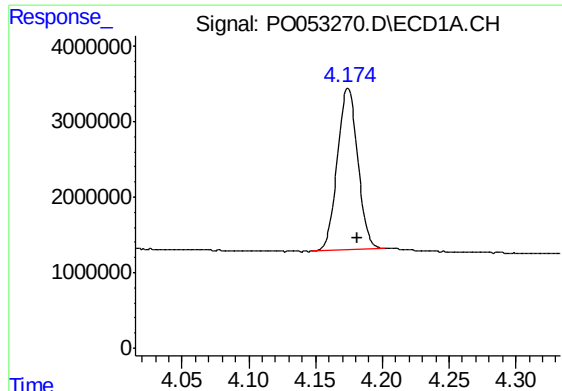


#1 Tetrachloro-m-xylene

R.T.: 4.174 min
Delta R.T.: -0.007 min
Response: 22790061
Conc: 17.42 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SSSI-0103-S-DH-8A


Manual Integrations
APPROVED

Sohil
1/8/2019 11:31:58 AM

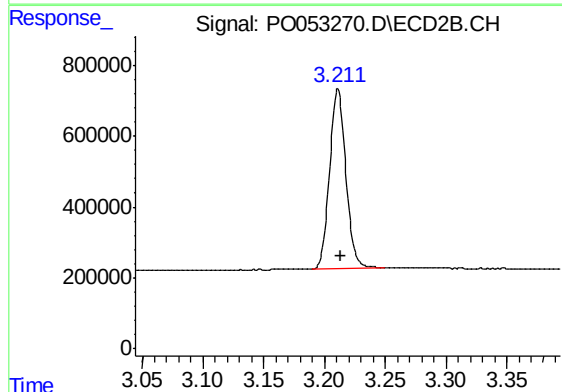


#1 Tetrachloro-m-xylene

R.T.: 3.211 min
Delta R.T.: -0.003 min
Response: 4742903
Conc: 21.14 ng/ml

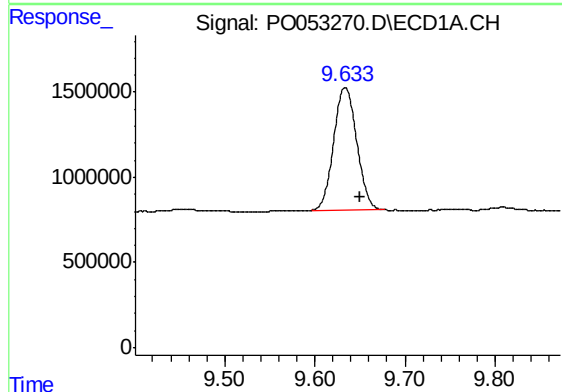

#2 Decachlorobiphenyl

R.T.: 9.633 min
Delta R.T.: -0.017 min
Response: 12827330
Conc: 16.19 ng/ml m

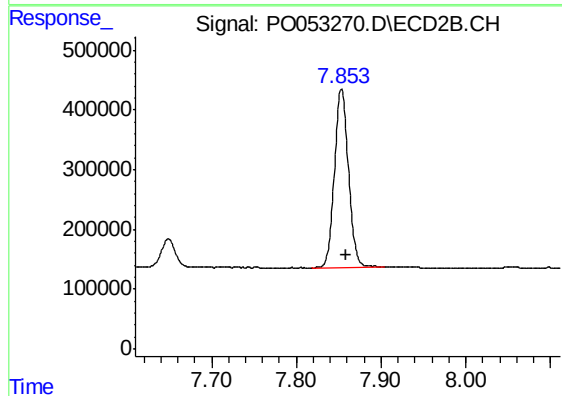

#2 Decachlorobiphenyl

R.T.: 7.853 min
Delta R.T.: -0.006 min
Response: 3431014
Conc: 13.35 ng/ml m