

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010720\
 Data File : P0065352.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2020 13:06
 Operator : AJ/MA
 Sample : L1038-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 01-06-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 13:23:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.166	3.440	482502	540271	26.423	24.561
2) SA Decachlor...	9.676	8.349	589297	687203	17.392	16.571

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010720\
Data File : P0065352.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2020 13:06
Operator : AJ/MA
Sample : L1038-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
01-06-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 13:23:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

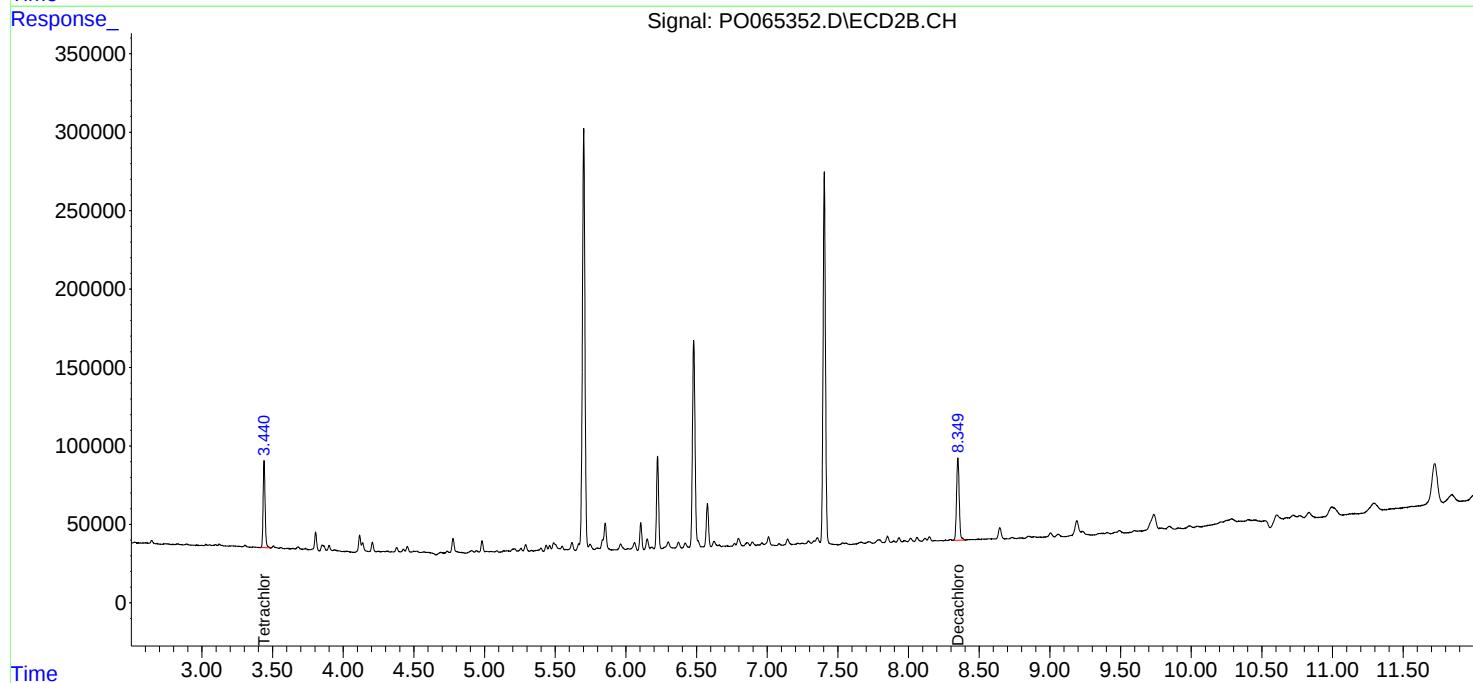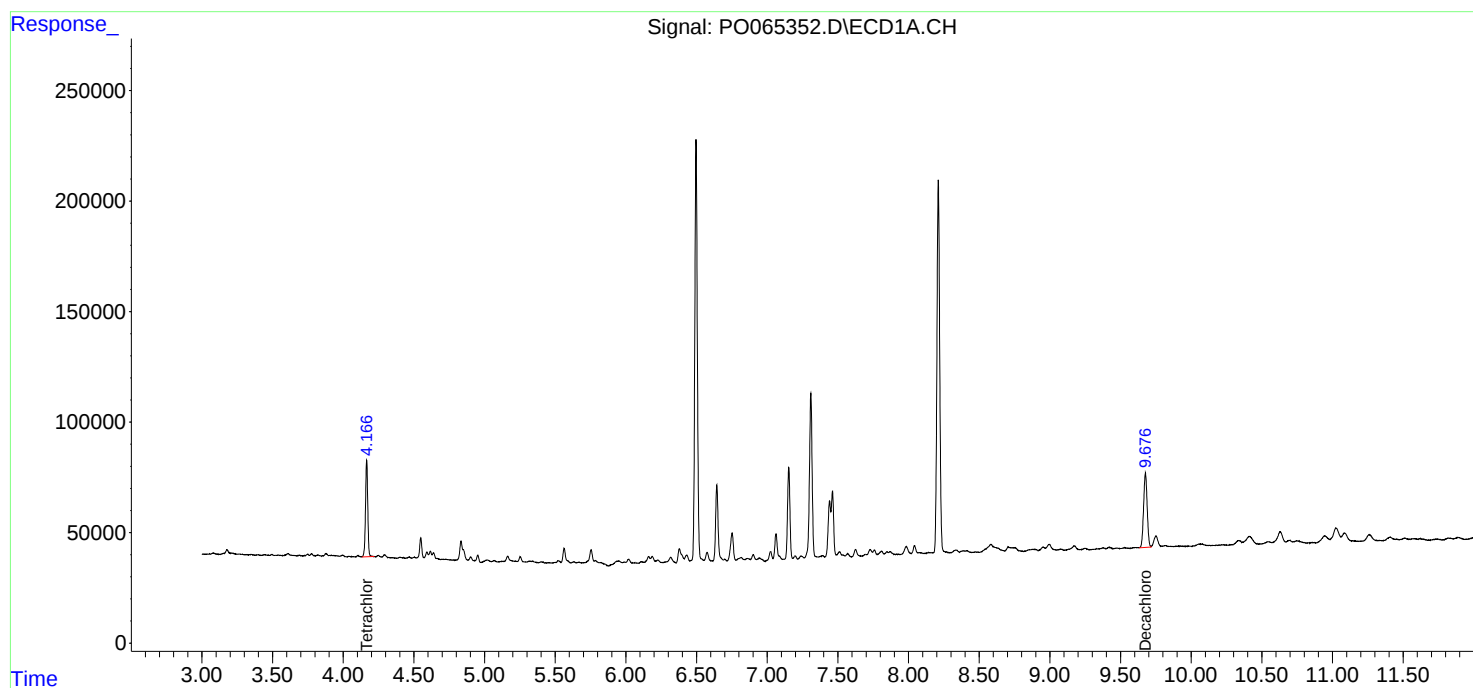


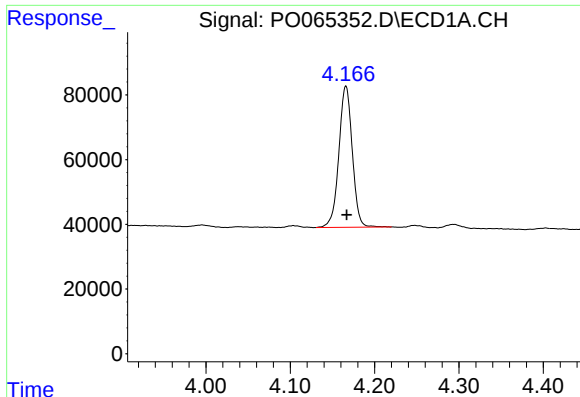

#1 Tetrachloro-m-xylene


R.T.: 4.166 min
Delta R.T.: 0.000 min
Response: 482502
Conc: 26.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
01-06-A

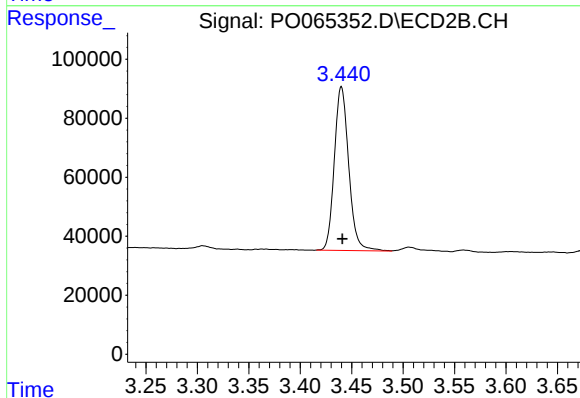


#1 Tetrachloro-m-xylene

R.T.: 3.440 min
Delta R.T.: -0.001 min
Response: 540271
Conc: 24.56 ng/ml

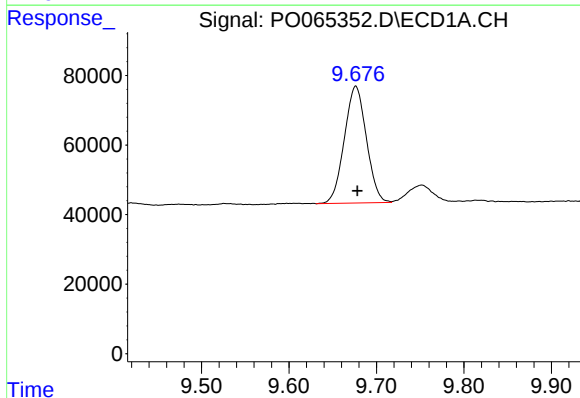

#2 Decachlorobiphenyl

R.T.: 9.676 min
Delta R.T.: -0.002 min
Response: 589297
Conc: 17.39 ng/ml

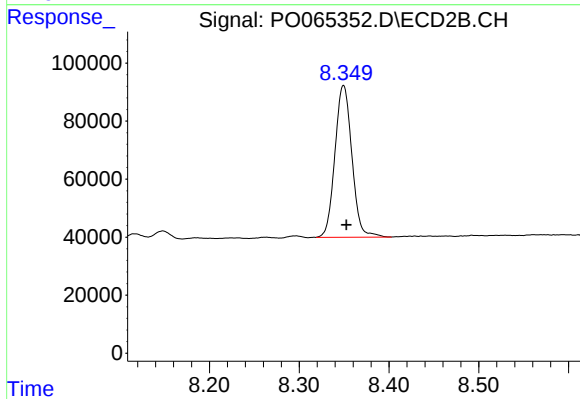

#2 Decachlorobiphenyl

R.T.: 8.349 min
Delta R.T.: -0.003 min
Response: 687203
Conc: 16.57 ng/ml