

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010720\
 Data File : P0065353.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2020 13:22
 Operator : AJ/MA
 Sample : L1038-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 01-06-B

Manual Integrations
 APPROVED

mohammad
 1/7/2020 4:16:26 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 13:36:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.170	3.447	511344	613890	28.003m	27.907
2) SA Decachlor...	9.677	8.351	541456	814090	15.980	19.631m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010720\
Data File : P0065353.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2020 13:22
Operator : AJ/MA
Sample : L1038-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
01-06-B


Manual Integrations
APPROVED

mohammad
1/7/2020 4:16:26 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 13:36:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

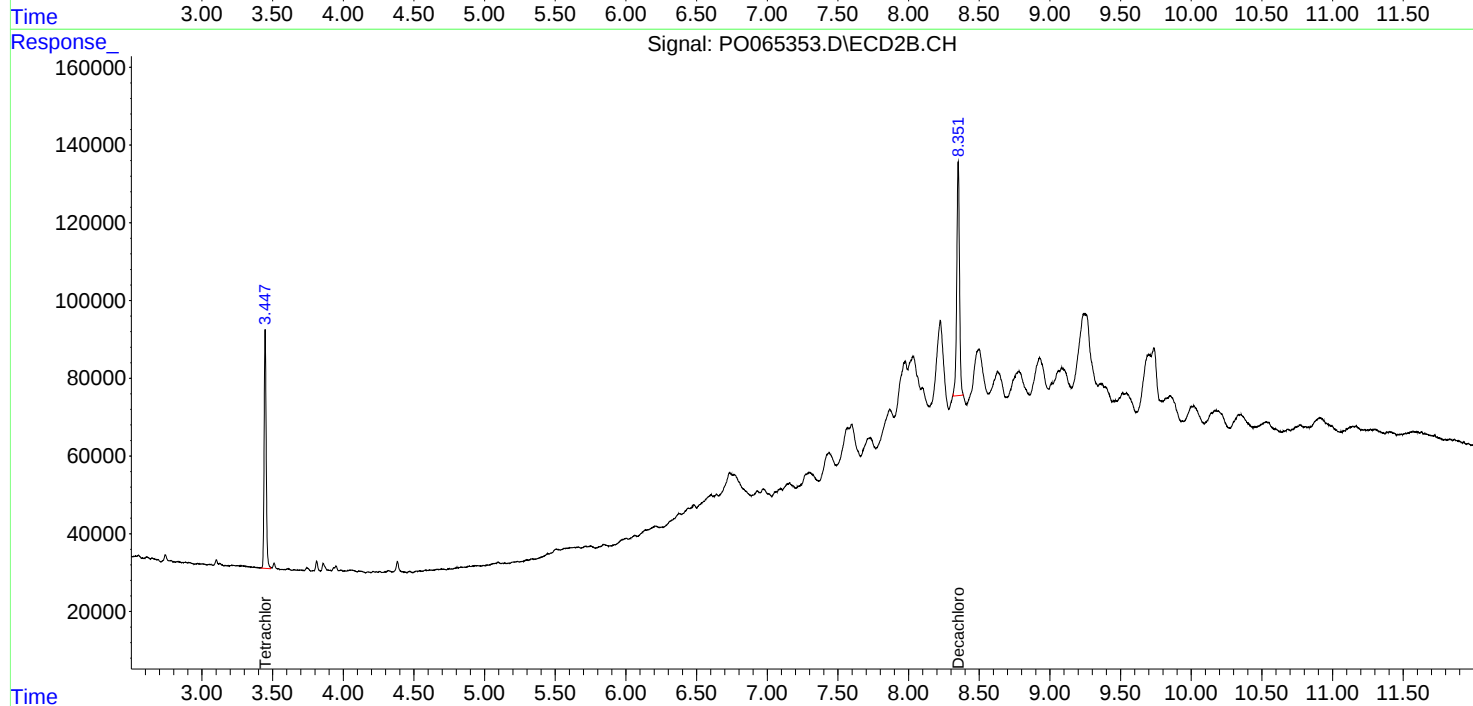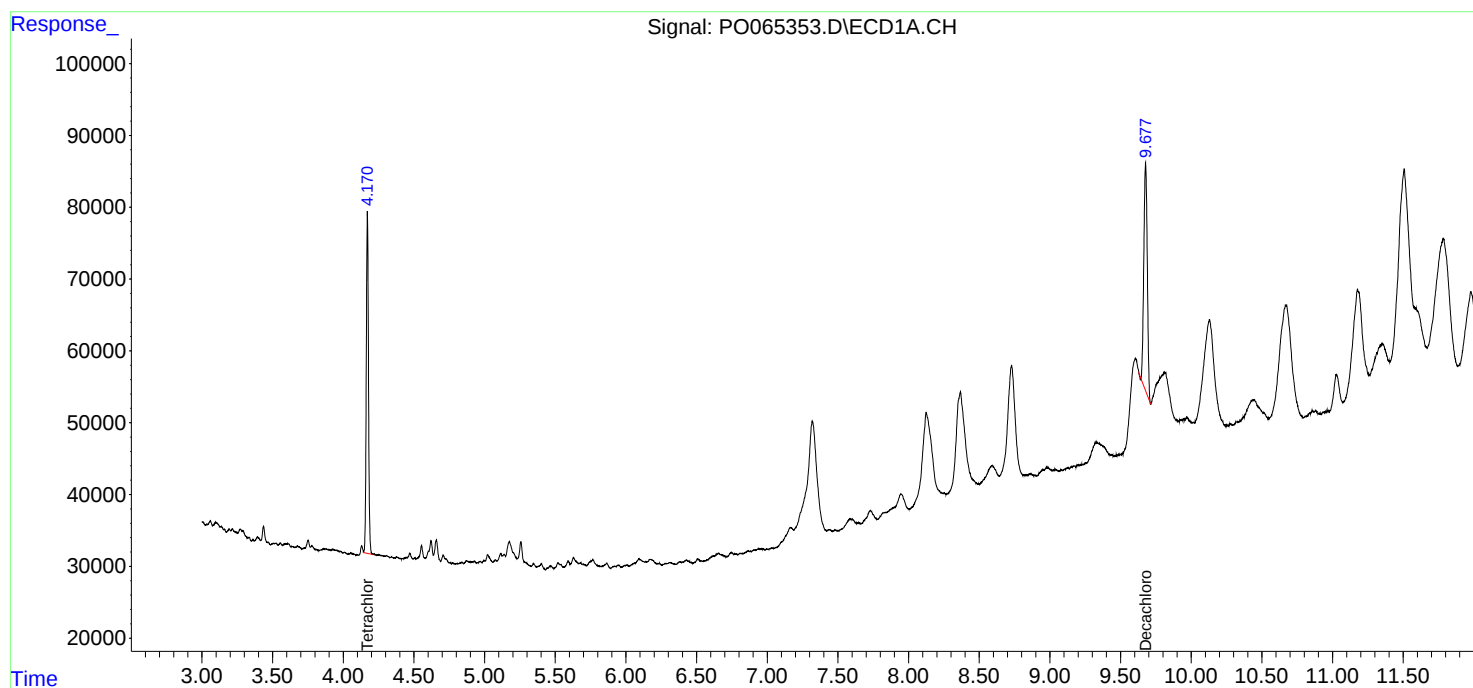

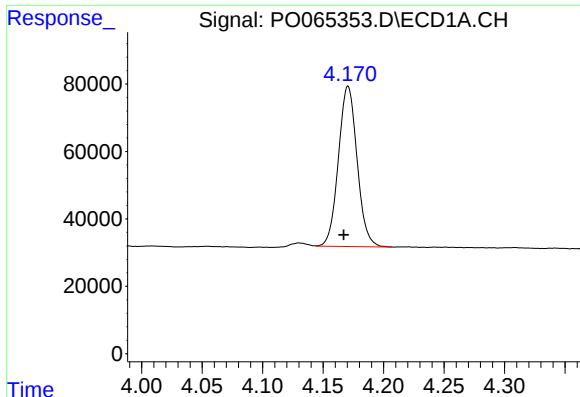


#1 Tetrachloro-m-xylene

R.T.: 4.170 min
Delta R.T.: 0.003 min
Response: 511344
Conc: 28.00 ng/ml m

Instrument :
ECD_O
ClientSampleId :
01-06-B


Manual Integrations
APPROVED

mohammad
1/7/2020 4:16:26 PM

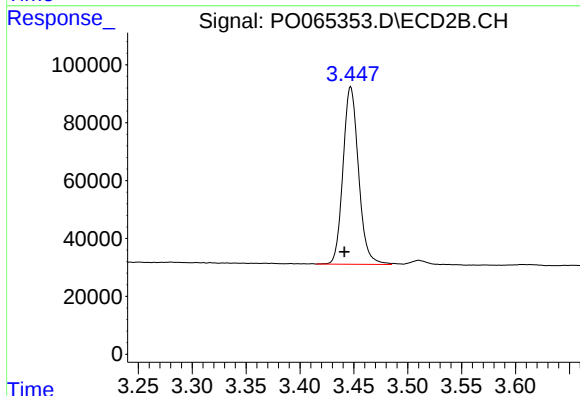


#1 Tetrachloro-m-xylene

R.T.: 3.447 min
Delta R.T.: 0.006 min
Response: 613890
Conc: 27.91 ng/ml

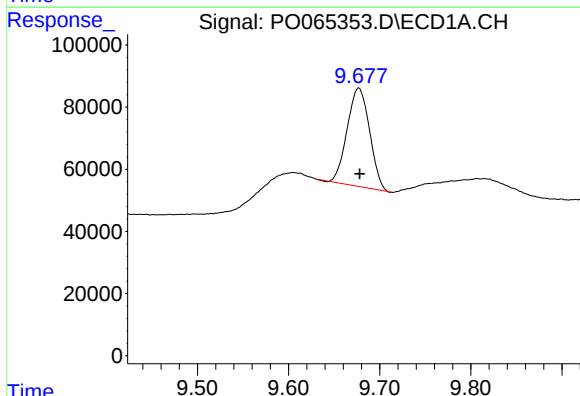

#2 Decachlorobiphenyl

R.T.: 9.677 min
Delta R.T.: -0.001 min
Response: 541456
Conc: 15.98 ng/ml

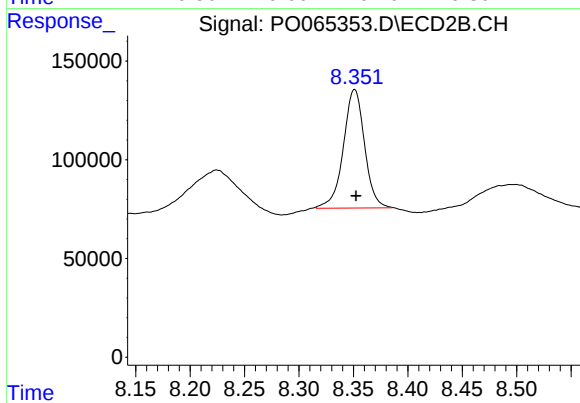

#2 Decachlorobiphenyl

R.T.: 8.351 min
Delta R.T.: -0.002 min
Response: 814090
Conc: 19.63 ng/ml m