

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010721\
 Data File : P0074418.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2021 12:14
 Operator : DD\AJ
 Sample : M1022-02 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40967

Manual Integrations
 APPROVED

Ankita
 1/8/2021 10:10:57 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 16:22:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 05:03:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.932	3.988	158085	102365	1.645m	1.922
2)	SA Decachlor...	10.960	9.252	226749	105764	2.439	2.032
Target Compounds							
26)	L6 AR-1254-1	7.167	6.101	295661	234787	71.742	64.838
27)	L6 AR-1254-2	7.398	6.260	509787	201285	78.358	63.647
28)	L6 AR-1254-3	7.781	6.677	452676	301985	68.482	60.183
29)	L6 AR-1254-4	8.078	6.917	479819	270136	84.330	73.959
30)	L6 AR-1254-5	8.509	7.345	544137	436282	100.560	92.579

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010721\
Data File : PO074418.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2021 12:14
Operator : DD\AJ
Sample : M1022-02 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
40967


Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:57 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 16:22:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

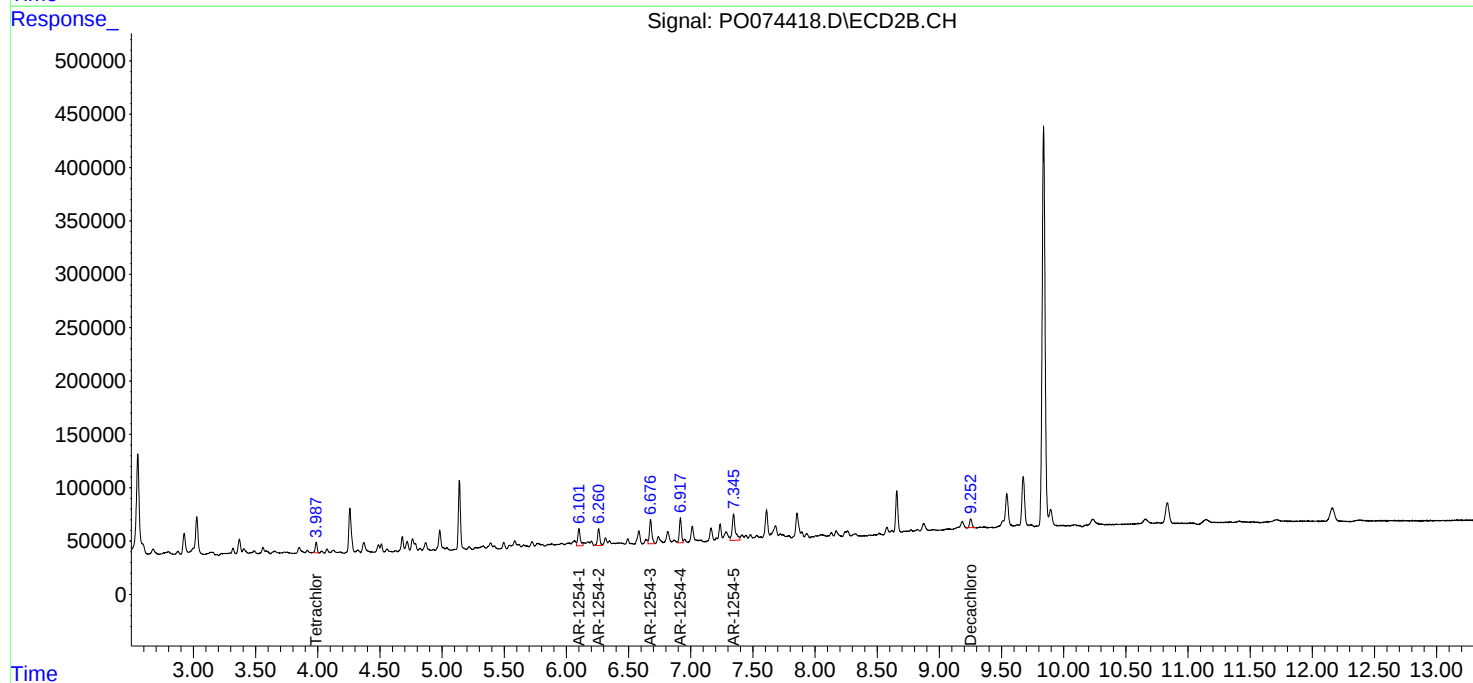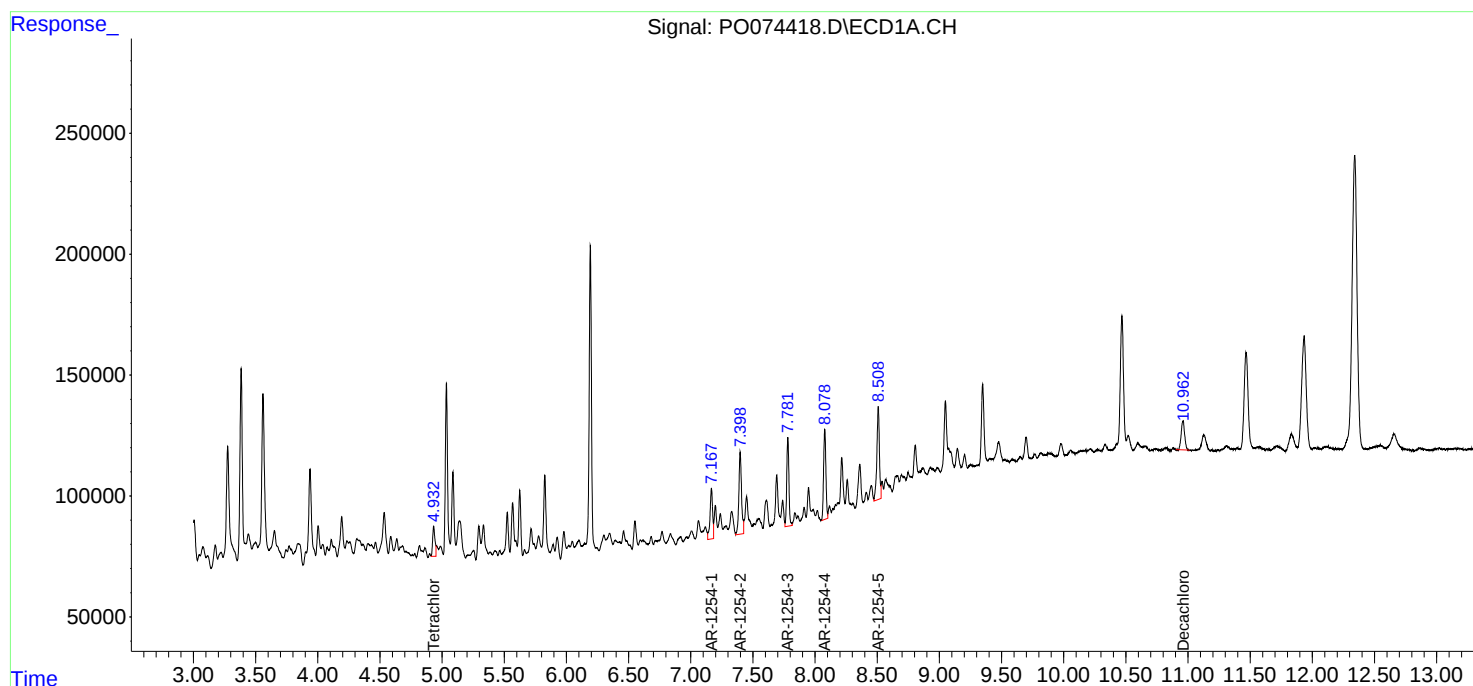

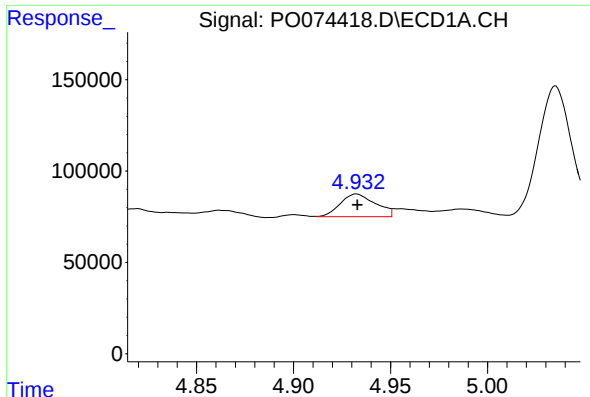


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 158085
Conc: 1.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
40967


Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:57 AM

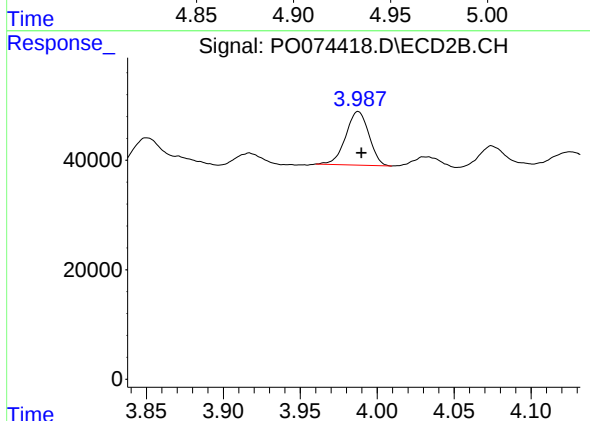


#1 Tetrachloro-m-xylene

R.T.: 3.988 min
Delta R.T.: -0.002 min
Response: 102365
Conc: 1.92 ng/ml

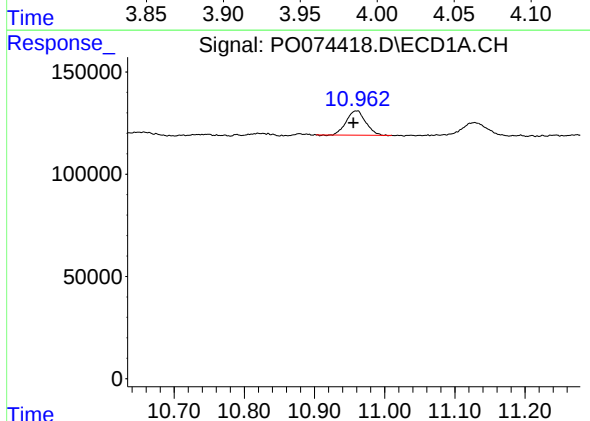


#2 Decachlorobiphenyl

R.T.: 10.960 min
Delta R.T.: 0.004 min
Response: 226749
Conc: 2.44 ng/ml

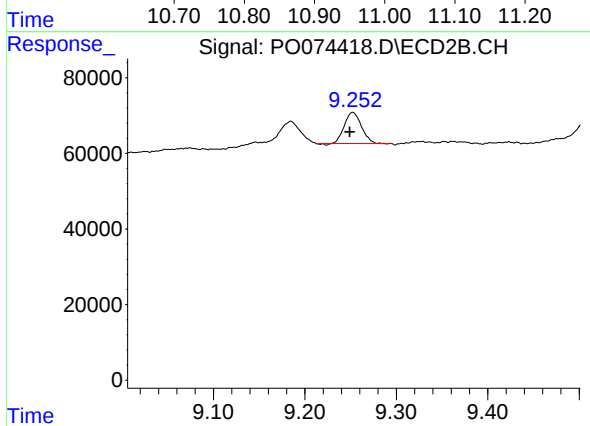

#2 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: 0.003 min
Response: 105764
Conc: 2.03 ng/ml

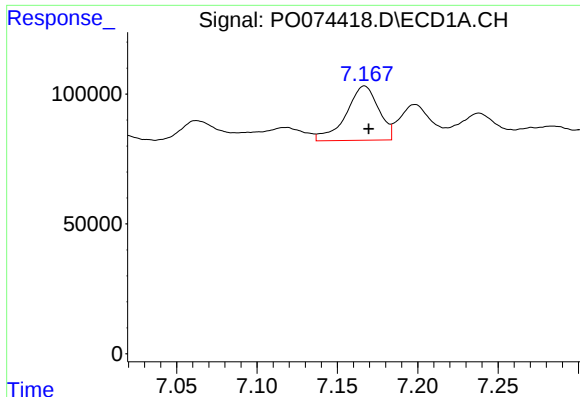


#26 AR-1254-1

R.T.: 7.167 min
Delta R.T.: -0.003 min
Response: 295661
Conc: 71.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
40967


Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:57 AM

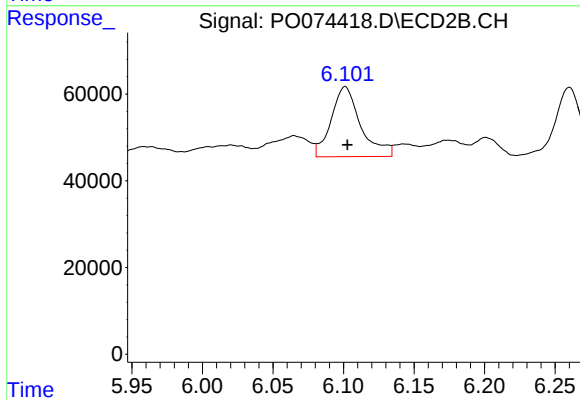


#26 AR-1254-1

R.T.: 6.101 min
Delta R.T.: -0.002 min
Response: 234787
Conc: 64.84 ng/ml

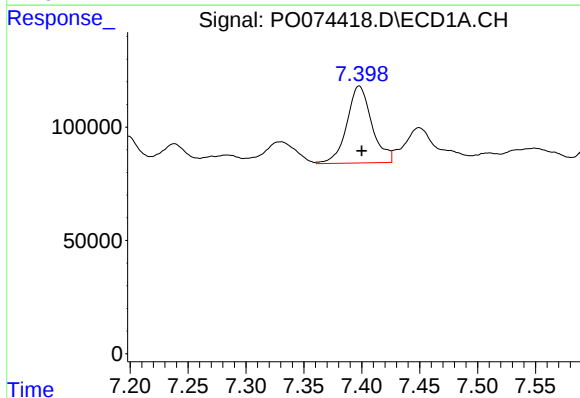


#27 AR-1254-2

R.T.: 7.398 min
Delta R.T.: -0.002 min
Response: 509787
Conc: 78.36 ng/ml

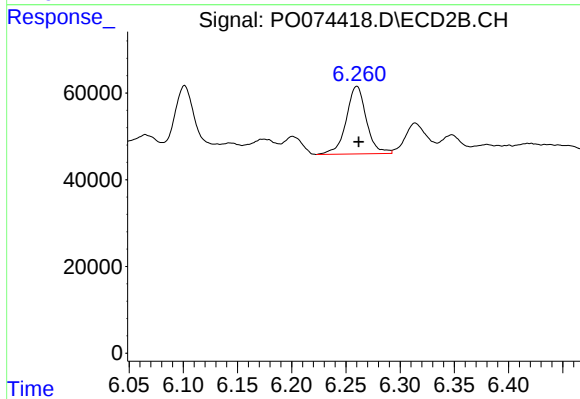

#27 AR-1254-2

R.T.: 6.260 min
Delta R.T.: -0.002 min
Response: 201285
Conc: 63.65 ng/ml

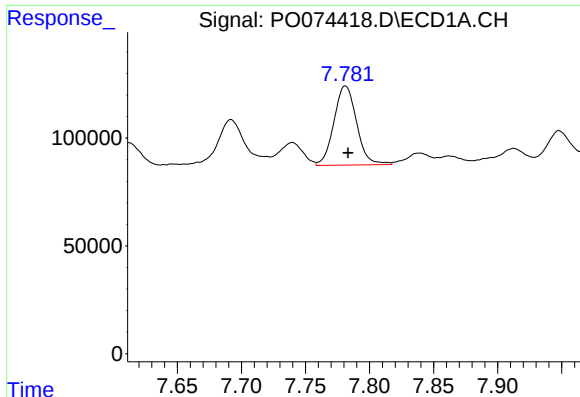


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: -0.002 min
Response: 452676
Conc: 68.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
40967


Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:57 AM

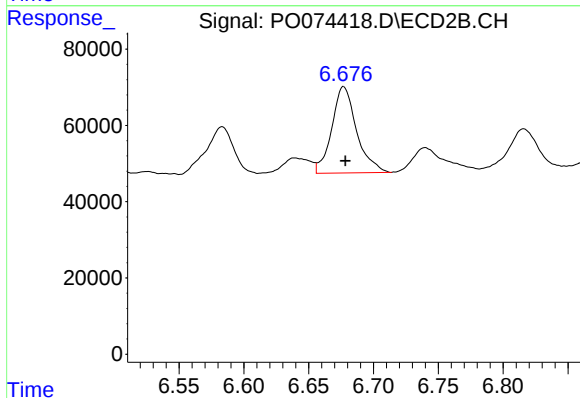


#28 AR-1254-3

R.T.: 6.677 min
Delta R.T.: -0.001 min
Response: 301985
Conc: 60.18 ng/ml

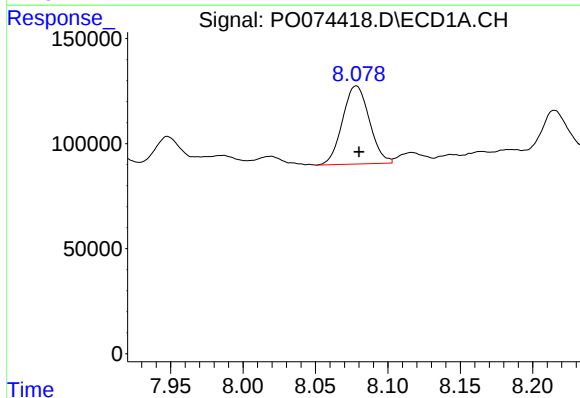


#29 AR-1254-4

R.T.: 8.078 min
Delta R.T.: -0.002 min
Response: 479819
Conc: 84.33 ng/ml

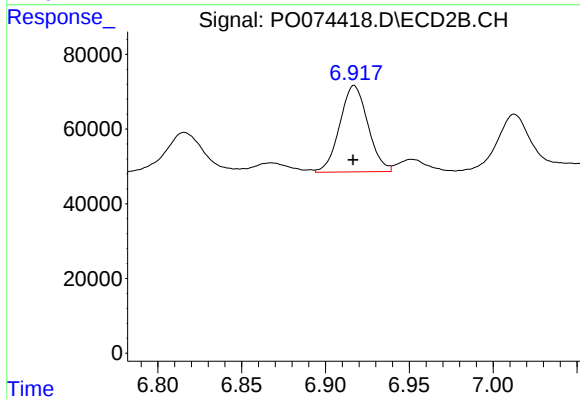

#29 AR-1254-4

R.T.: 6.917 min
Delta R.T.: 0.000 min
Response: 270136
Conc: 73.96 ng/ml

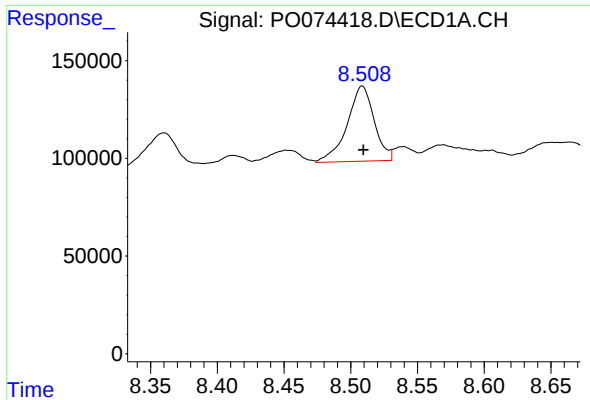


#30 AR-1254-5

R.T.: 8.509 min
Delta R.T.: 0.000 min
Response: 544137
Conc: 100.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
40967

Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:57 AM

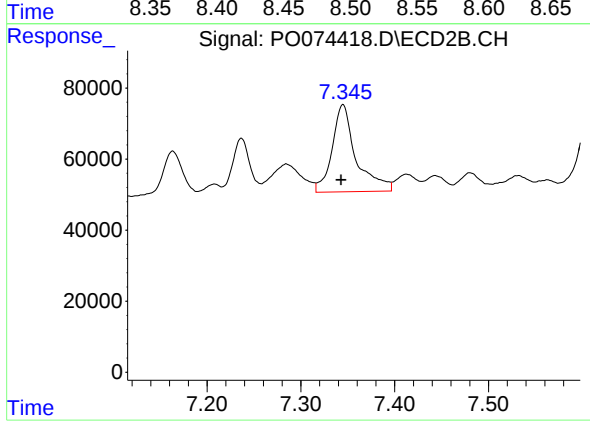

#30 AR-1254-5

R.T.: 7.345 min
Delta R.T.: 0.002 min
Response: 436282
Conc: 92.58 ng/ml