

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010721\
 Data File : P0074419.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2021 12:32
 Operator : DD\AJ
 Sample : M1019-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20410

Manual Integrations
 APPROVED

Ankita
 1/8/2021 10:10:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 16:23:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 05:03:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.934	3.991	2366514	1381636	24.629m	25.937
2) SA Decachlor...	10.952	9.247	2126892	1135432	22.878	21.811

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010721\
Data File : P0074419.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2021 12:32
Operator : DD\AJ
Sample : M1019-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20410


Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 16:23:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

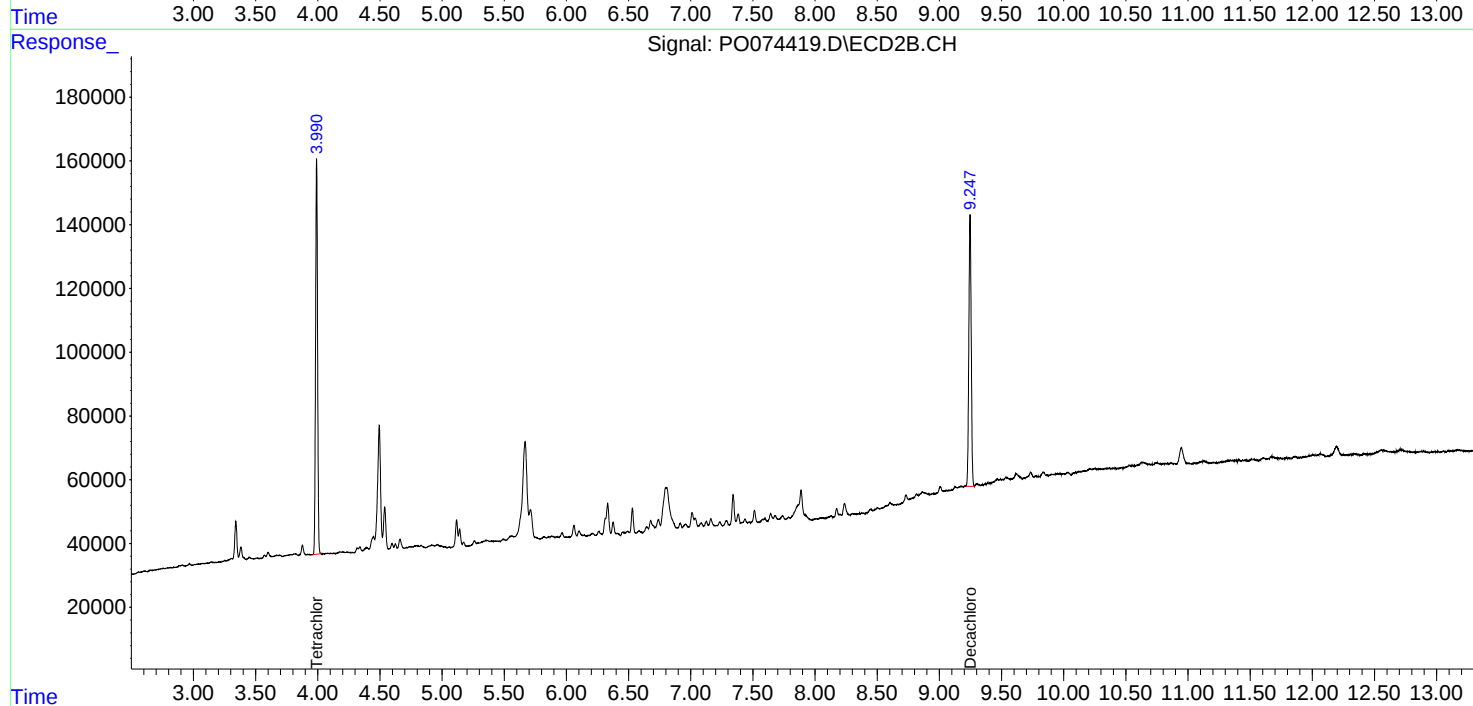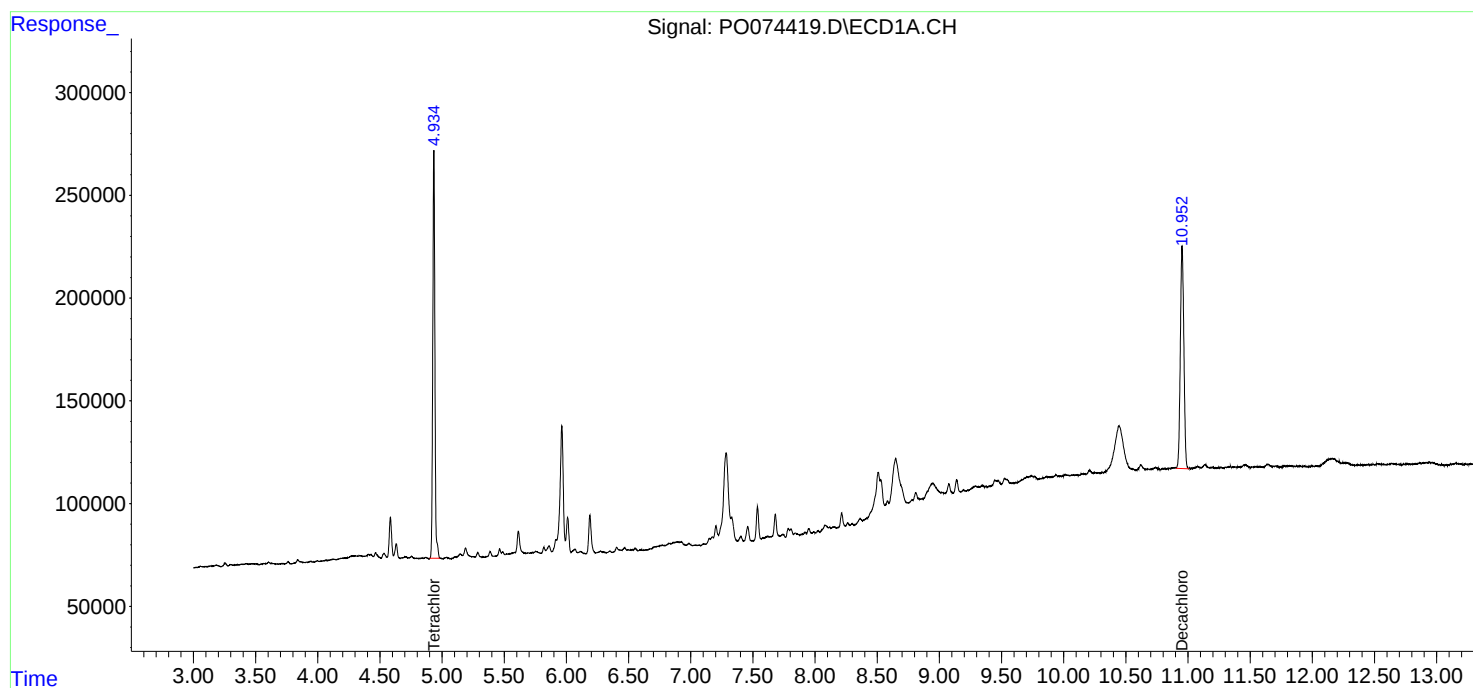

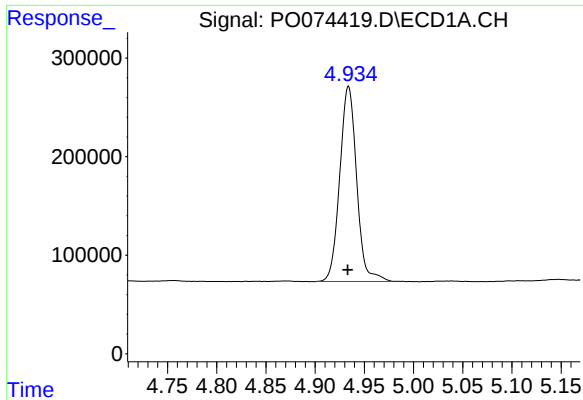


#1 Tetrachloro-m-xylene

R.T.: 4.934 min
Delta R.T.: 0.000 min
Response: 2366514
Conc: 24.63 ng/ml m

Instrument :
ECD_O
ClientSampleId :
20410


Manual Integrations
APPROVED

Ankita
1/8/2021 10:10:59 AM

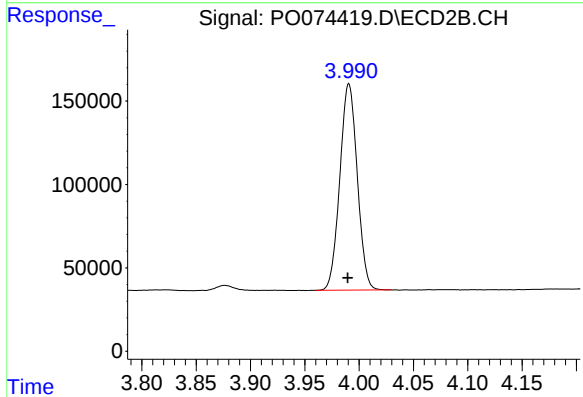


#1 Tetrachloro-m-xylene

R.T.: 3.991 min
Delta R.T.: 0.000 min
Response: 1381636
Conc: 25.94 ng/ml

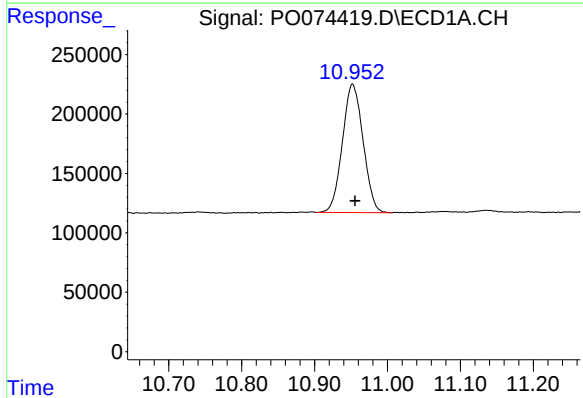

#2 Decachlorobiphenyl

R.T.: 10.952 min
Delta R.T.: -0.004 min
Response: 2126892
Conc: 22.88 ng/ml

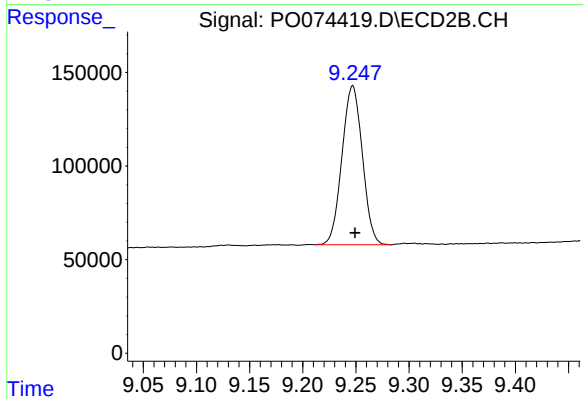

#2 Decachlorobiphenyl

R.T.: 9.247 min
Delta R.T.: -0.002 min
Response: 1135432
Conc: 21.81 ng/ml