

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010721\
 Data File : P0074421.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2021 13:06
 Operator : DD\AJ
 Sample : M1021-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-010621

Manual Integrations
 APPROVED

Ankita
 1/8/2021 10:11:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 16:24:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 05:03:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.933	3.991	2241232	1344099	23.325m	25.233
2) SA Decachlor...	10.953	9.247	2164481	1026880	23.283	19.726

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010721\
Data File : P0074421.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2021 13:06
Operator : DD\AJ
Sample : M1021-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-02-010621


Manual Integrations
APPROVED

Ankita
1/8/2021 10:11:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 16:24:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

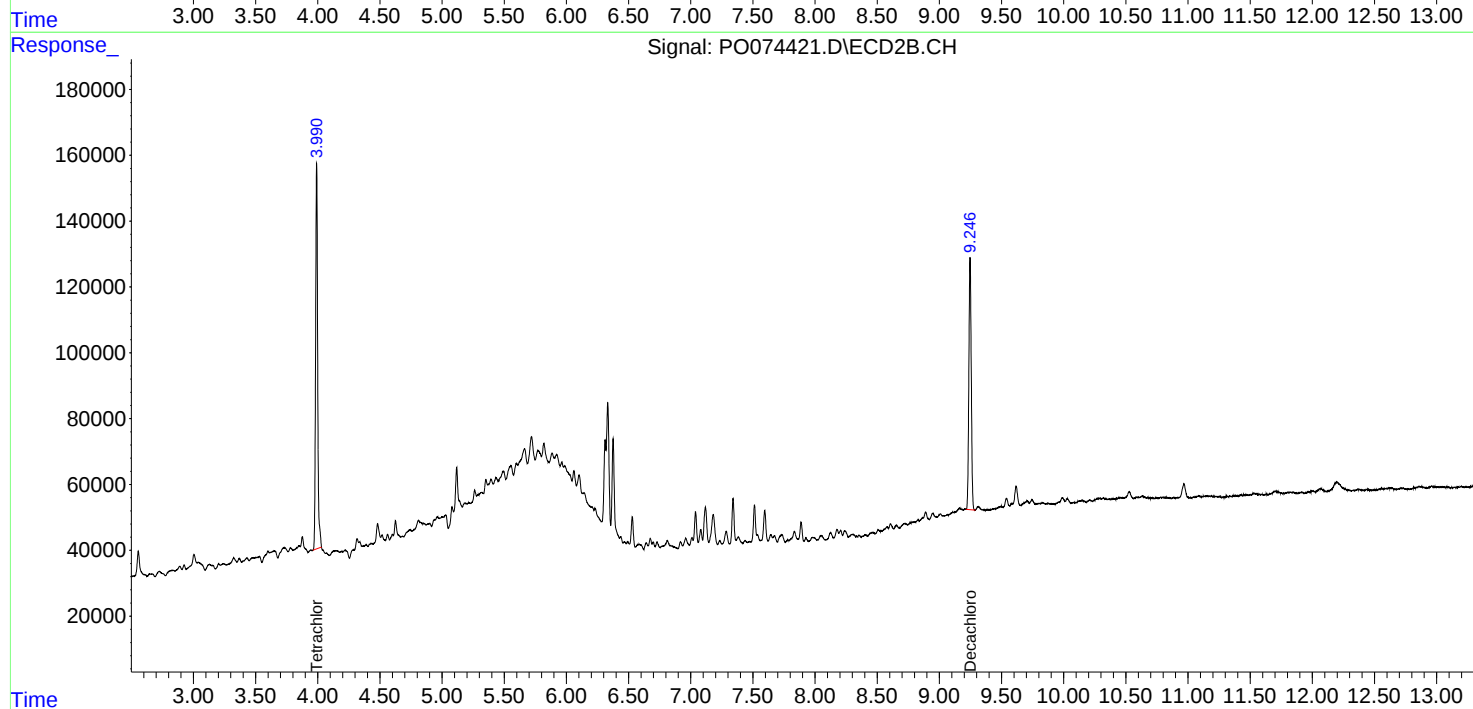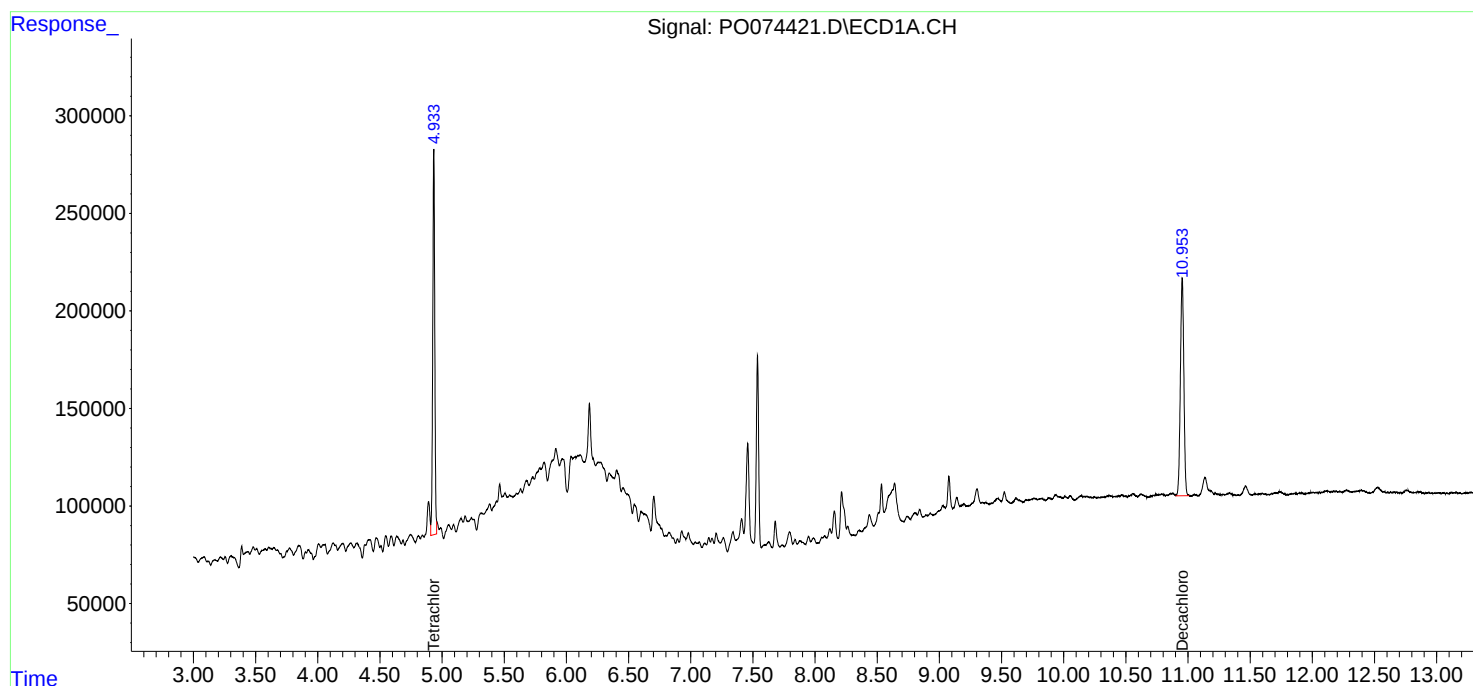

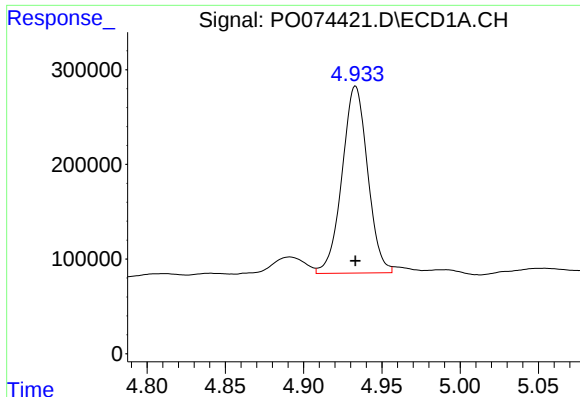


#1 Tetrachloro-m-xylene

R.T.: 4.933 min
Delta R.T.: 0.000 min
Response: 2241232
Conc: 23.32 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-02-010621


Manual Integrations
APPROVED

Ankita
1/8/2021 10:11:02 AM

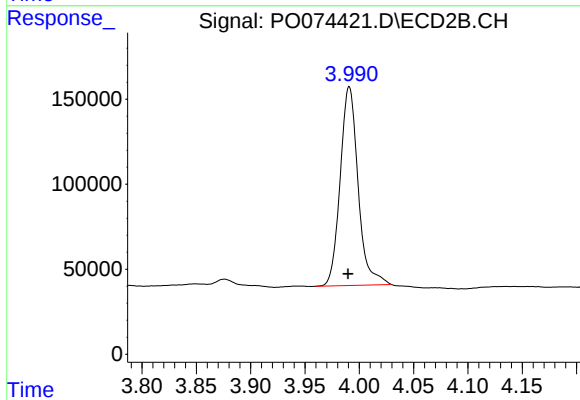


#1 Tetrachloro-m-xylene

R.T.: 3.991 min
Delta R.T.: 0.001 min
Response: 1344099
Conc: 25.23 ng/ml

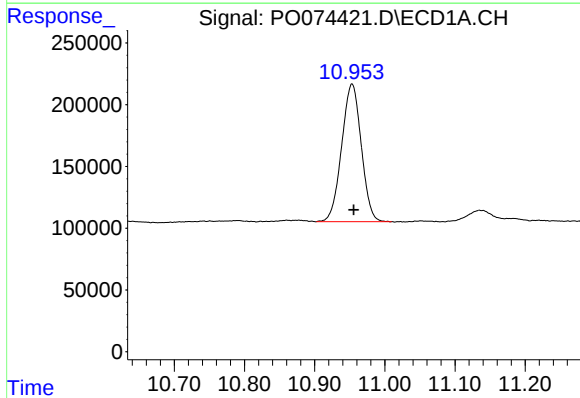

#2 Decachlorobiphenyl

R.T.: 10.953 min
Delta R.T.: -0.002 min
Response: 2164481
Conc: 23.28 ng/ml

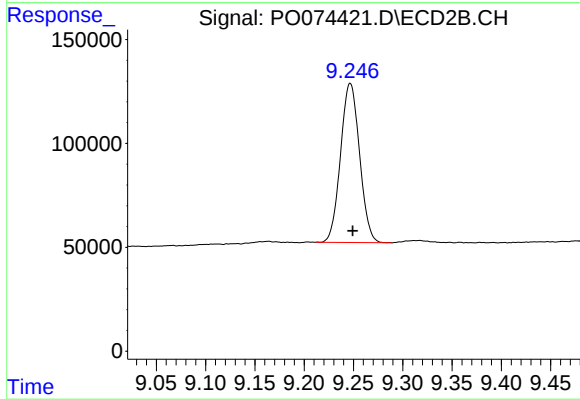

#2 Decachlorobiphenyl

R.T.: 9.247 min
Delta R.T.: -0.003 min
Response: 1026880
Conc: 19.73 ng/ml