

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0010721\
 Data File : P0074429.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2021 15:45
 Operator : DD\AJ
 Sample : M1022-02 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40967

Manual Integrations
 APPROVED

Ankita
 1/8/2021 10:11:09 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 16:27:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 05:03:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.933	3.989	180205	102908	1.875m	1.932
2) SA Decachlor...	10.961	9.254	237659	109166	2.556	2.097
Target Compounds						
26) L6 AR-1254-1	7.168	6.102	342507	251983	83.109	69.587
27) L6 AR-1254-2	7.399	6.261	527224	188644	81.038	59.650 #
28) L6 AR-1254-3	7.781	6.678	448964	303144	67.920	60.414
29) L6 AR-1254-4	8.079	6.918	491799	269043	86.436	73.660
30) L6 AR-1254-5	8.509	7.345	529004	402252	97.763	85.357

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010721\
Data File : PO074429.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2021 15:45
Operator : DD\AJ
Sample : M1022-02 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
40967


Manual Integrations
APPROVED

Ankita
1/8/2021 10:11:09 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 16:27:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

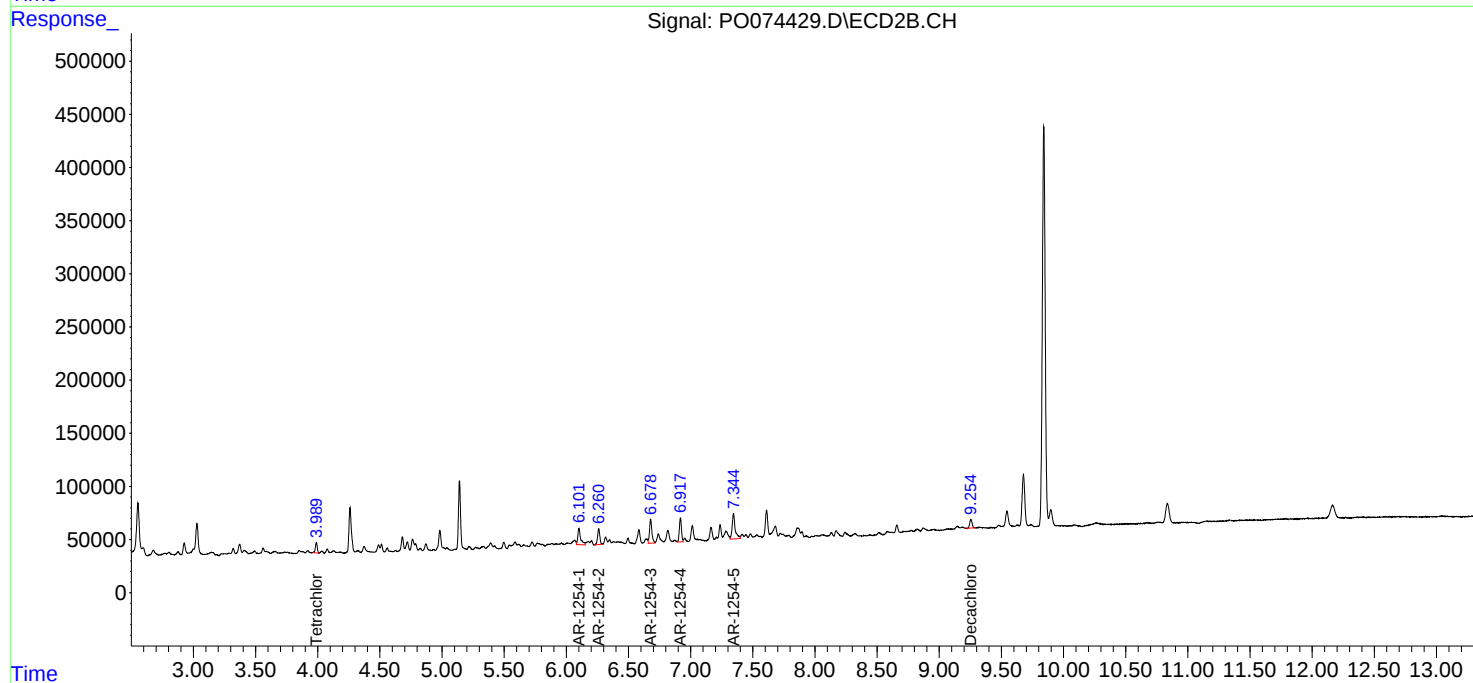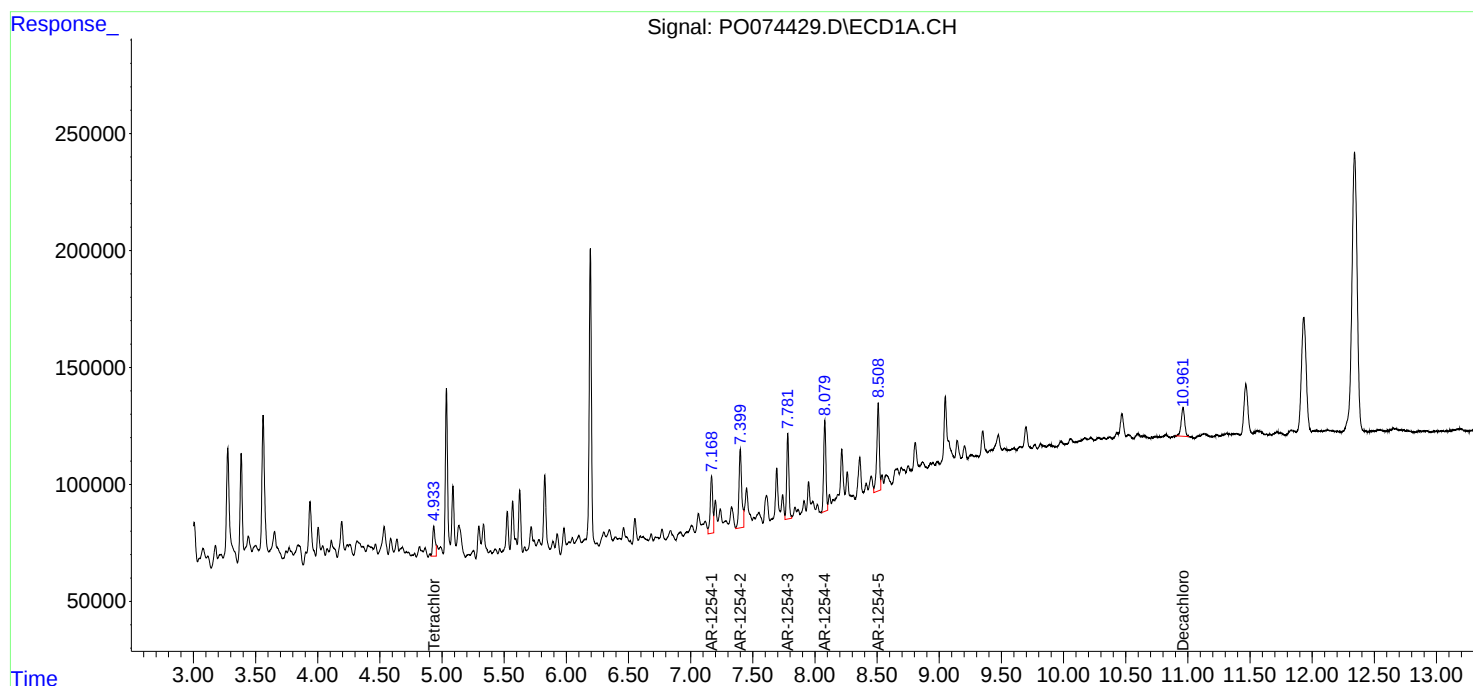

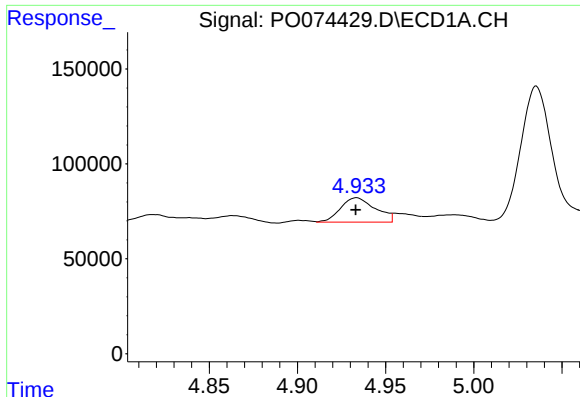


#1 Tetrachloro-m-xylene

R.T.: 4.933 min
Delta R.T.: 0.000 min
Response: 180205
Conc: 1.88 ng/ml m

Instrument :
ECD_O
ClientSampleId :
40967


Manual Integrations
APPROVED

Ankita
1/8/2021 10:11:09 AM

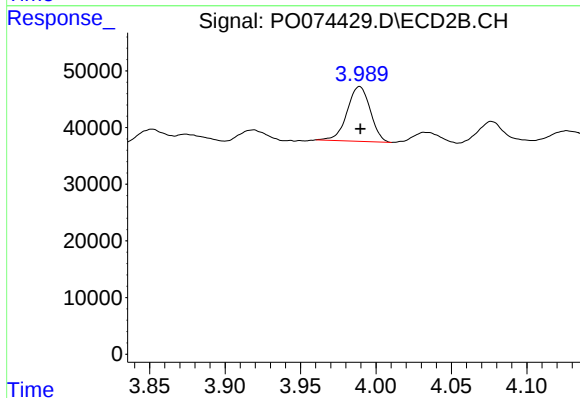


#1 Tetrachloro-m-xylene

R.T.: 3.989 min
Delta R.T.: 0.000 min
Response: 102908
Conc: 1.93 ng/ml

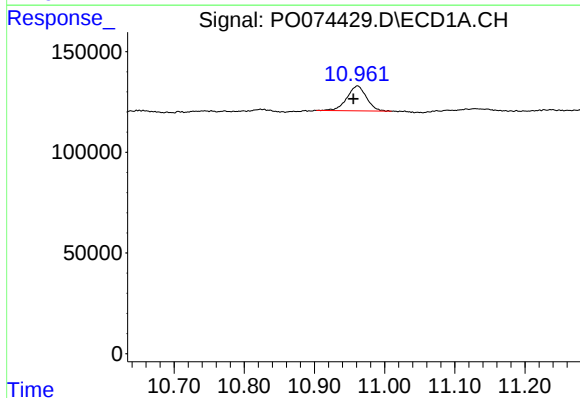


#2 Decachlorobiphenyl

R.T.: 10.961 min
Delta R.T.: 0.006 min
Response: 237659
Conc: 2.56 ng/ml

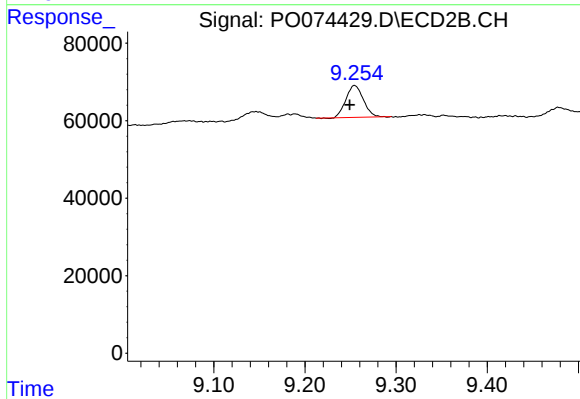

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: 0.005 min
Response: 109166
Conc: 2.10 ng/ml

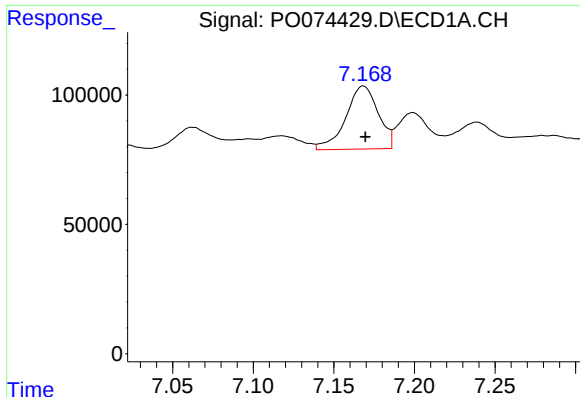


#26 AR-1254-1

R.T.: 7.168 min
Delta R.T.: -0.001 min
Response: 342507
Conc: 83.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
40967


Manual Integrations
APPROVED

Ankita
1/8/2021 10:11:09 AM

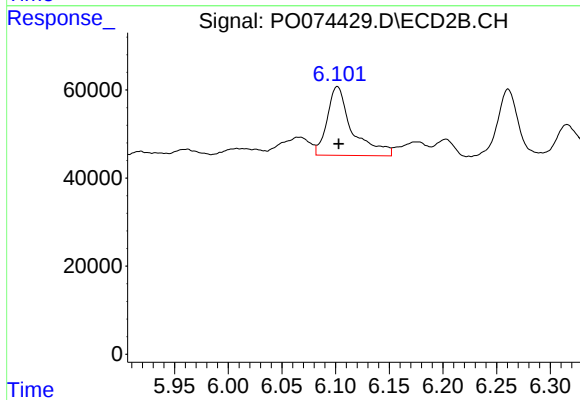


#26 AR-1254-1

R.T.: 6.102 min
Delta R.T.: -0.001 min
Response: 251983
Conc: 69.59 ng/ml

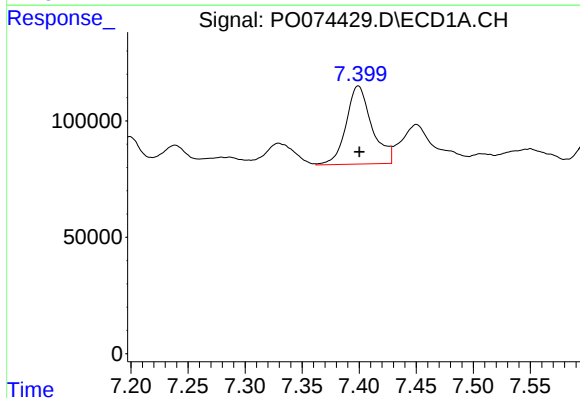


#27 AR-1254-2

R.T.: 7.399 min
Delta R.T.: 0.000 min
Response: 527224
Conc: 81.04 ng/ml

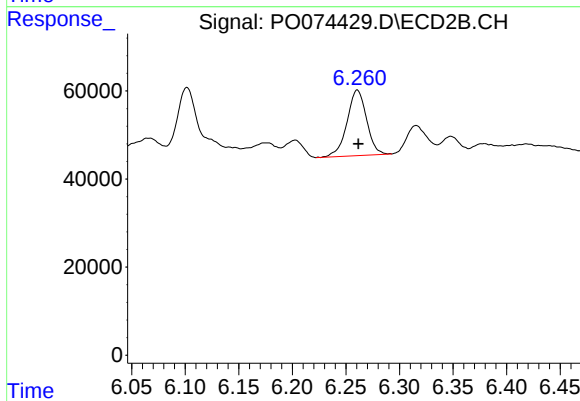

#27 AR-1254-2

R.T.: 6.261 min
Delta R.T.: -0.001 min
Response: 188644
Conc: 59.65 ng/ml

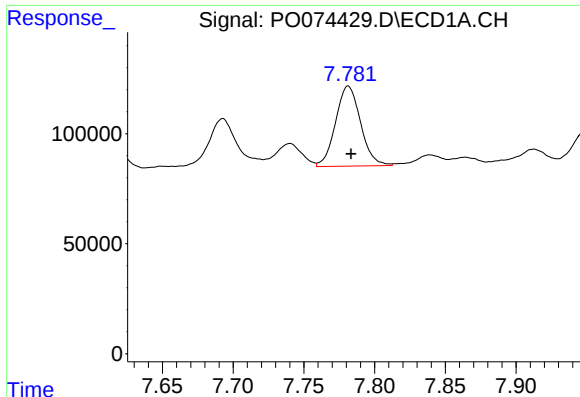


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: -0.002 min
Response: 448964
Conc: 67.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
40967


Manual Integrations
APPROVED

Ankita
1/8/2021 10:11:09 AM

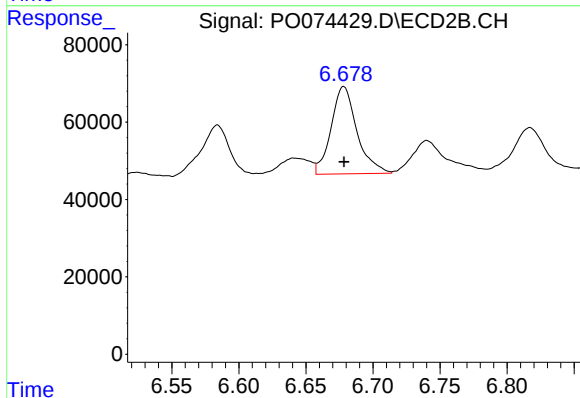


#28 AR-1254-3

R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 303144
Conc: 60.41 ng/ml

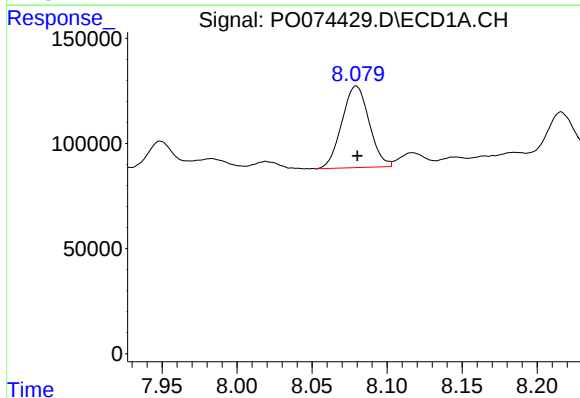


#29 AR-1254-4

R.T.: 8.079 min
Delta R.T.: 0.000 min
Response: 491799
Conc: 86.44 ng/ml

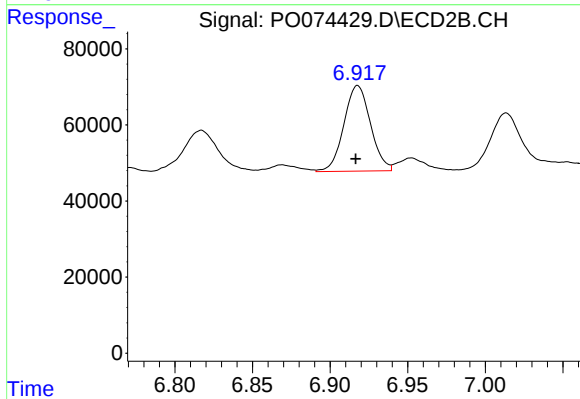

#29 AR-1254-4

R.T.: 6.918 min
Delta R.T.: 0.001 min
Response: 269043
Conc: 73.66 ng/ml

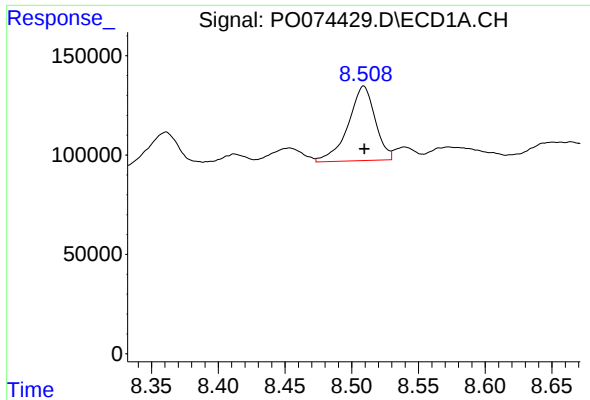


#30 AR-1254-5

R.T.: 8.509 min
Delta R.T.: 0.000 min
Response: 529004
Conc: 97.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
40967

Manual Integrations
APPROVED

Ankita
1/8/2021 10:11:09 AM

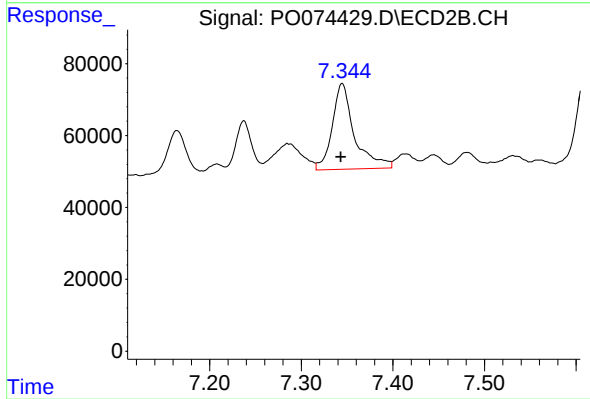

#30 AR-1254-5

R.T.: 7.345 min
Delta R.T.: 0.002 min
Response: 402252
Conc: 85.36 ng/ml