

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0010722\
 Data File : P0084076.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jan 2022 15:23
 Operator : AJ\MA
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AR1254ICC050

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
 Supervised By :mohammad ahmed 01/10/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 10:57:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0010722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 10 10:56:03 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.046	4.037	558053	101436	5.644	4.722
2) SA Decachlor...	11.249	9.448	377125	103708	5.538	4.992
Target Compounds						
26) L6 AR-1254-1	7.293	6.210	205256	63391	59.502	52.178
27) L6 AR-1254-2	7.526	6.371	312841	58858	59.094m	54.944
28) L6 AR-1254-3	7.909	6.799	332679	93575	59.014m	54.305
29) L6 AR-1254-4	8.208	7.042	236764	58382	57.872m	53.379
30) L6 AR-1254-5	8.644	7.479	259723	79906	61.743	52.827

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010722\
Data File : PO084076.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jan 2022 15:23
Operator : AJ\MA
Sample : AR1254ICC050
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 10:57:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 10 10:56:03 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

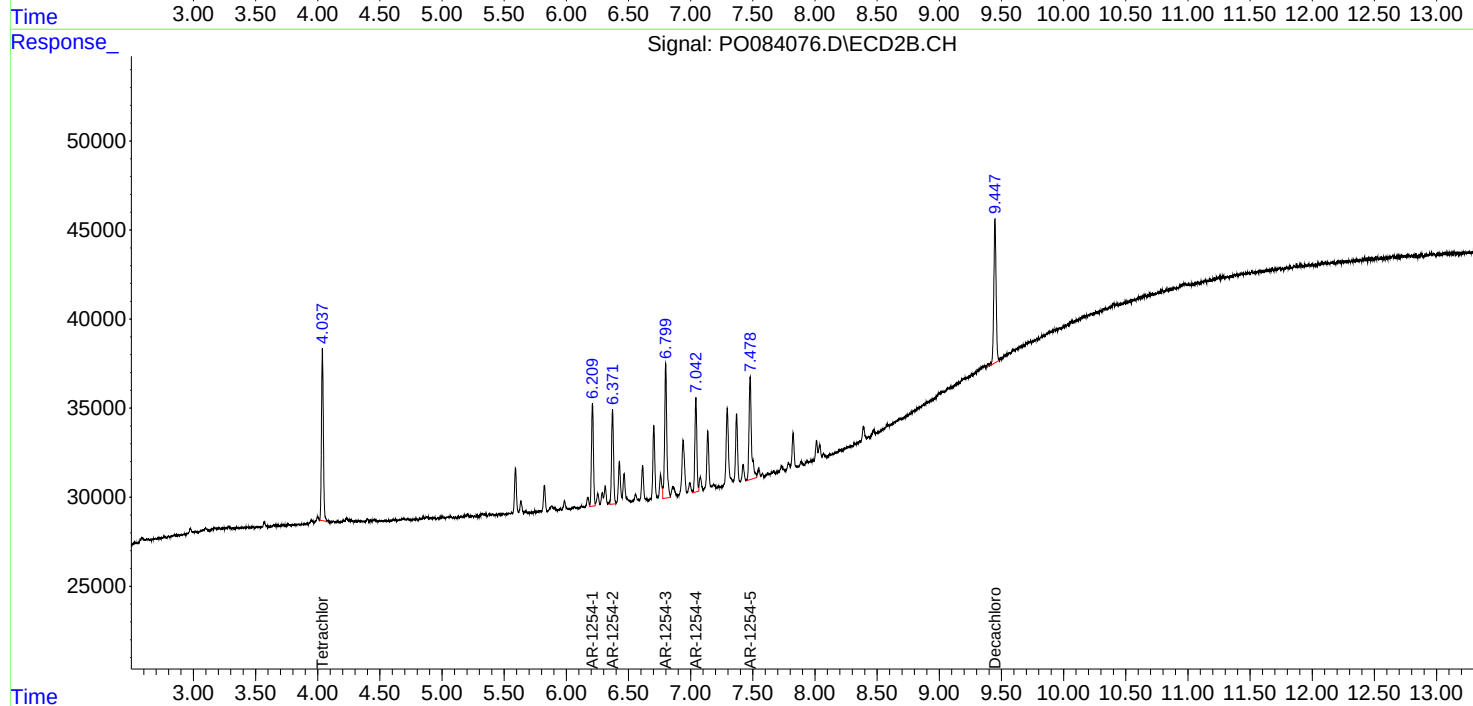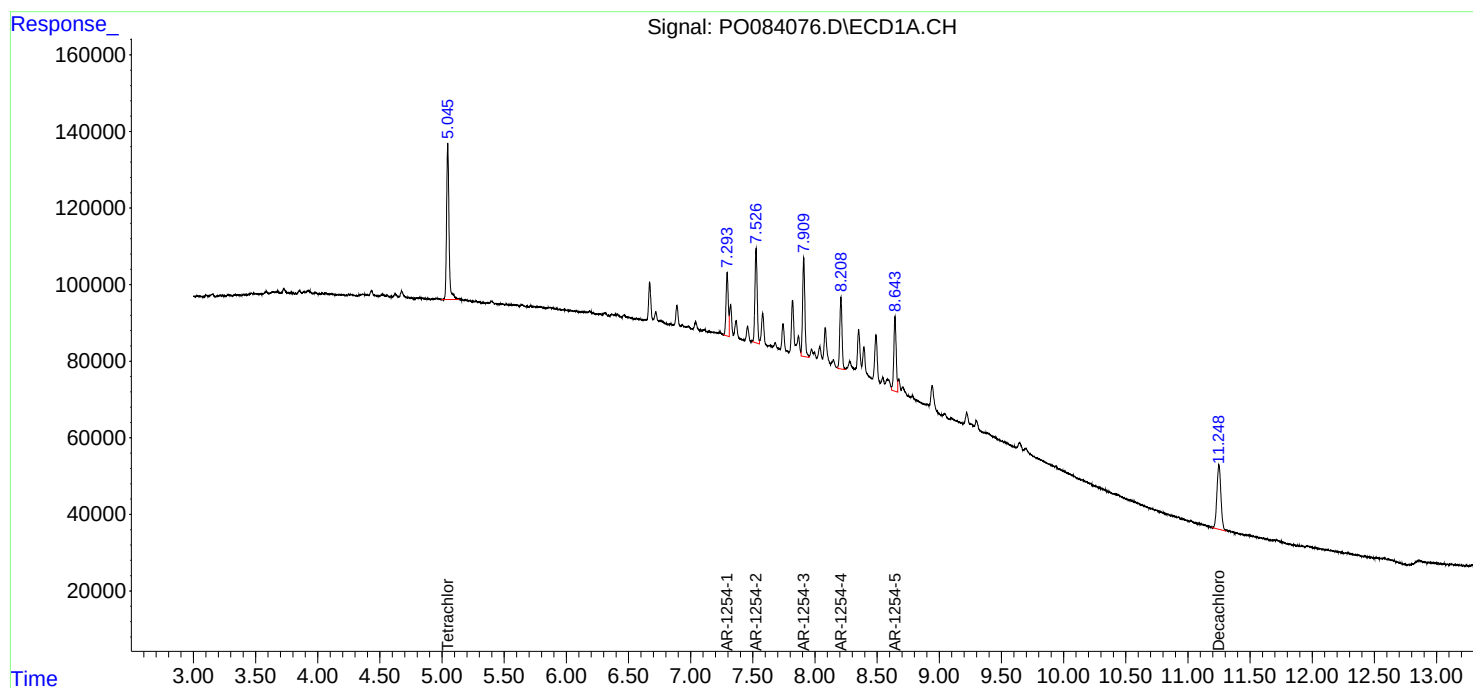

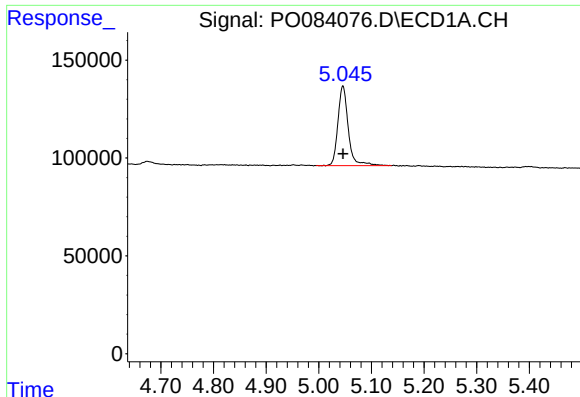


#1 Tetrachloro-m-xylene

R.T.: 5.046 min
Delta R.T.: 0.000 min
Response: 558053
Conc: 5.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

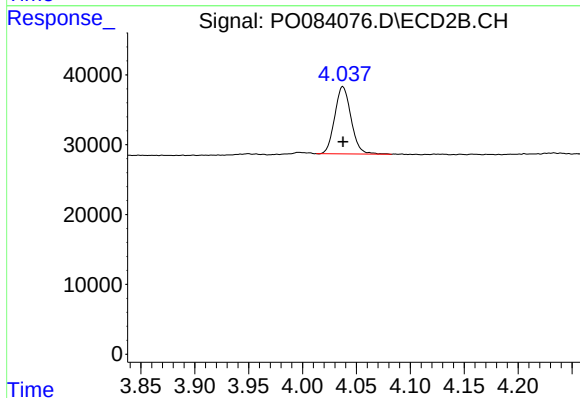


#1 Tetrachloro-m-xylene

R.T.: 4.037 min
Delta R.T.: 0.000 min
Response: 101436
Conc: 4.72 ng/ml

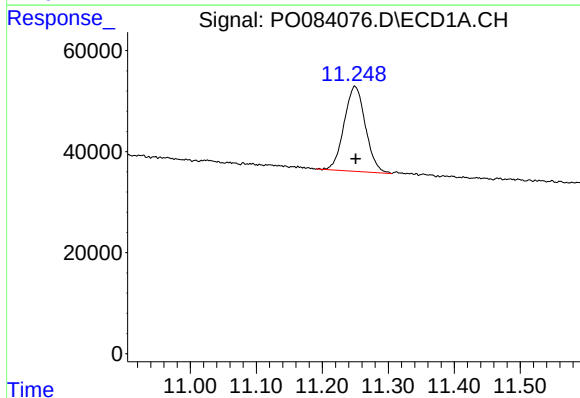


#2 Decachlorobiphenyl

R.T.: 11.249 min
Delta R.T.: -0.002 min
Response: 377125
Conc: 5.54 ng/ml

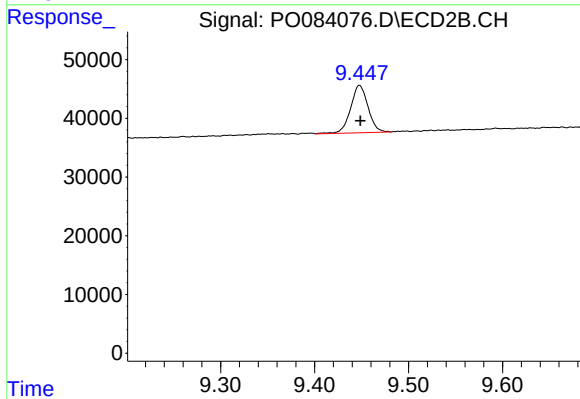

#2 Decachlorobiphenyl

R.T.: 9.448 min
Delta R.T.: 0.000 min
Response: 103708
Conc: 4.99 ng/ml

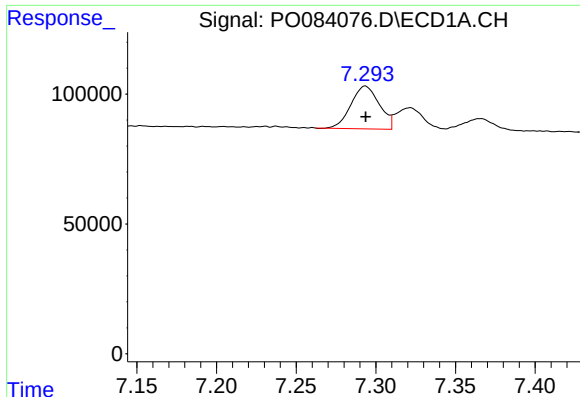


#26 AR-1254-1

R.T.: 7.293 min
Delta R.T.: 0.000 min
Response: 205256
Conc: 59.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

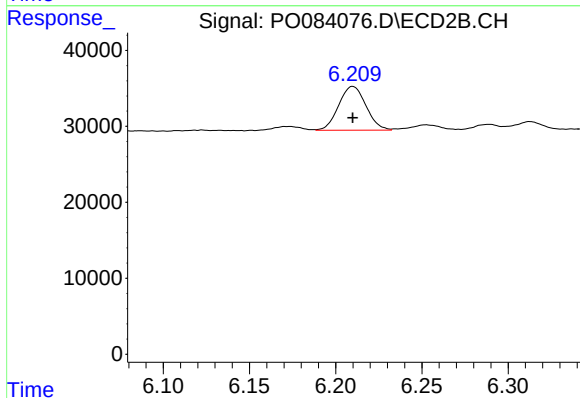


#26 AR-1254-1

R.T.: 6.210 min
Delta R.T.: 0.000 min
Response: 63391
Conc: 52.18 ng/ml

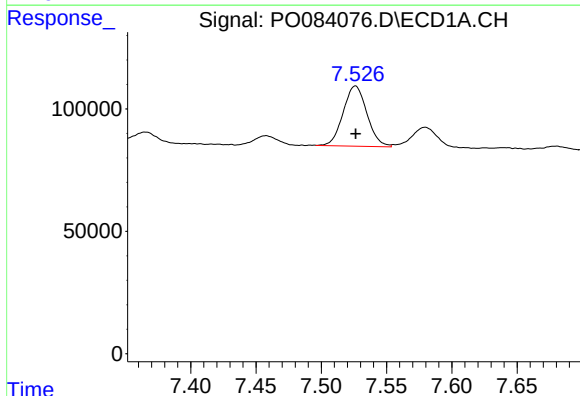


#27 AR-1254-2

R.T.: 7.526 min
Delta R.T.: 0.000 min
Response: 312841
Conc: 59.09 ng/ml m

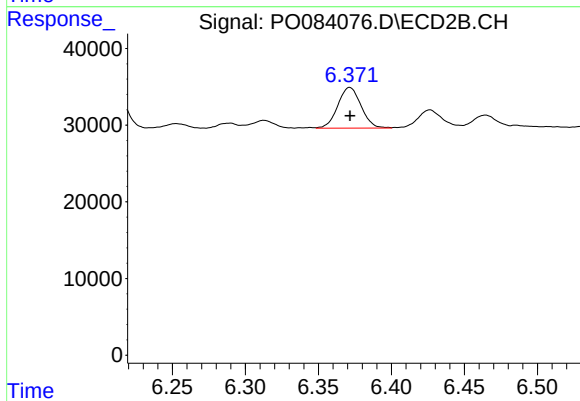

#27 AR-1254-2

R.T.: 6.371 min
Delta R.T.: 0.000 min
Response: 58858
Conc: 54.94 ng/ml

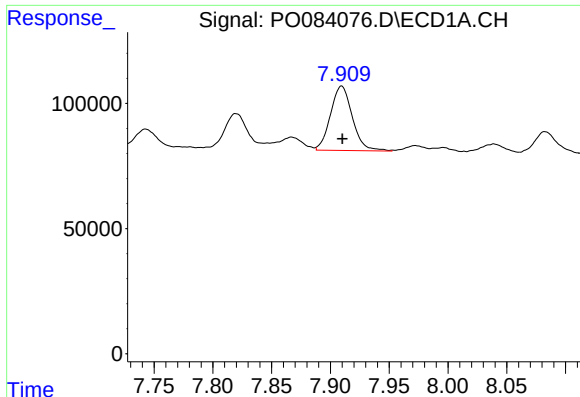


#28 AR-1254-3

R.T.: 7.909 min
Delta R.T.: -0.001 min
Response: 332679
Conc: 59.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

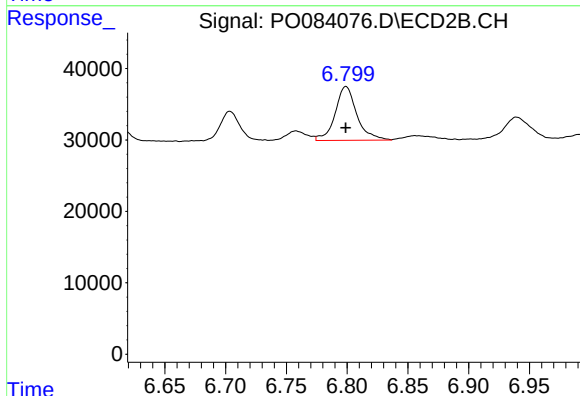


#28 AR-1254-3

R.T.: 6.799 min
Delta R.T.: 0.000 min
Response: 93575
Conc: 54.31 ng/ml

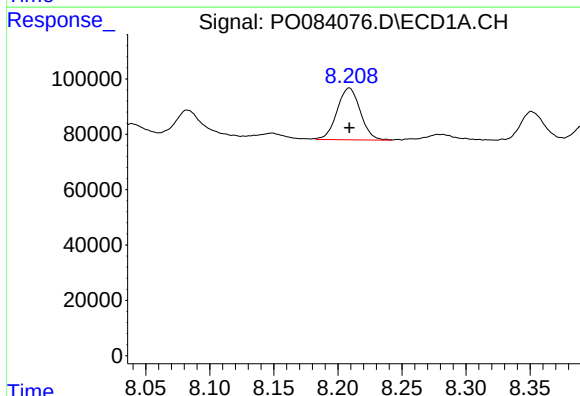


#29 AR-1254-4

R.T.: 8.208 min
Delta R.T.: 0.000 min
Response: 236764
Conc: 57.87 ng/ml m

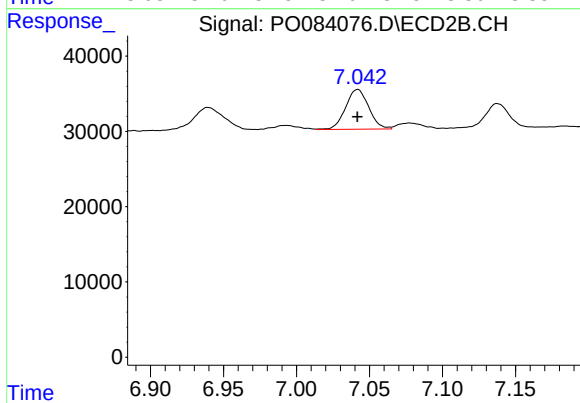

#29 AR-1254-4

R.T.: 7.042 min
Delta R.T.: 0.000 min
Response: 58382
Conc: 53.38 ng/ml

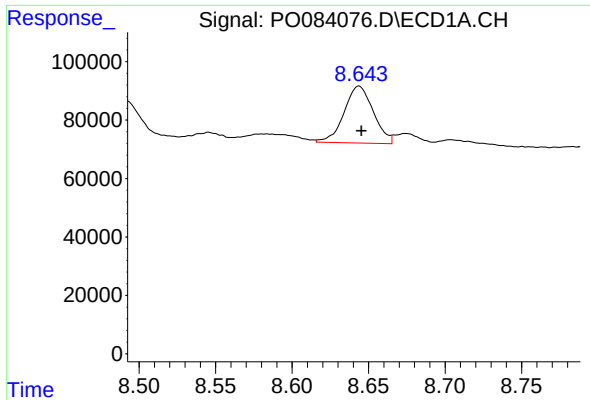


#30 AR-1254-5

R.T.: 8.644 min
Delta R.T.: -0.002 min
Response: 259723
Conc: 61.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/10/2022
Supervised By :mohammad ahmed 01/10/2022

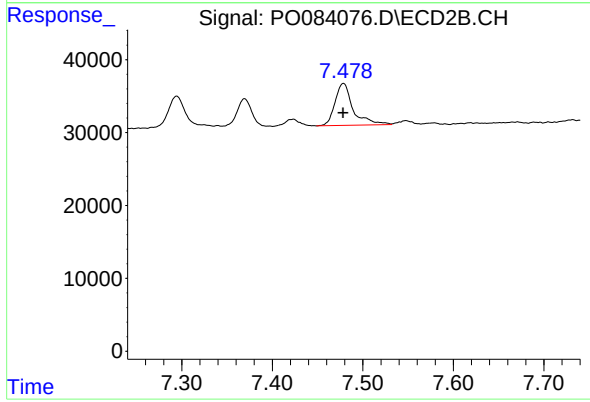

#30 AR-1254-5

R.T.: 7.479 min
Delta R.T.: 0.000 min
Response: 79906
Conc: 52.83 ng/ml