

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010725\
 Data File : P0108946.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2025 09:47
 Operator : YP/AJ
 Sample : Q1009-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SU-03-1-03-2025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/08/2025
 Supervised By :Ankita Jodhani 01/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 12:02:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010225.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 03 04:48:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.701	3.698	145.5E6	95175130	15.711m	17.166m
2) SA Decachlor...	8.767	8.718	108.8E6	53450916	15.324	14.243

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010725\
Data File : PO108946.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2025 09:47
Operator : YP/AJ
Sample : Q1009-01
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SU-03-1-03-2025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2025
Supervised By :Ankita Jodhani 01/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 12:02:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010225.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 03 04:48:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

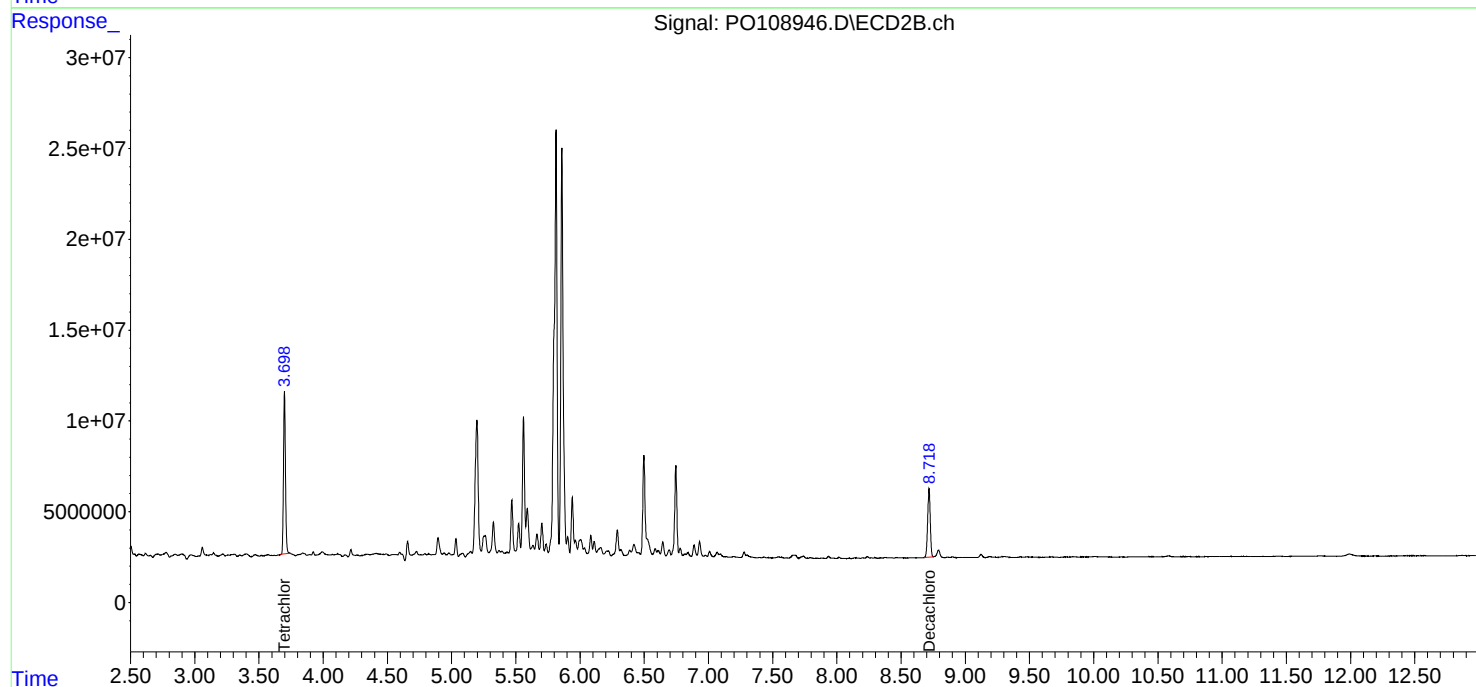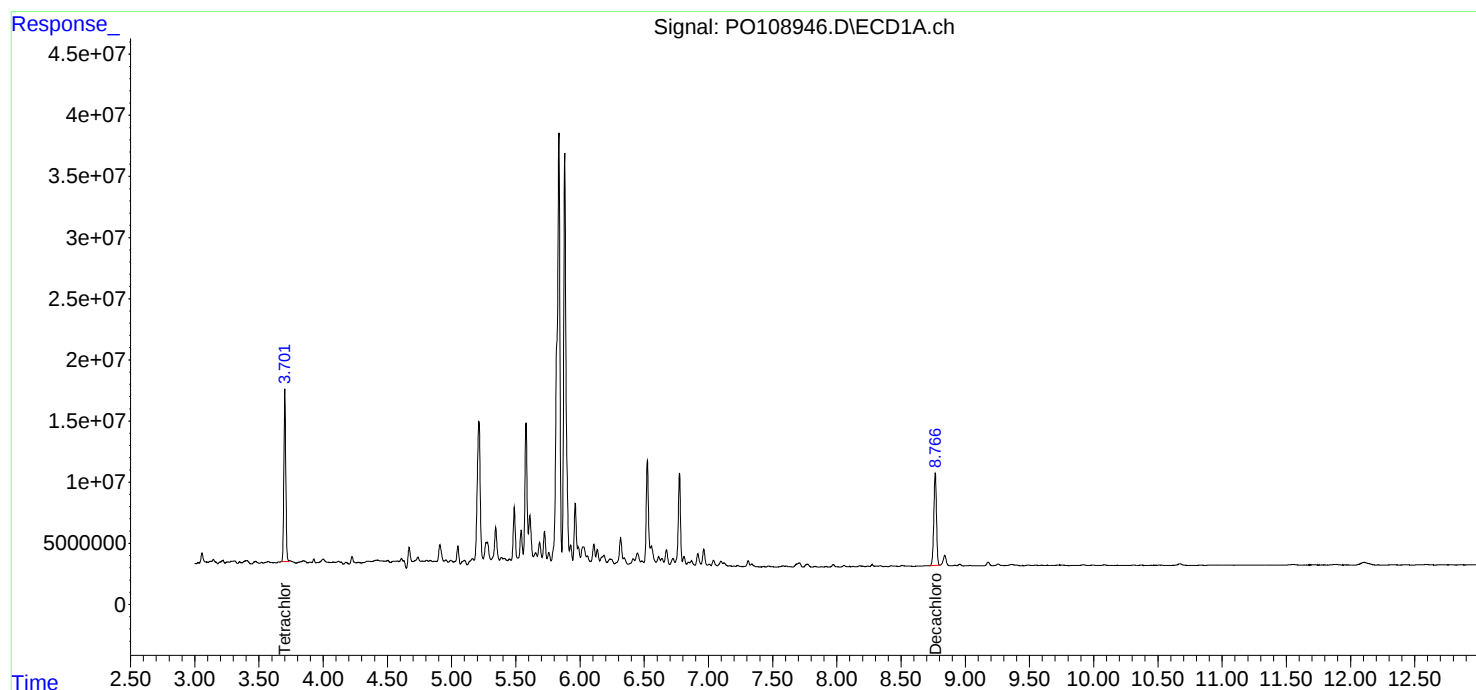

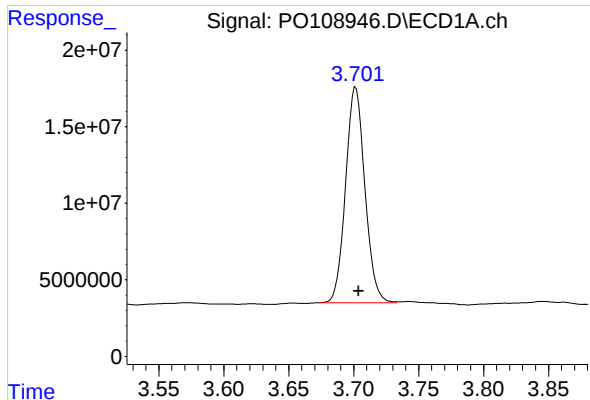


#1 Tetrachloro-m-xylene

R.T.: 3.701 min
Delta R.T.: -0.003 min
Response: 145532021
Conc: 15.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
SU-03-1-03-2025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2025
Supervised By :Ankita Jodhani 01/08/2025

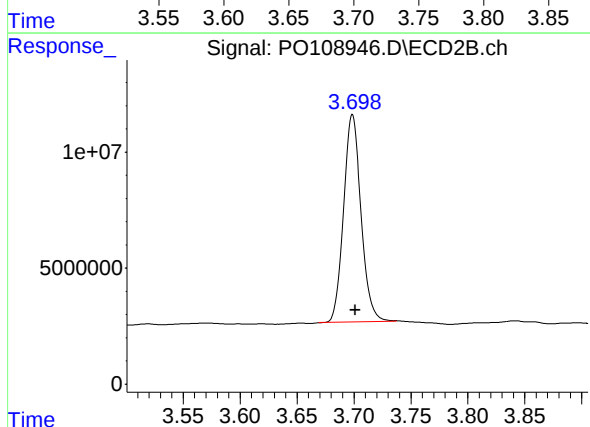


#1 Tetrachloro-m-xylene

R.T.: 3.698 min
Delta R.T.: -0.003 min
Response: 95175130
Conc: 17.17 ng/ml

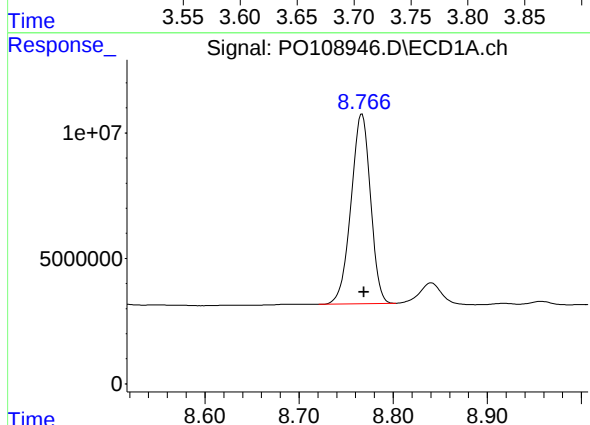

#2 Decachlorobiphenyl

R.T.: 8.767 min
Delta R.T.: -0.002 min
Response: 108793309
Conc: 15.32 ng/ml

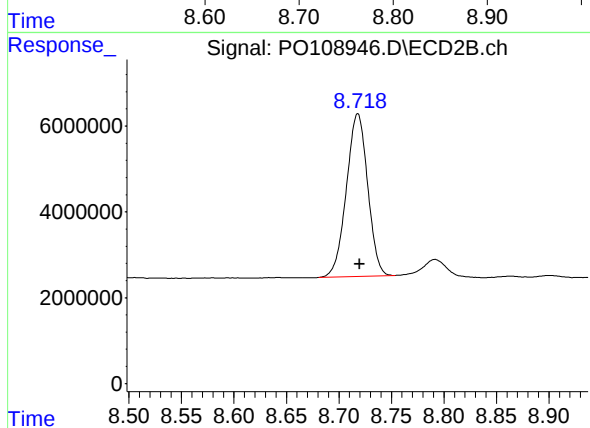

#2 Decachlorobiphenyl

R.T.: 8.718 min
Delta R.T.: -0.002 min
Response: 53450916
Conc: 14.24 ng/ml