

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010725\
 Data File : P0108955.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2025 17:56
 Operator : YP/AJ
 Sample : Q1016-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 275

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/08/2025
 Supervised By :Ankita Jodhani 01/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 00:30:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010225.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jan 03 04:48:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.704	3.701	91696929	62362724	9.899	11.248
2) SA Decachlor...	8.766	8.718	44918626	21736373	6.327m	5.792m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010725\
Data File : PO108955.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2025 17:56
Operator : YP/AJ
Sample : Q1016-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
275


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2025
Supervised By :Ankita Jodhani 01/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 00:30:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010225.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jan 03 04:48:29 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

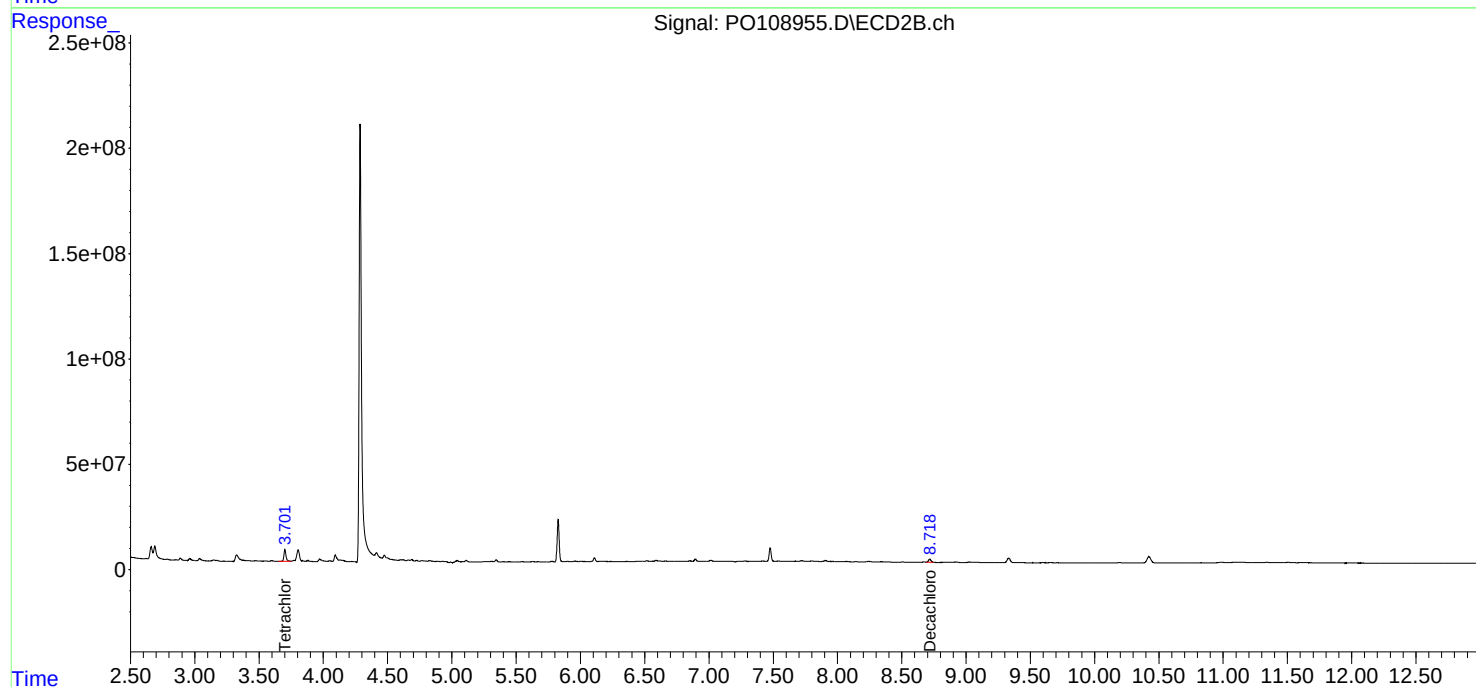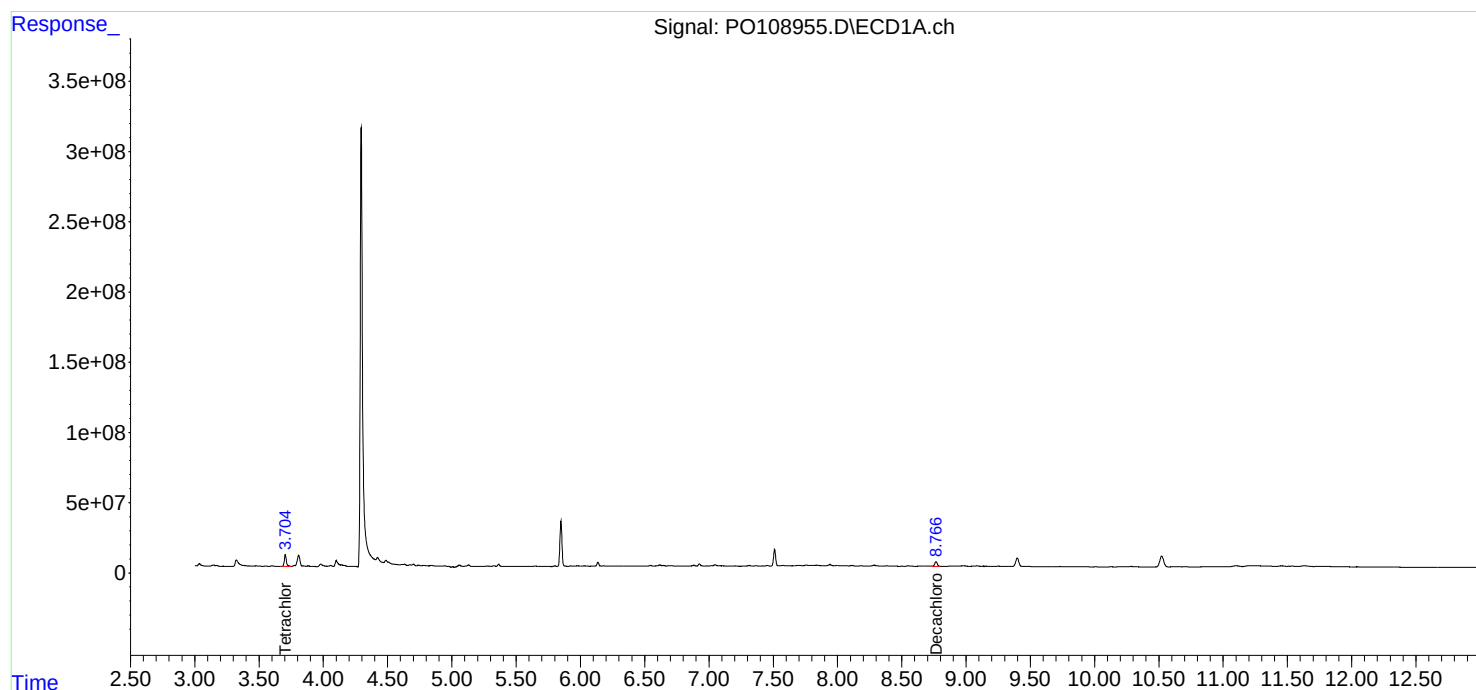

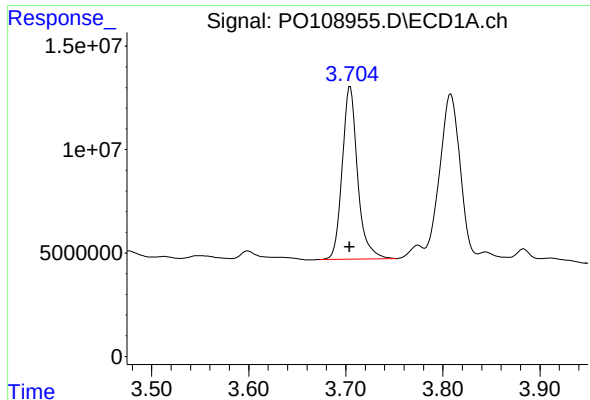


#1 Tetrachloro-m-xylene

R.T.: 3.704 min
Delta R.T.: 0.000 min
Response: 91696929
Conc: 9.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
275

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/08/2025
Supervised By :Ankita Jodhani 01/08/2025

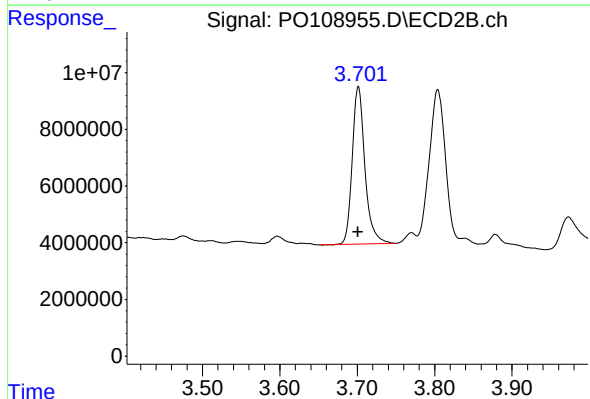

#1 Tetrachloro-m-xylene

R.T.: 3.701 min
Delta R.T.: 0.000 min
Response: 62362724
Conc: 11.25 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: -0.003 min
Response: 44918626
Conc: 6.33 ng/ml m

#2 Decachlorobiphenyl

R.T.: 8.718 min
Delta R.T.: -0.002 min
Response: 21736373
Conc: 5.79 ng/ml m