

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010820\
 Data File : P0065381.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jan 2020 17:09
 Operator : AJ/MA
 Sample : L1048-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FRONT-PIER-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 00:44:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.168	3.442	377515	426949	20.674	19.409
2) SA Decachlor...	9.680	8.351	728523	811089	21.501	19.558

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010820\
Data File : P0065381.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2020 17:09
Operator : AJ/MA
Sample : L1048-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FRONT-PIER-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 00:44:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

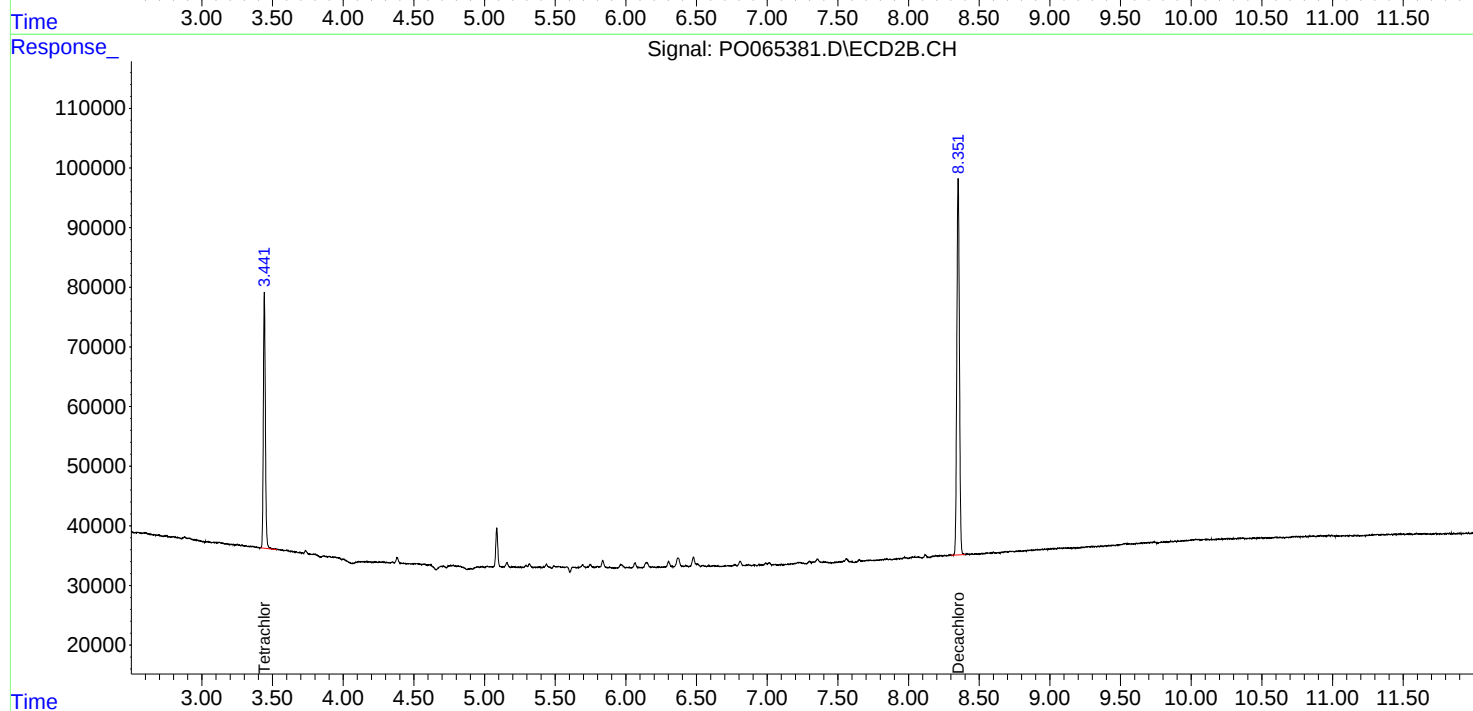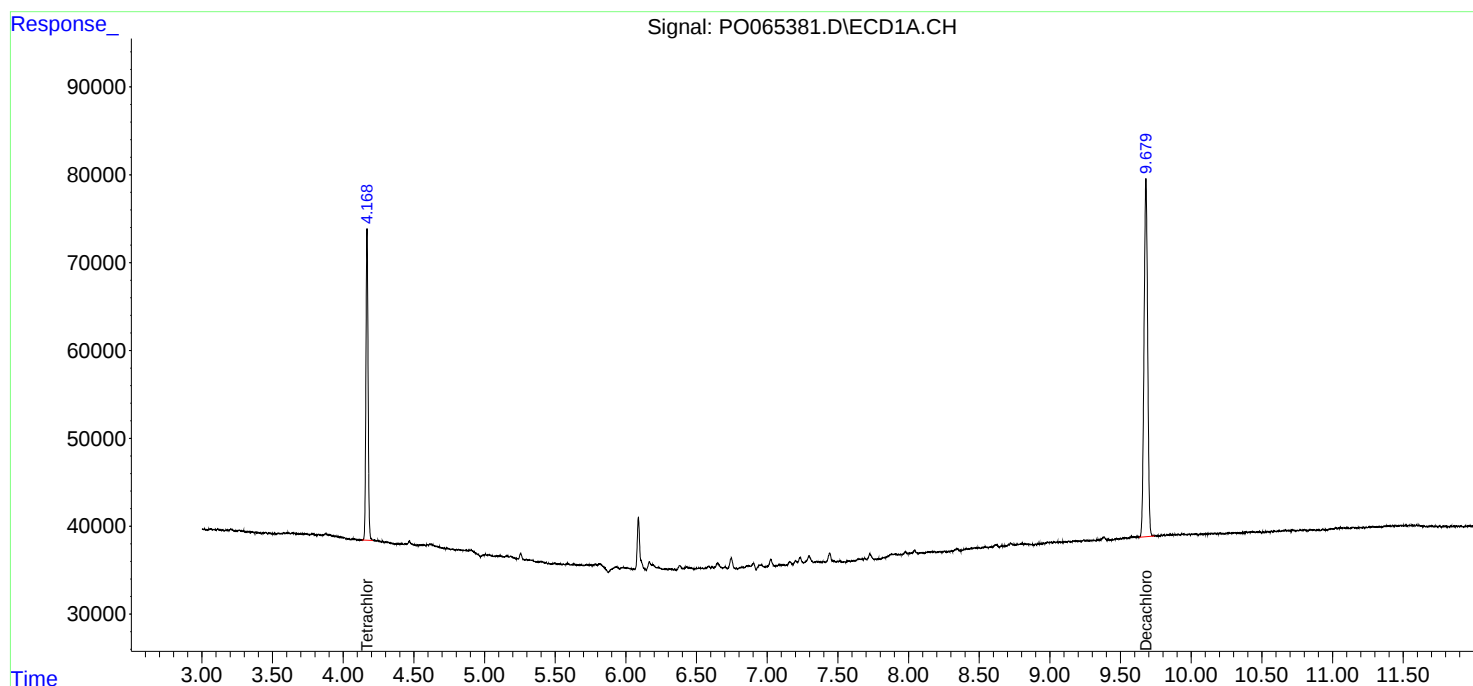


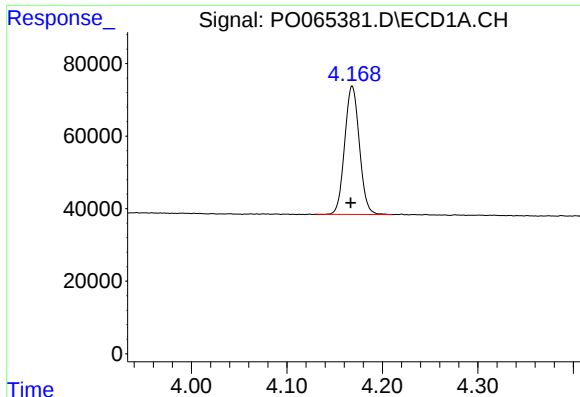

#1 Tetrachloro-m-xylene


R.T.: 4.168 min
Delta R.T.: 0.001 min
Response: 377515
Conc: 20.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
FRONT-PIER-A

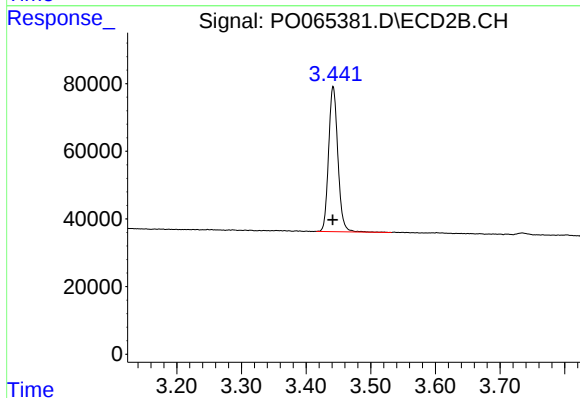


#1 Tetrachloro-m-xylene

R.T.: 3.442 min
Delta R.T.: 0.000 min
Response: 426949
Conc: 19.41 ng/ml

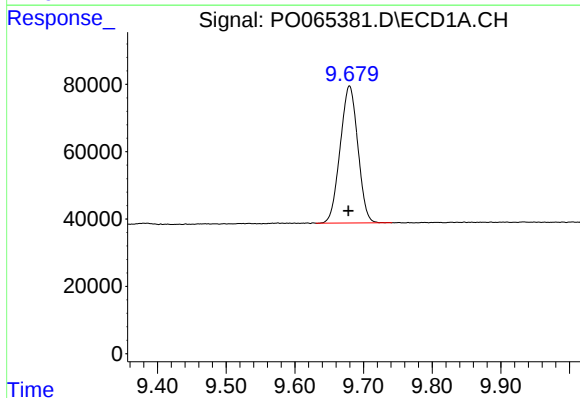

#2 Decachlorobiphenyl

R.T.: 9.680 min
Delta R.T.: 0.001 min
Response: 728523
Conc: 21.50 ng/ml

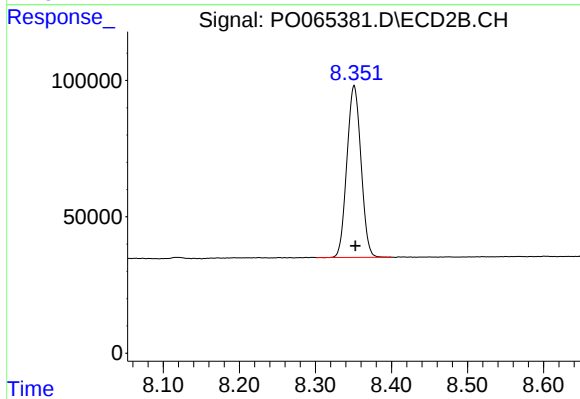

#2 Decachlorobiphenyl

R.T.: 8.351 min
Delta R.T.: -0.002 min
Response: 811089
Conc: 19.56 ng/ml