

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0010821\
 Data File : P0074437.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jan 2021 9:25
 Operator : DD\AJ
 Sample : M1025-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HD-01-010621

Manual Integrations
 APPROVED

Ankita
 1/11/2021 11:12:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 16:18:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 05:03:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	3.990	2424448	1429380	25.232m	26.834
2) SA Decachlor...	10.951	9.245	2358148	1217948	25.366	23.396
Target Compounds						
26) L6 AR-1254-1	7.169	6.099	103280	53987	25.061m	14.909m#
27) L6 AR-1254-2	7.397	6.258	105558	65548	16.225m	20.727m#
28) L6 AR-1254-3	7.784	6.673	118762	95283	17.967m	18.989m
29) L6 AR-1254-4	8.077	6.913	147665	74598	25.953m	20.424m
30) L6 AR-1254-5	8.508	7.339	229173	136100	42.353	28.880 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010821\
Data File : PO074437.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2021 9:25
Operator : DD\AJ
Sample : M1025-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HD-01-010621


Manual Integrations
APPROVED

Ankita
1/11/2021 11:12:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 16:18:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

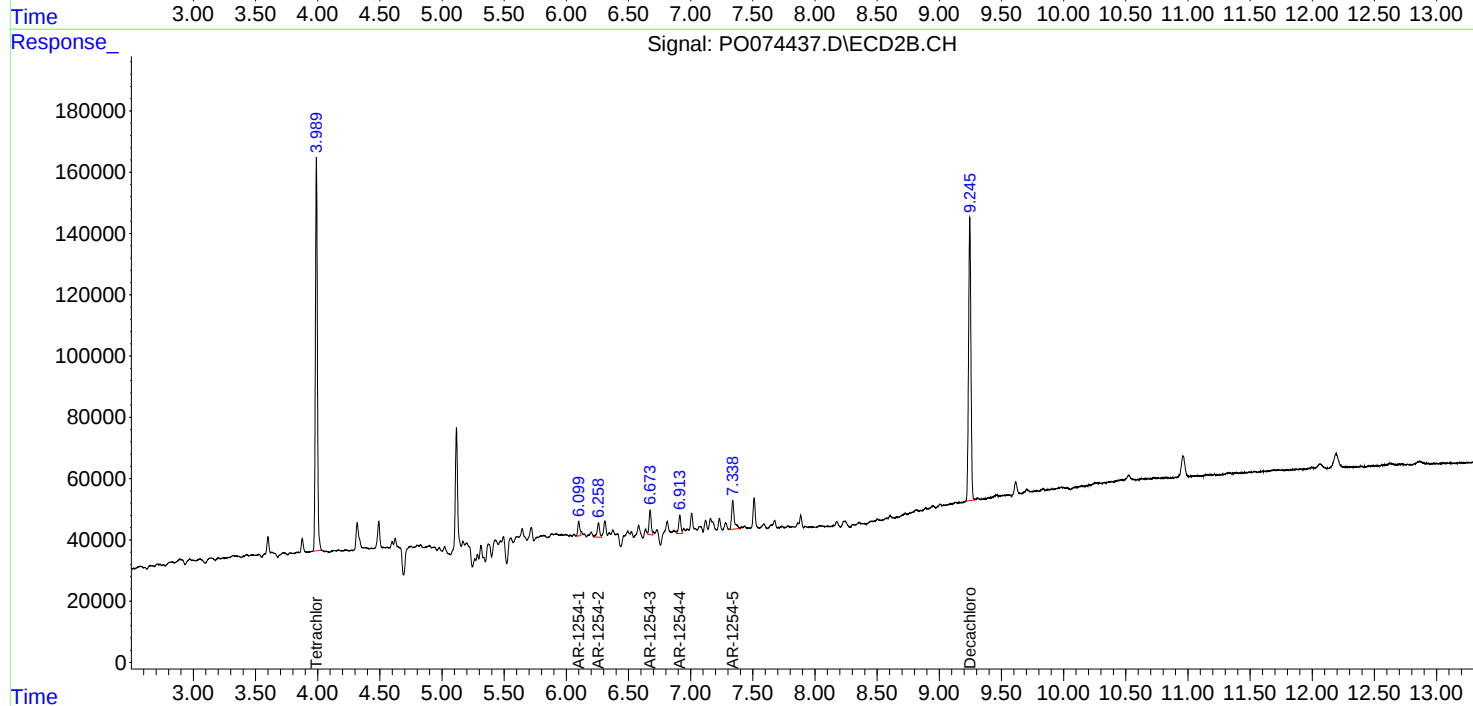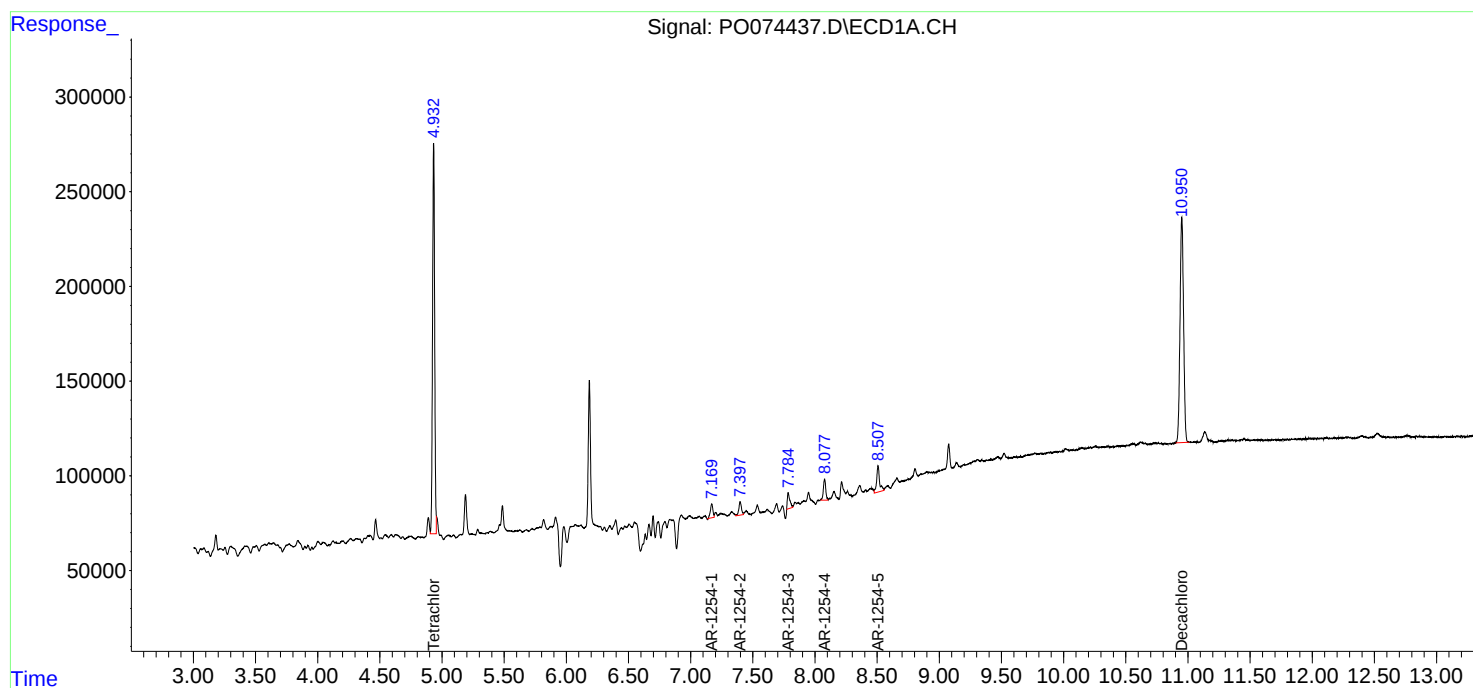

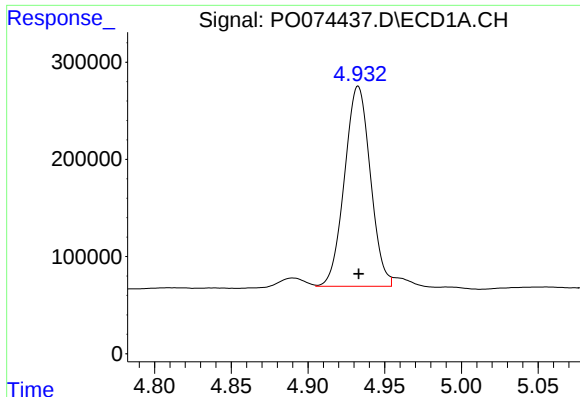


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 2424448
Conc: 25.23 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HD-01-010621


Manual Integrations
APPROVED

Ankita
1/11/2021 11:12:55 AM

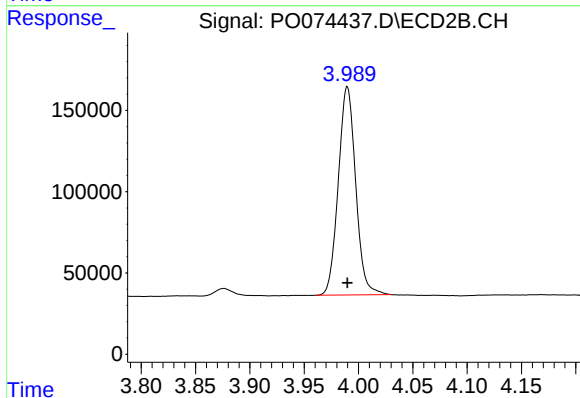


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: 0.000 min
Response: 1429380
Conc: 26.83 ng/ml

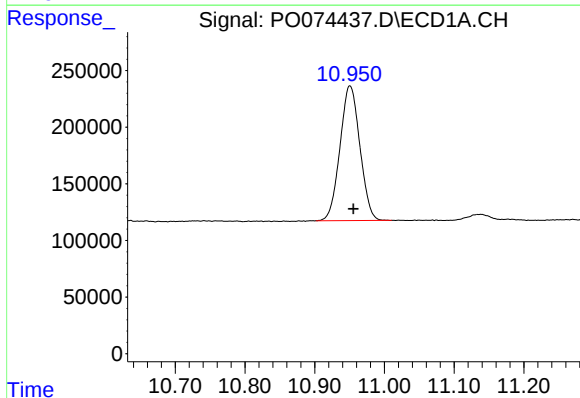


#2 Decachlorobiphenyl

R.T.: 10.951 min
Delta R.T.: -0.005 min
Response: 2358148
Conc: 25.37 ng/ml

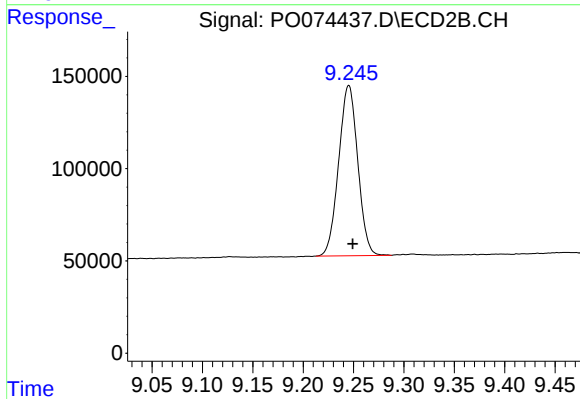

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.004 min
Response: 1217948
Conc: 23.40 ng/ml

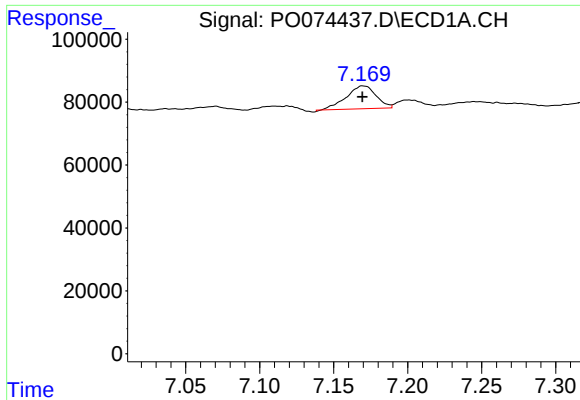


#26 AR-1254-1

R.T.: 7.169 min
Delta R.T.: 0.000 min
Response: 103280
Conc: 25.06 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HD-01-010621


Manual Integrations
APPROVED

Ankita
1/11/2021 11:12:55 AM

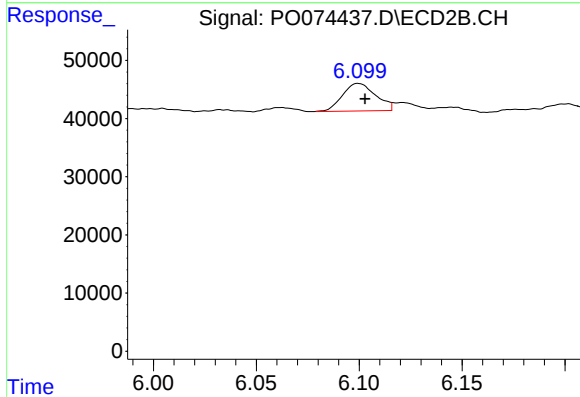


#26 AR-1254-1

R.T.: 6.099 min
Delta R.T.: -0.004 min
Response: 53987
Conc: 14.91 ng/ml m

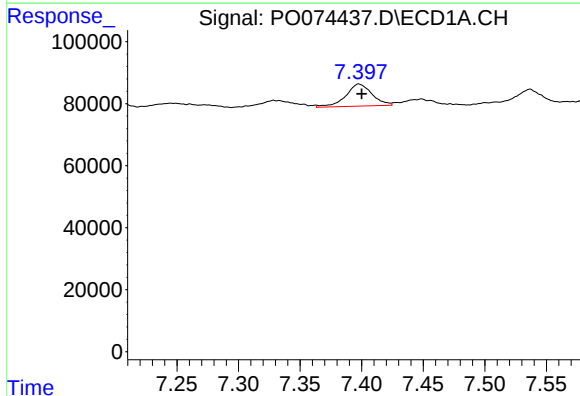


#27 AR-1254-2

R.T.: 7.397 min
Delta R.T.: -0.003 min
Response: 105558
Conc: 16.23 ng/ml m

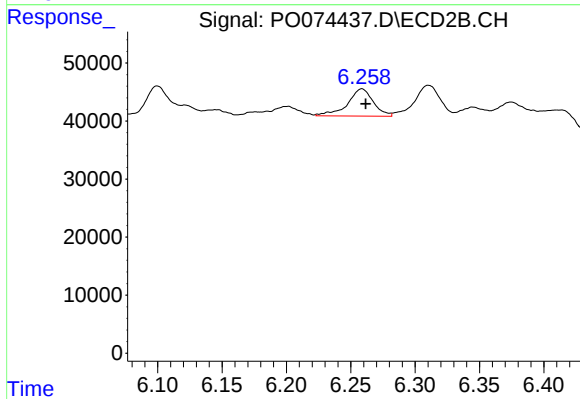

#27 AR-1254-2

R.T.: 6.258 min
Delta R.T.: -0.003 min
Response: 65548
Conc: 20.73 ng/ml m

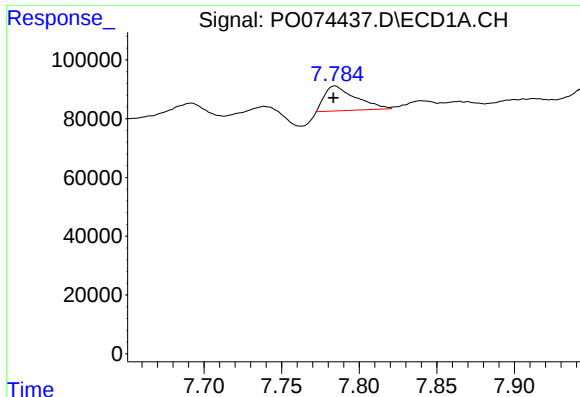


#28 AR-1254-3

R.T.: 7.784 min
Delta R.T.: 0.000 min
Response: 118762
Conc: 17.97 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HD-01-010621


Manual Integrations
APPROVED

Ankita
1/11/2021 11:12:55 AM

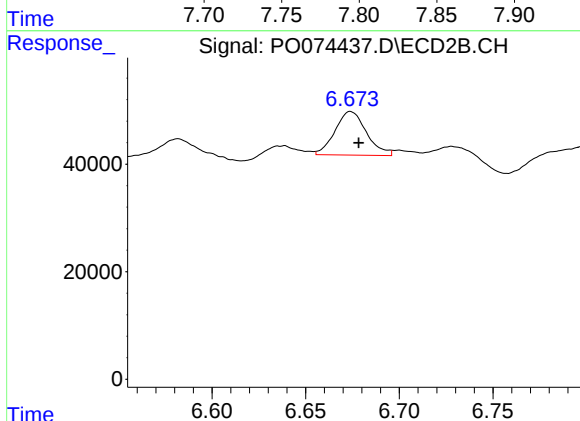


#28 AR-1254-3

R.T.: 6.673 min
Delta R.T.: -0.005 min
Response: 95283
Conc: 18.99 ng/ml m

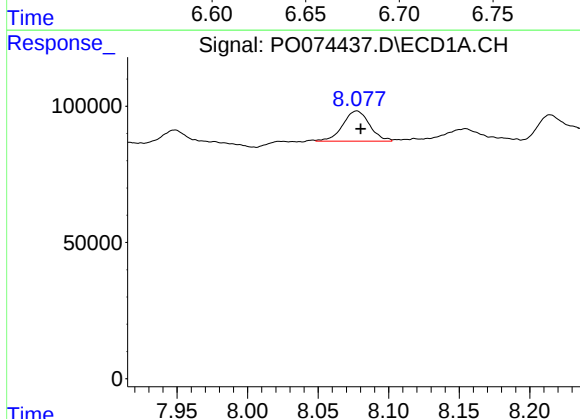


#29 AR-1254-4

R.T.: 8.077 min
Delta R.T.: -0.003 min
Response: 147665
Conc: 25.95 ng/ml m

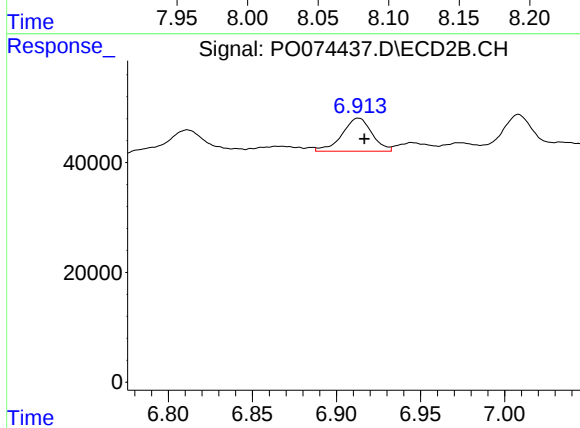

#29 AR-1254-4

R.T.: 6.913 min
Delta R.T.: -0.004 min
Response: 74598
Conc: 20.42 ng/ml m

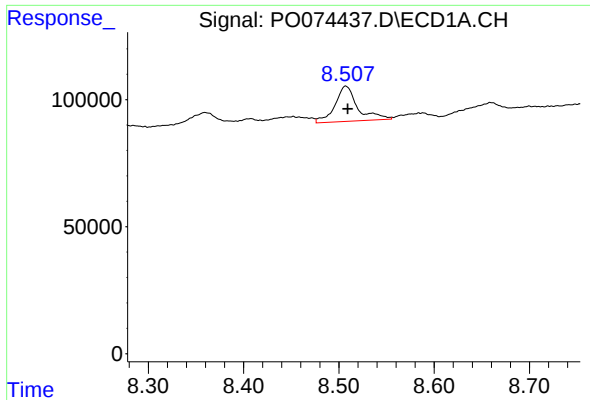


#30 AR-1254-5

R.T.: 8.508 min
Delta R.T.: -0.002 min
Response: 229173
Conc: 42.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
HD-01-010621

Manual Integrations
APPROVED

Ankita
1/11/2021 11:12:55 AM

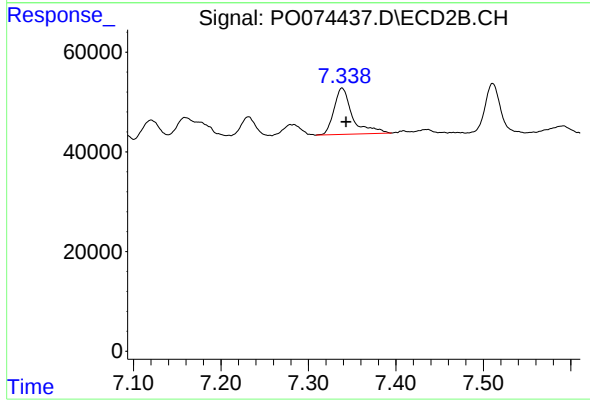

#30 AR-1254-5

R.T.: 7.339 min
Delta R.T.: -0.005 min
Response: 136100
Conc: 28.88 ng/ml