

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010821\
 Data File : P0074445.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jan 2021 13:12
 Operator : DD\AJ
 Sample : M1038-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TC-2A

Manual Integrations
 APPROVED

Ankita
 1/11/2021 11:13:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 08 16:21:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 05:03:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	3.990	2486635	1348033	25.879m	25.306
2) SA Decachlor...	10.950	9.245	2527119	1347469	27.183	25.884
Target Compounds						
31) L7 AR-1260-1	7.947	6.811	66337	46771	16.034	15.704
32) L7 AR-1260-2	8.214	7.007	80612	63314	13.893	15.538
33) L7 AR-1260-3	8.578	7.160	72632	43370	13.991m	12.459
34) L7 AR-1260-4	8.811	7.640	66098	57208	13.238m	20.008m#
35) L7 AR-1260-5	9.137	7.887	145605	113355	12.843	14.761

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010821\
Data File : PO074445.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2021 13:12
Operator : DD\AJ
Sample : M1038-05
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
TC-2A


Manual Integrations
APPROVED

Ankita
1/11/2021 11:13:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 08 16:21:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

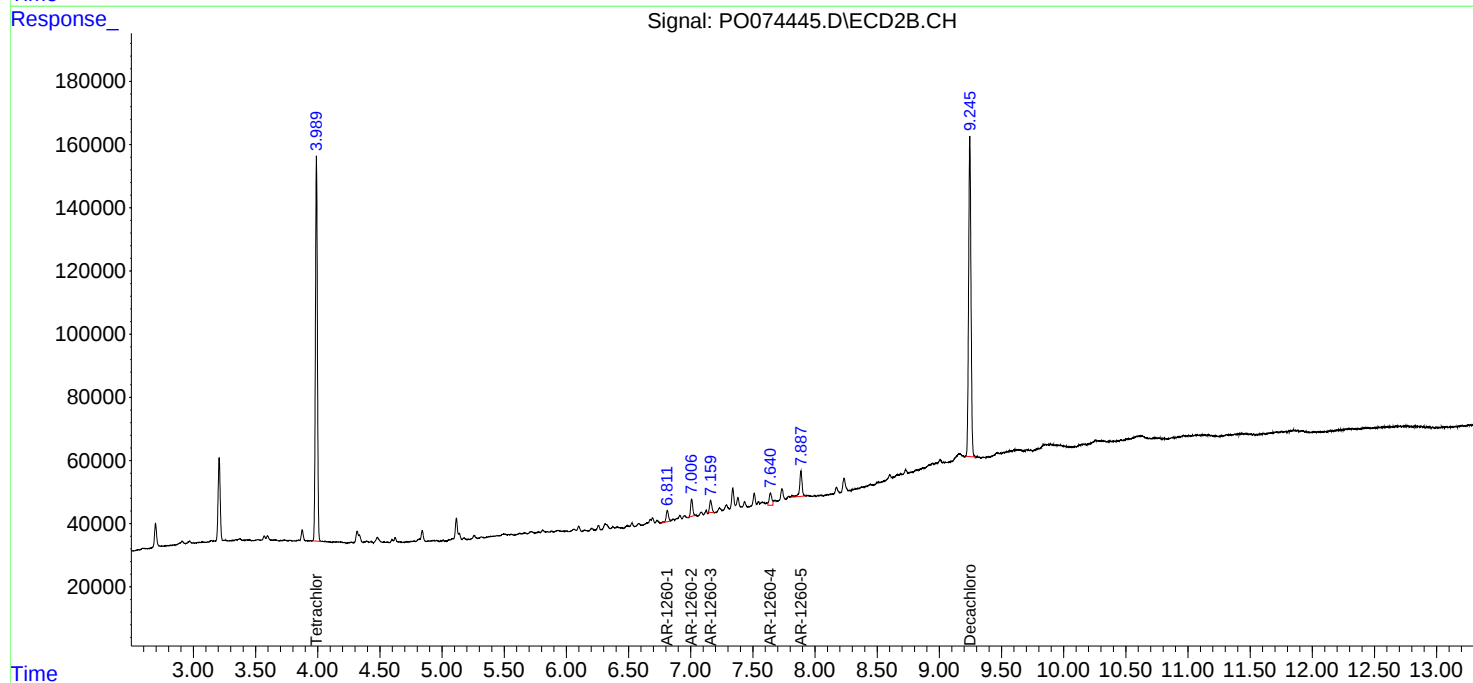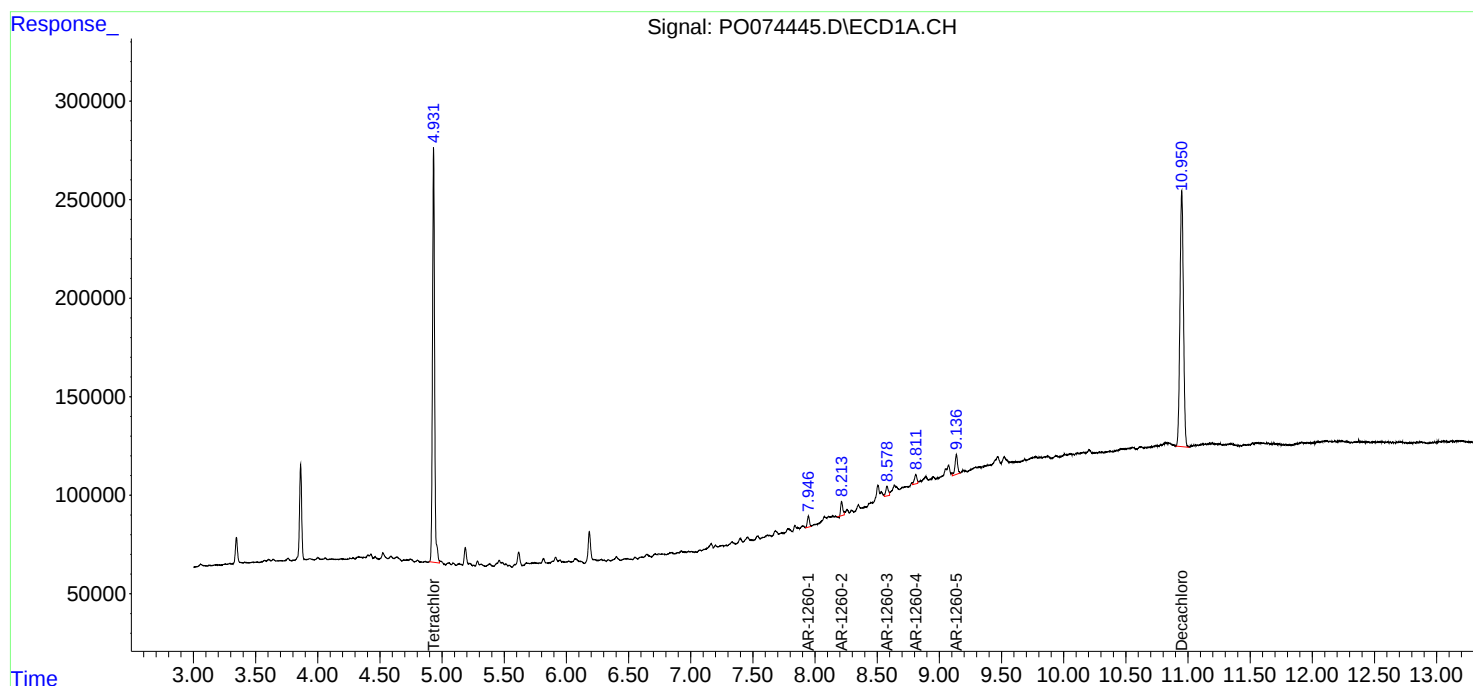

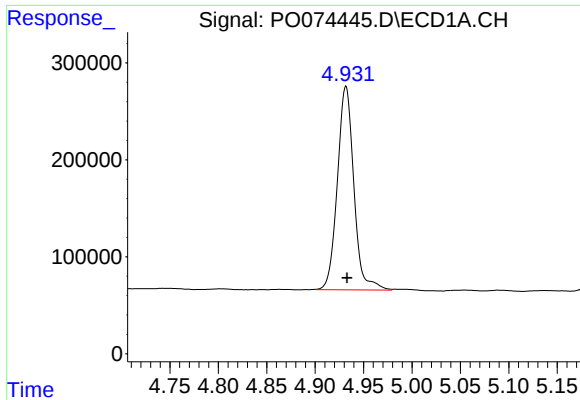


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: -0.002 min
Response: 2486635
Conc: 25.88 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TC-2A


Manual Integrations
APPROVED

Ankita
1/11/2021 11:13:05 AM

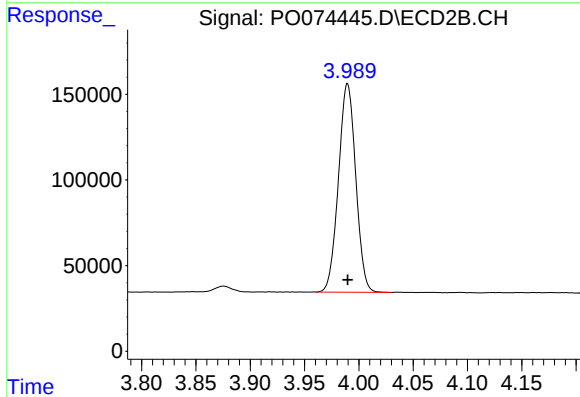


#1 Tetrachloro-m-xylene

R.T.: 3.990 min
Delta R.T.: 0.000 min
Response: 1348033
Conc: 25.31 ng/ml

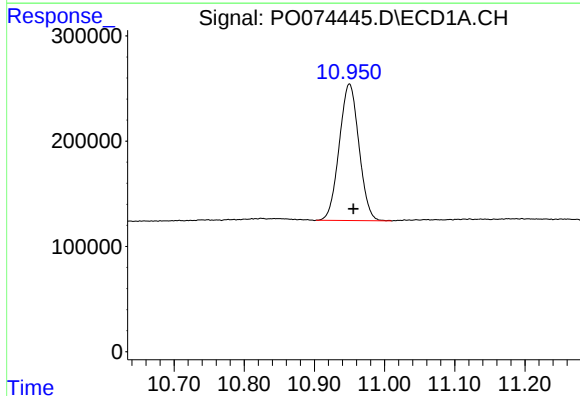


#2 Decachlorobiphenyl

R.T.: 10.950 min
Delta R.T.: -0.006 min
Response: 2527119
Conc: 27.18 ng/ml

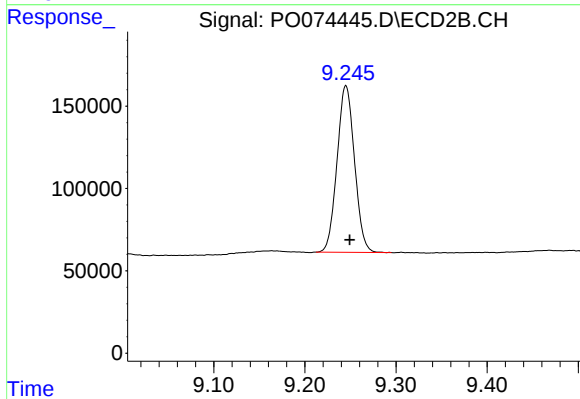

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.004 min
Response: 1347469
Conc: 25.88 ng/ml

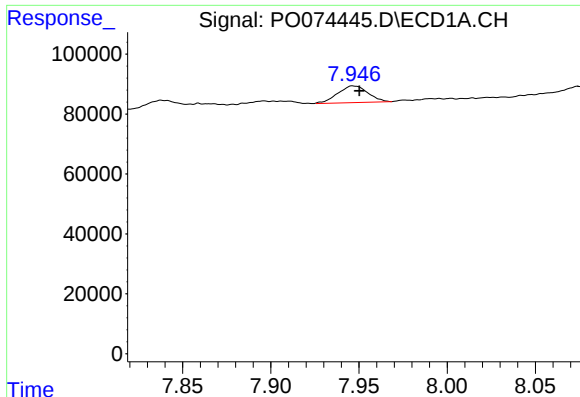


#31 AR-1260-1

R.T.: 7.947 min
Delta R.T.: -0.003 min
Response: 66337
Conc: 16.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
TC-2A


Manual Integrations
APPROVED

Ankita
1/11/2021 11:13:05 AM

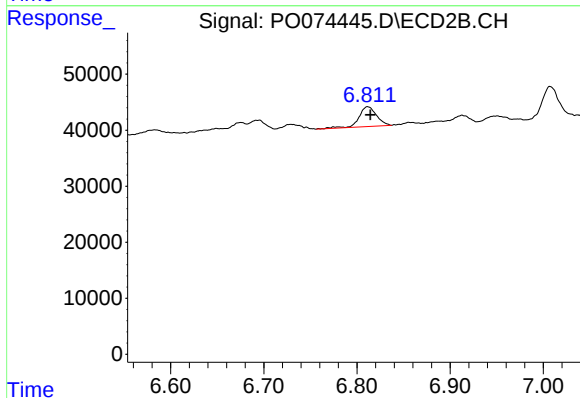


#31 AR-1260-1

R.T.: 6.811 min
Delta R.T.: -0.003 min
Response: 46771
Conc: 15.70 ng/ml

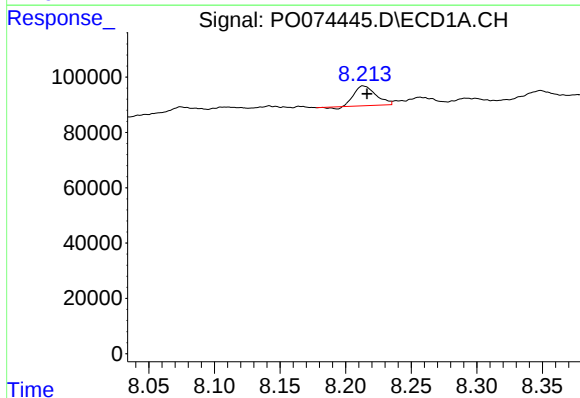


#32 AR-1260-2

R.T.: 8.214 min
Delta R.T.: -0.003 min
Response: 80612
Conc: 13.89 ng/ml

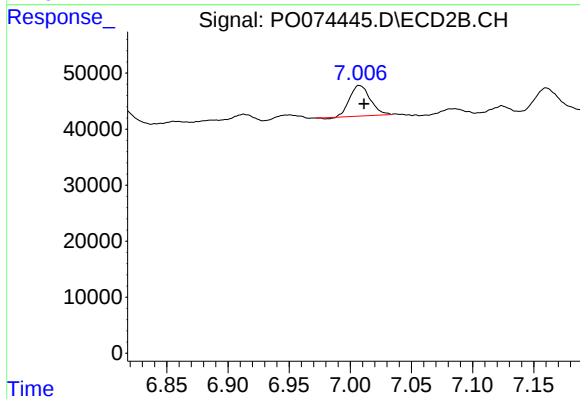

#32 AR-1260-2

R.T.: 7.007 min
Delta R.T.: -0.004 min
Response: 63314
Conc: 15.54 ng/ml

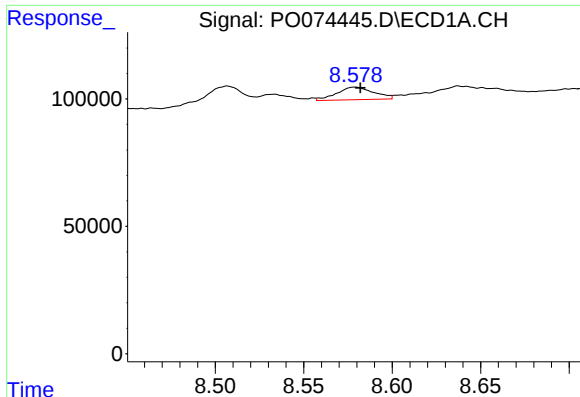


#33 AR-1260-3

R.T.: 8.578 min
Delta R.T.: -0.004 min
Response: 72632
Conc: 13.99 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TC-2A


Manual Integrations
APPROVED

Ankita
1/11/2021 11:13:05 AM

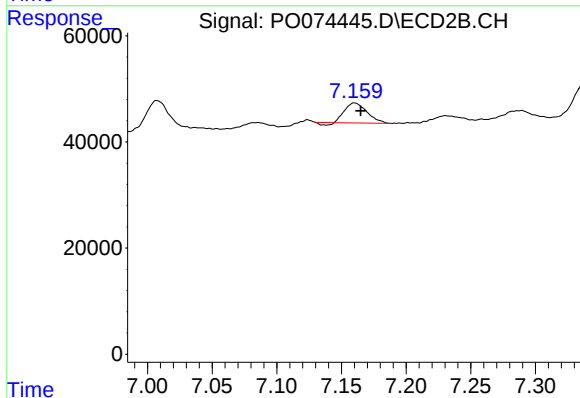


#33 AR-1260-3

R.T.: 7.160 min
Delta R.T.: -0.005 min
Response: 43370
Conc: 12.46 ng/ml

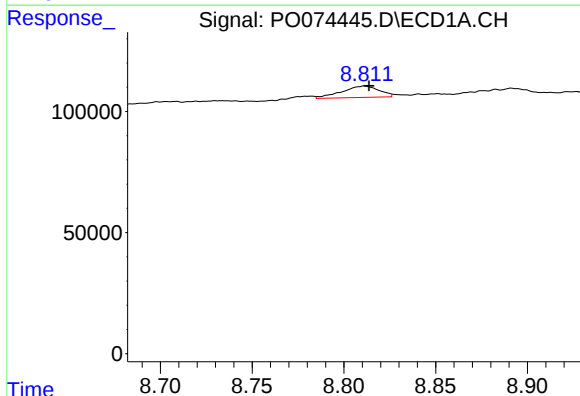


#34 AR-1260-4

R.T.: 8.811 min
Delta R.T.: -0.003 min
Response: 66098
Conc: 13.24 ng/ml m

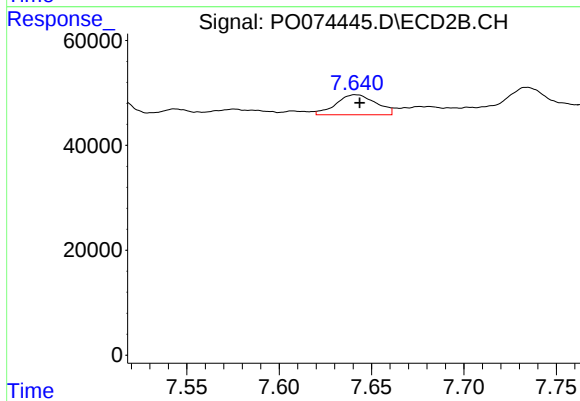

#34 AR-1260-4

R.T.: 7.640 min
Delta R.T.: -0.003 min
Response: 57208
Conc: 20.01 ng/ml m

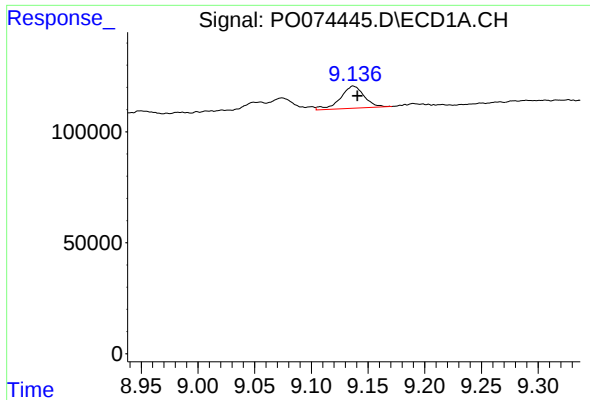


#35 AR-1260-5

R.T.: 9.137 min
Delta R.T.: -0.004 min
Response: 145605
Conc: 12.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
TC-2A

Manual Integrations
APPROVED

Ankita
1/11/2021 11:13:05 AM

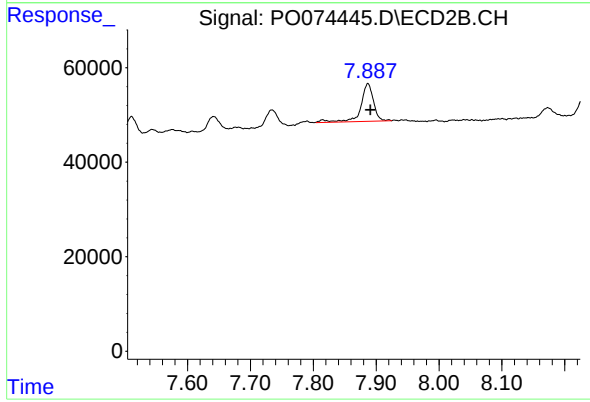

#35 AR-1260-5

R.T.: 7.887 min
Delta R.T.: -0.004 min
Response: 113355
Conc: 14.76 ng/ml