Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010821\
Data File : PO074456.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2021 16:43
Operator : DD\AJ
Sample : M1039-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
41030

Manual Integrations APPROVED
Ankita
1/11/2021 11:13:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 00:36:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	4.931	3.989	157304	67485	1.637m	1.267m
2)	SA Decachlor...	10.950	9.245	156660	50540	1.685	0.971 #
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010821\
Data File : PO074456.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2021 16:43
Operator : DD\AJ
Sample : M1039-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
41030

Manual Integrations APPROVED
Ankita
1/11/2021 11:13:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 00:36:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

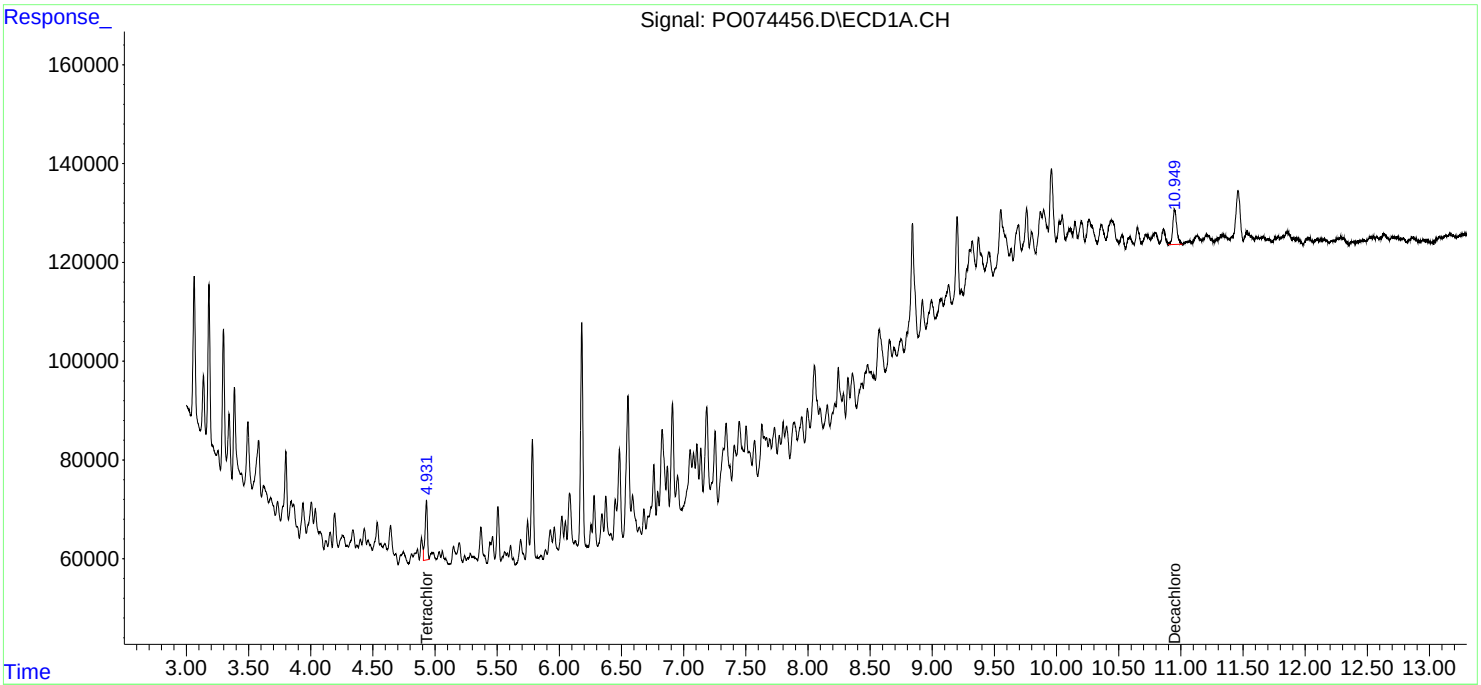

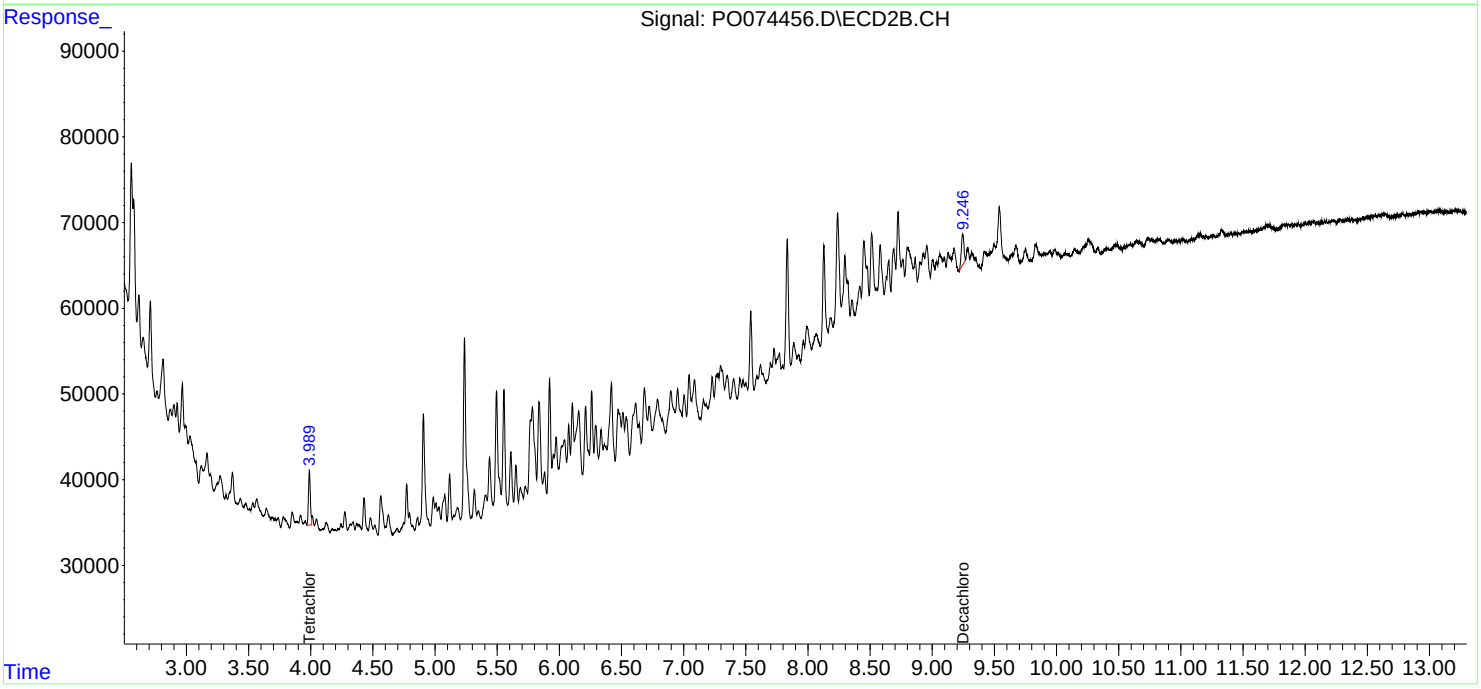

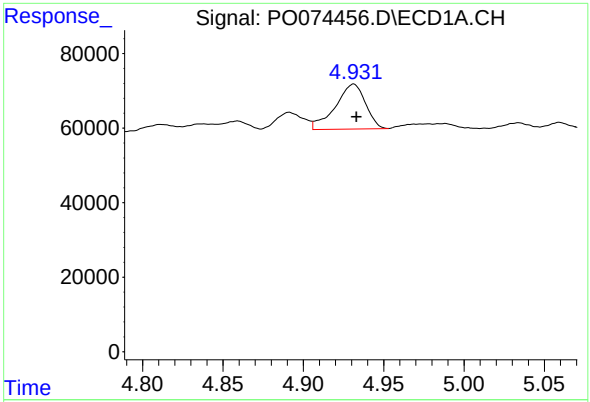

#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: -0.002 min
Response: 157304
Conc: 1.64 ng/ml m

Instrument :
ECD_O
ClientSampleId :
41030

Manual Integrations APPROVED
Ankita
1/11/2021 11:13:18 AM

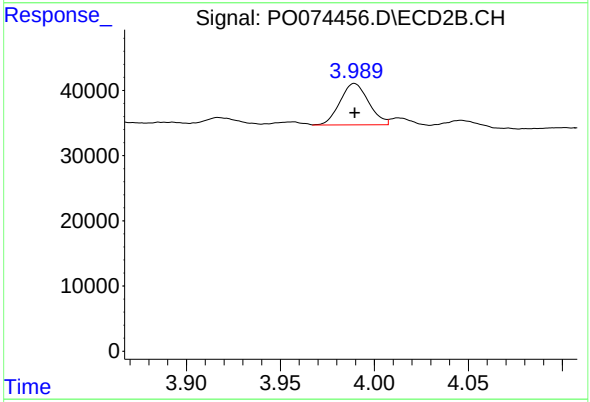

#1 Tetrachloro-m-xylene

R.T.: 3.989 min
Delta R.T.: 0.000 min
Response: 67485
Conc: 1.27 ng/ml m

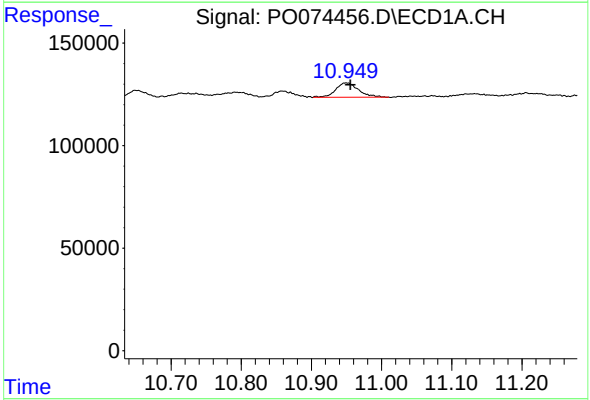

#2 Decachlorobiphenyl

R.T.: 10.950 min
Delta R.T.: -0.006 min
Response: 156660
Conc: 1.69 ng/ml

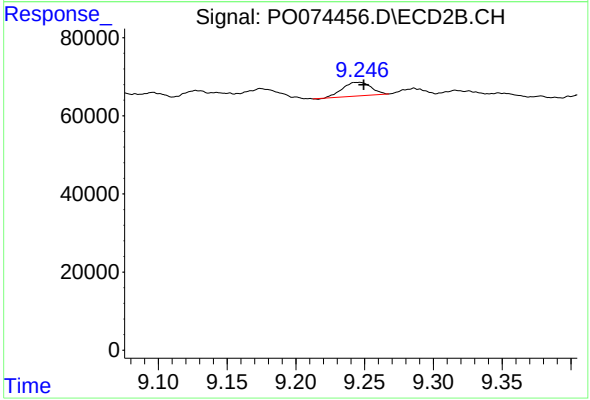

#2 Decachlorobiphenyl

R.T.: 9.245 min
Delta R.T.: -0.004 min
Response: 50540
Conc: 0.97 ng/ml