

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010821\
 Data File : P0074459.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jan 2021 17:35
 Operator : DD\AJ
 Sample : M1040-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 41661

Manual Integrations
 APPROVED

Ankita
 1/11/2021 11:13:20 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 00:38:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 05 05:03:05 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.954f	4.026f	1806181	930436	18.797m	17.467m
2) SA Decachlor...	10.951	9.246	1438403	728828	15.472	14.000

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010821\
Data File : P0074459.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jan 2021 17:35
Operator : DD\AJ
Sample : M1040-04
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
41661


Manual Integrations
APPROVED

Ankita
1/11/2021 11:13:20 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 00:38:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010421.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 05 05:03:05 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

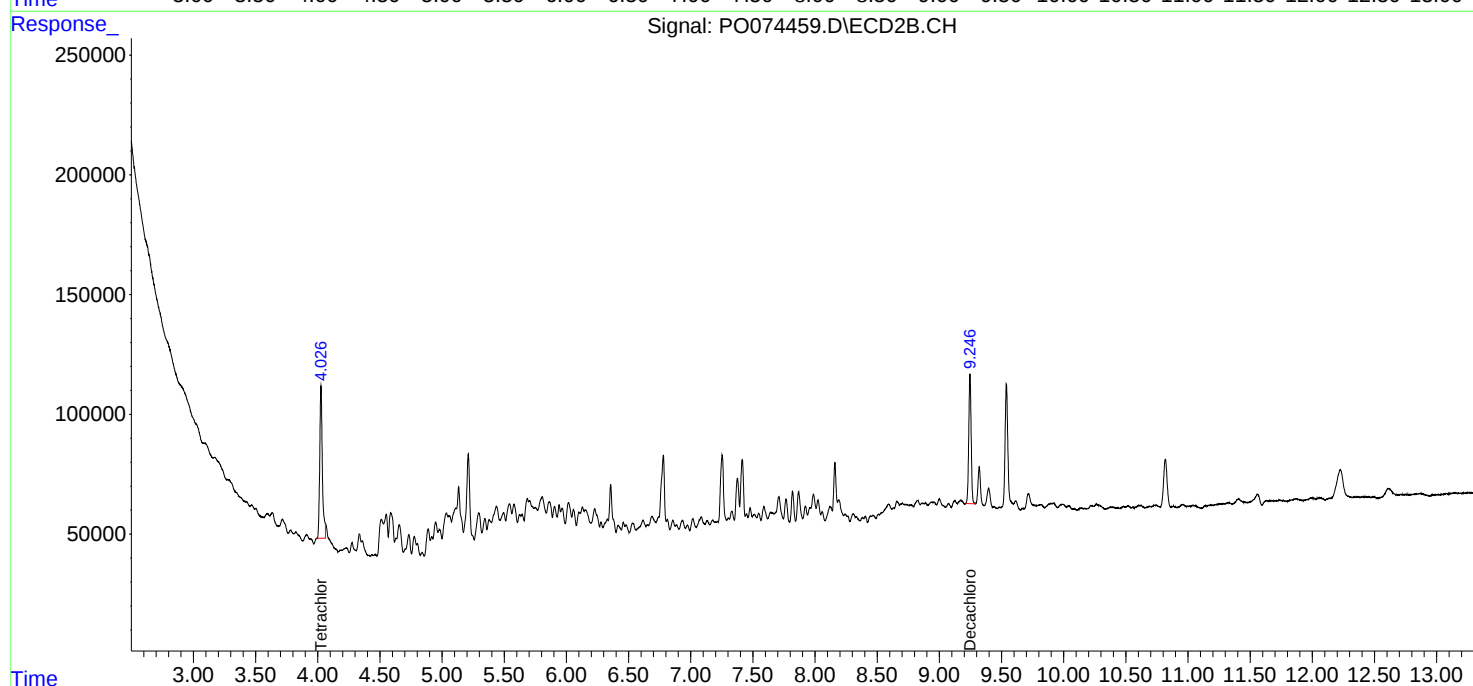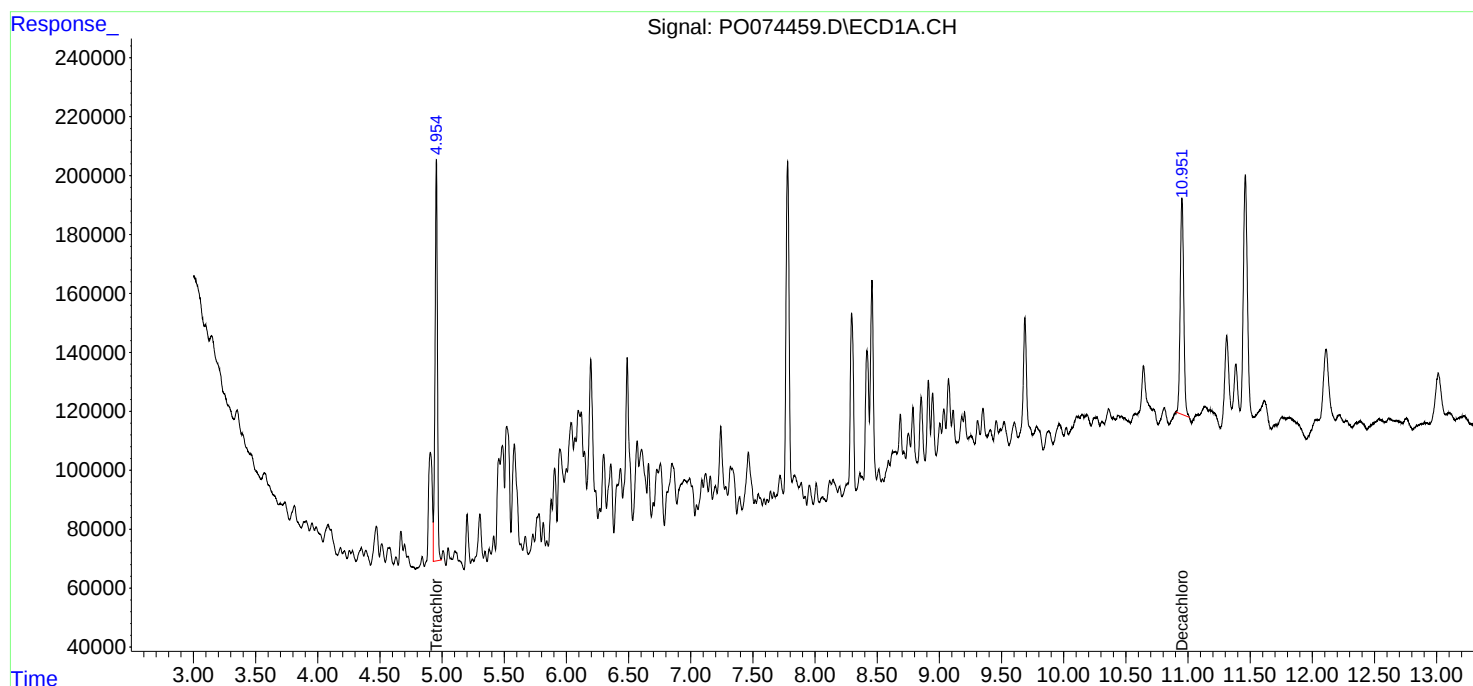

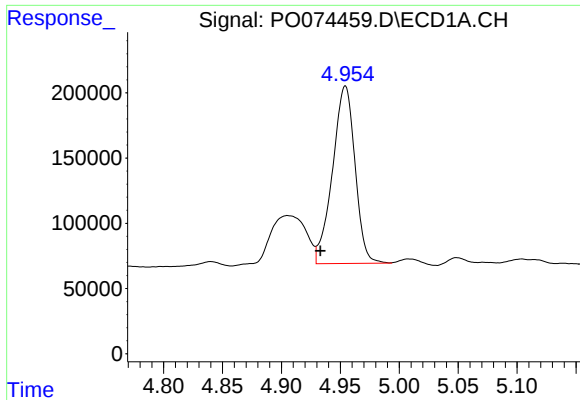


#1 Tetrachloro-m-xylene

R.T.: 4.954 min
Delta R.T.: 0.021 min
Response: 1806181
Conc: 18.80 ng/ml m

Instrument :
ECD_O
ClientSampleId :
41661


Manual Integrations
APPROVED

Ankita
1/11/2021 11:13:20 AM

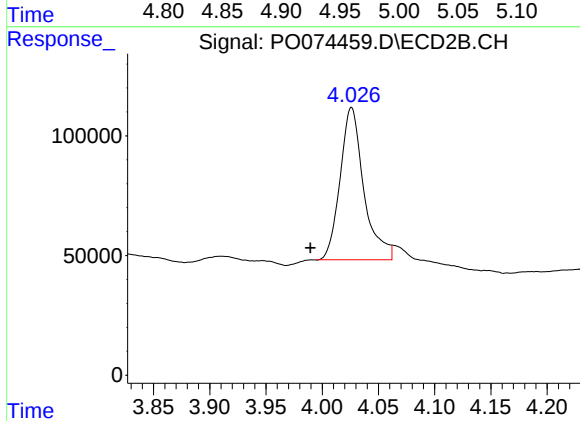


#1 Tetrachloro-m-xylene

R.T.: 4.026 min
Delta R.T.: 0.036 min
Response: 930436
Conc: 17.47 ng/ml m

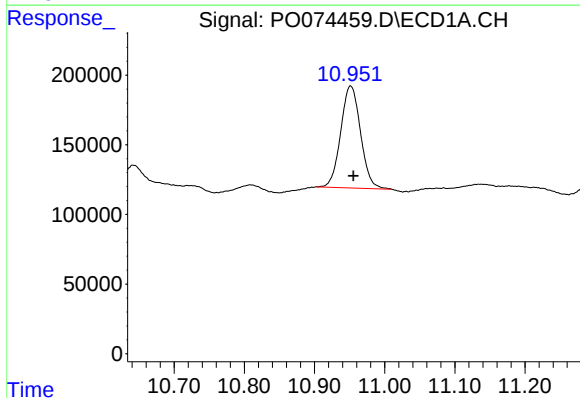

#2 Decachlorobiphenyl

R.T.: 10.951 min
Delta R.T.: -0.004 min
Response: 1438403
Conc: 15.47 ng/ml

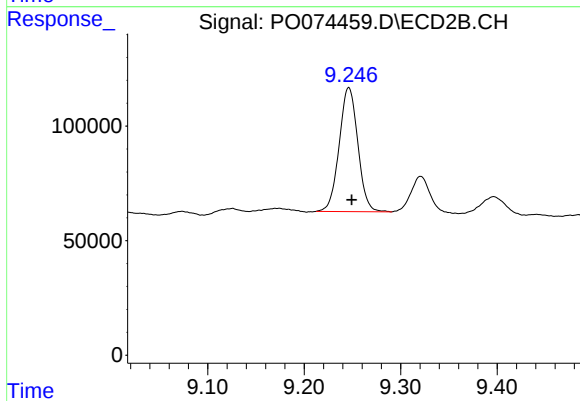

#2 Decachlorobiphenyl

R.T.: 9.246 min
Delta R.T.: -0.003 min
Response: 728828
Conc: 14.00 ng/ml