

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010824\
 Data File : P0100972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2024 14:20
 Operator : YP/AJ
 Sample : P1055-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-1221

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/09/2024
 Supervised By :Ankita Jodhani 01/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 00:26:28 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.348	3.647	47185747	26332947	15.122m	12.887m
2) SA Decachlor...	10.080	8.695	49196315	33857221	23.549	22.432

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010824\
Data File : PO100972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2024 14:20
Operator : YP/AJ
Sample : P1055-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TOTE-1221


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/09/2024
Supervised By :Ankita Jodhani 01/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 00:26:28 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

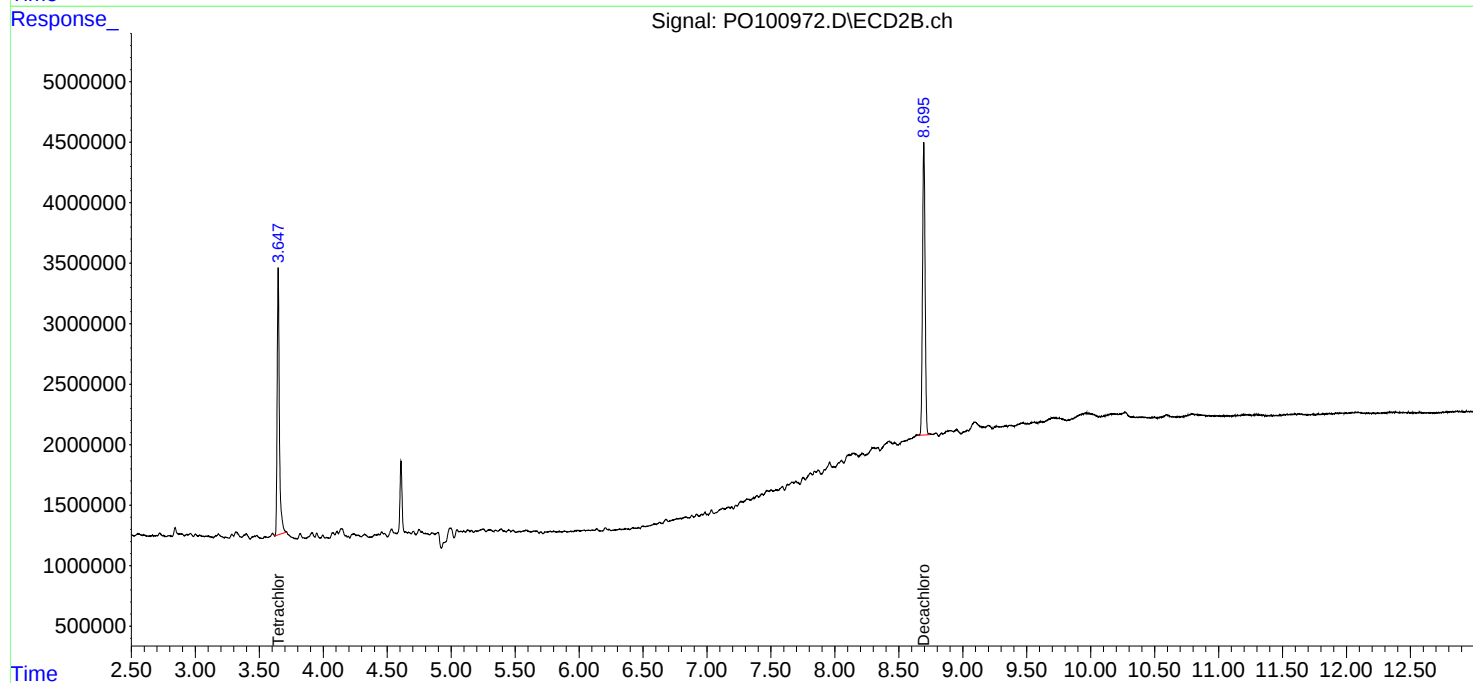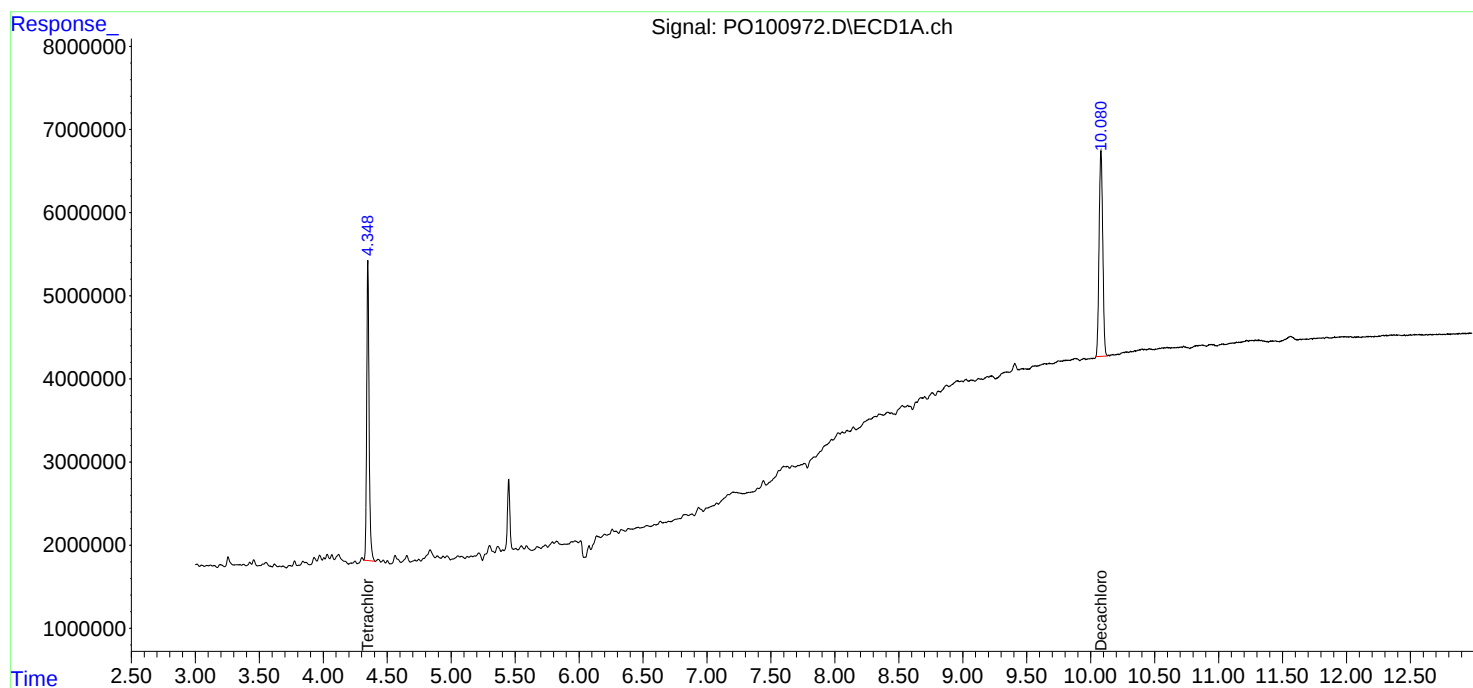

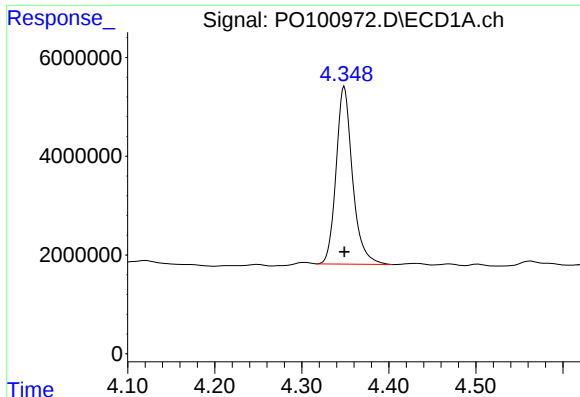


#1 Tetrachloro-m-xylene

R.T.: 4.348 min
Delta R.T.: 0.000 min
Response: 47185747
Conc: 15.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-1221


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/09/2024
Supervised By :Ankita Jodhani 01/09/2024

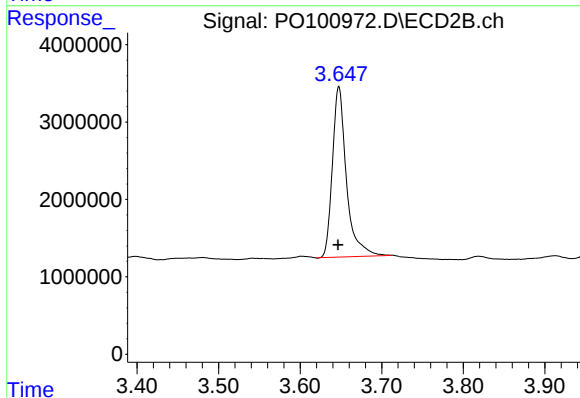


#1 Tetrachloro-m-xylene

R.T.: 3.647 min
Delta R.T.: 0.000 min
Response: 26332947
Conc: 12.89 ng/ml m

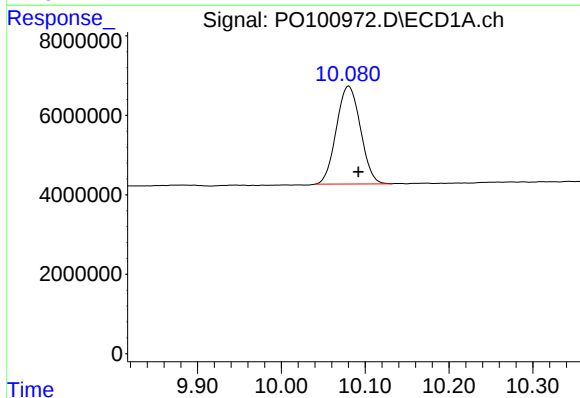

#2 Decachlorobiphenyl

R.T.: 10.080 min
Delta R.T.: -0.011 min
Response: 49196315
Conc: 23.55 ng/ml

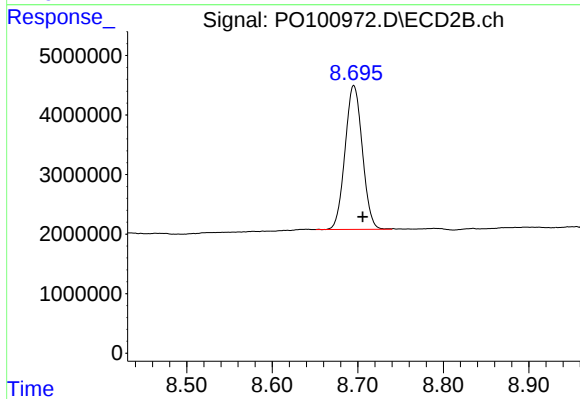

#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: -0.011 min
Response: 33857221
Conc: 22.43 ng/ml