

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0010824\
 Data File : P0100983.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Jan 2024 17:40
 Operator : YP/AJ
 Sample : P1050-01 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHRT24029

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/09/2024
 Supervised By :Ankita Jodhani 01/09/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 09 00:31:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0122023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Dec 21 04:28:19 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.640	4417300	2345774	1.416	1.148
2) SA Decachlor...	10.082	8.693	4144535	4936434	1.984	3.271m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO010824\
Data File : PO100983.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Jan 2024 17:40
Operator : YP/AJ
Sample : P1050-01 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CHRT24029


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/09/2024
Supervised By :Ankita Jodhani 01/09/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 09 00:31:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO122023.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Dec 21 04:28:19 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

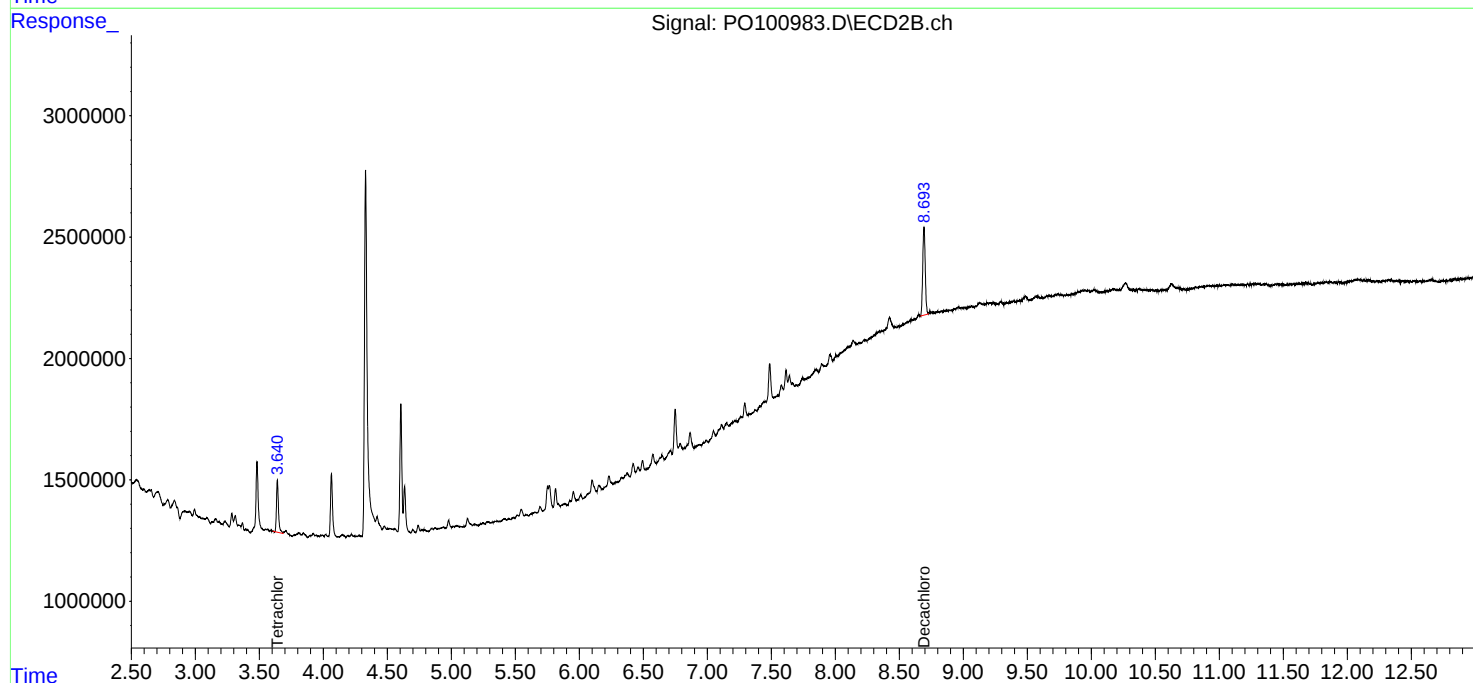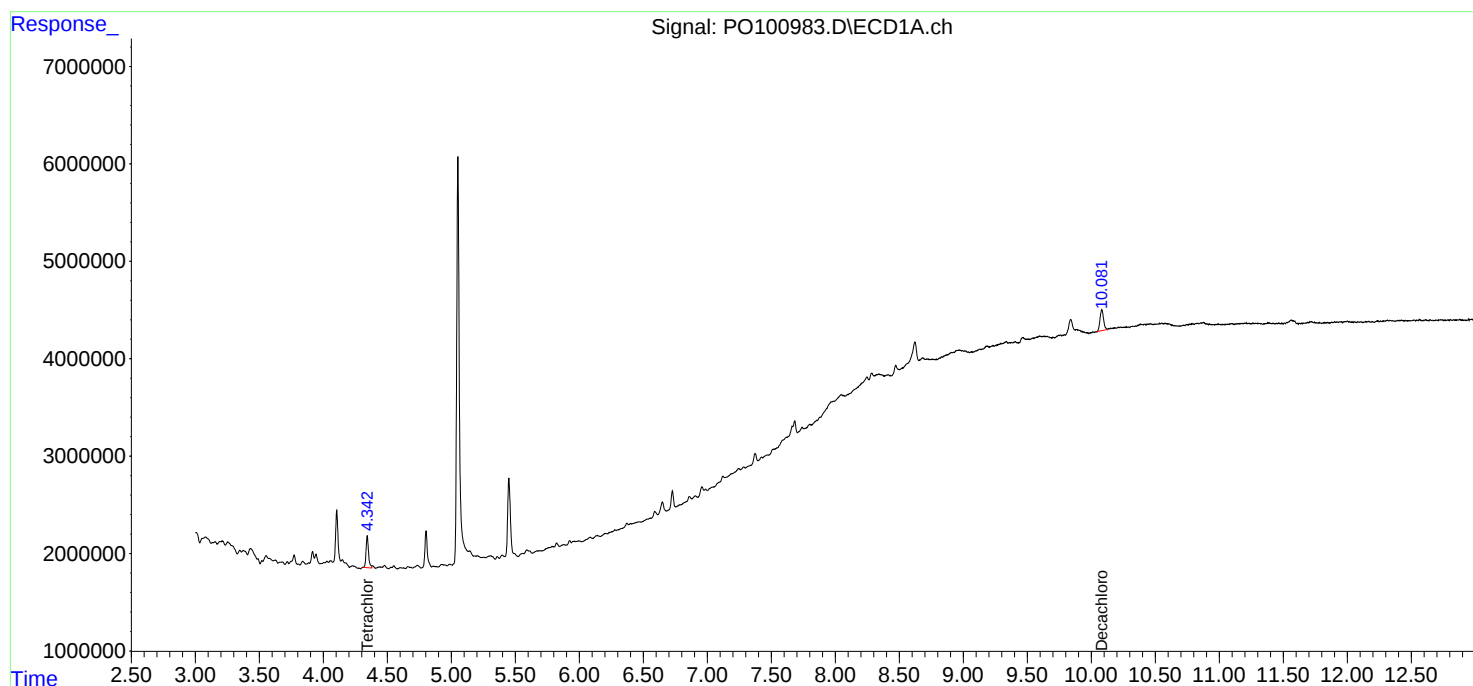

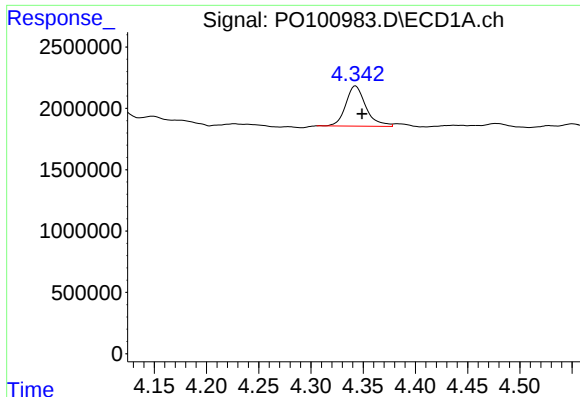


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: -0.006 min
Response: 4417300
Conc: 1.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT24029


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/09/2024
Supervised By :Ankita Jodhani 01/09/2024

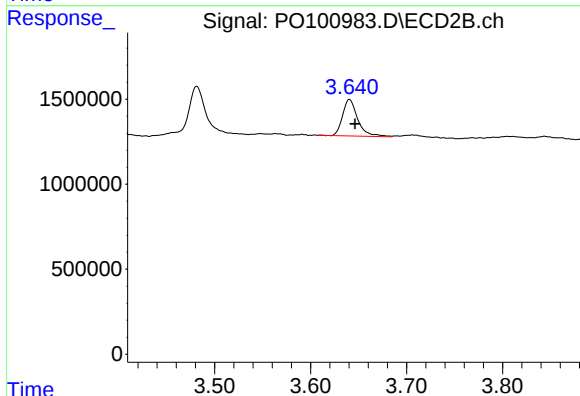


#1 Tetrachloro-m-xylene

R.T.: 3.640 min
Delta R.T.: -0.006 min
Response: 2345774
Conc: 1.15 ng/ml

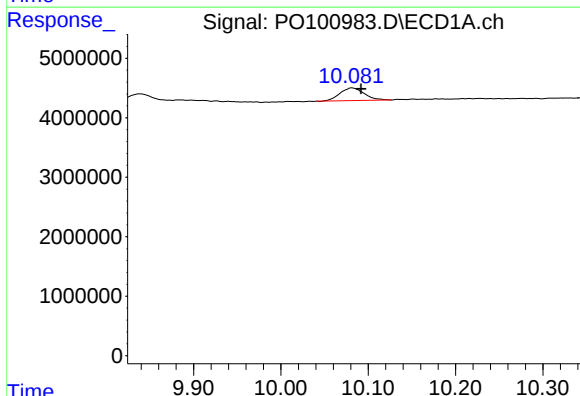

#2 Decachlorobiphenyl

R.T.: 10.082 min
Delta R.T.: -0.010 min
Response: 4144535
Conc: 1.98 ng/ml

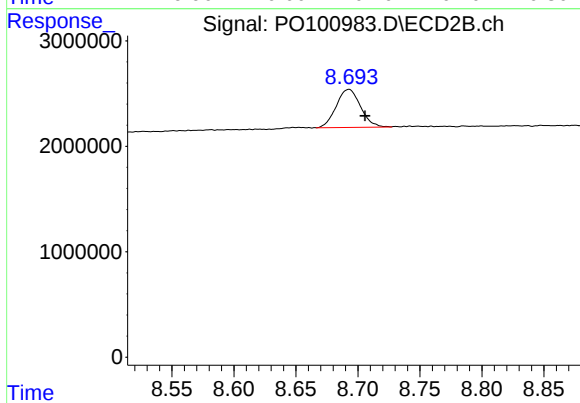

#2 Decachlorobiphenyl

R.T.: 8.693 min
Delta R.T.: -0.013 min
Response: 4936434
Conc: 3.27 ng/ml m