

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011019\
 Data File : P0053335.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2019 7:53
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 00:38:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 09 03:34:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.167	3.204	28504092	4877059	21.331	19.505
2) SA Decachlor...	9.627	7.848	18704745	6079665	23.681	26.548

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011019\
Data File : P0053335.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2019 7:53
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 00:38:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

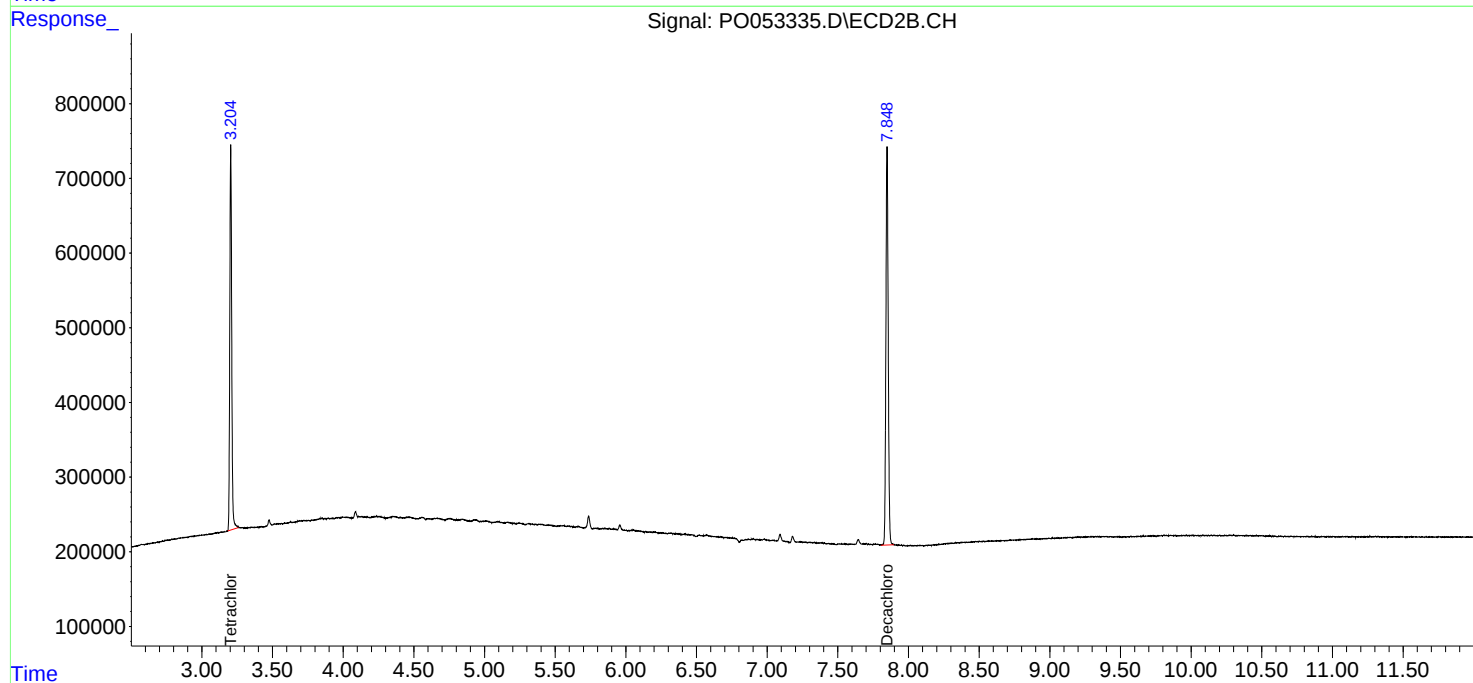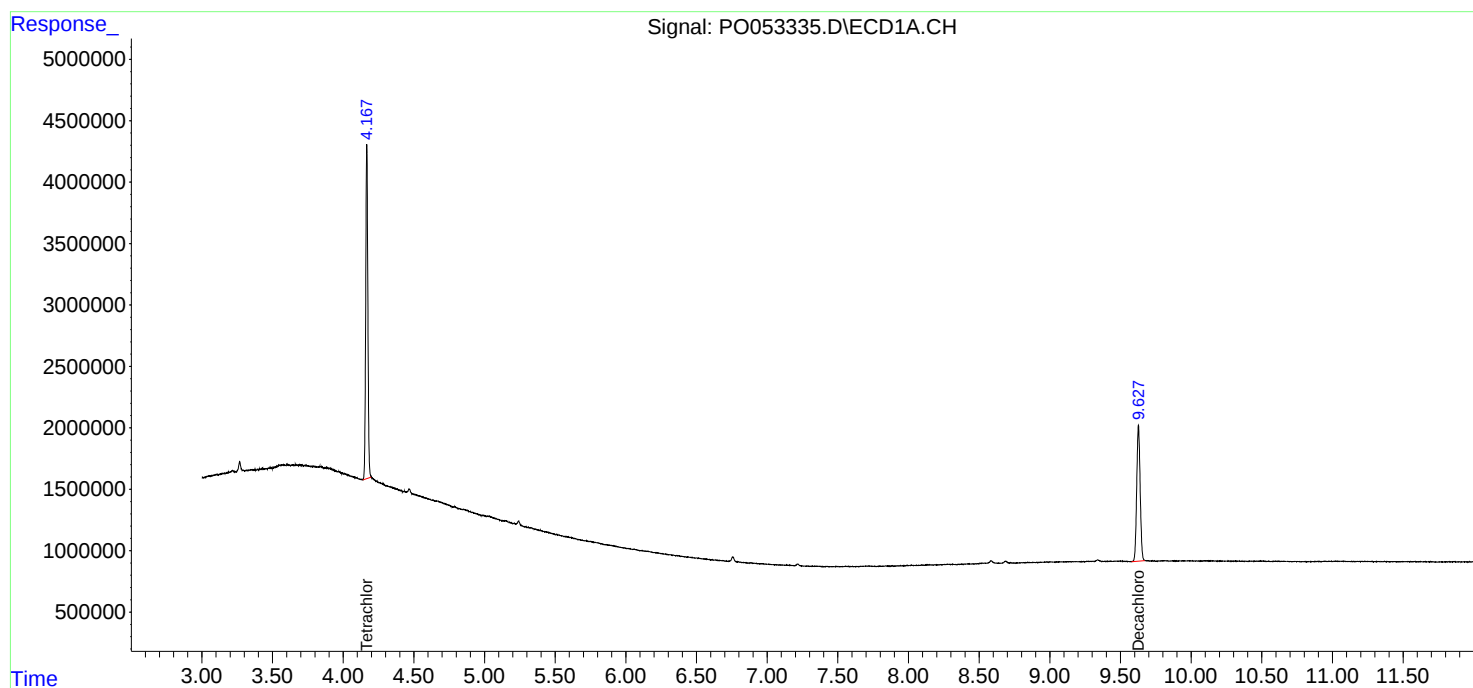


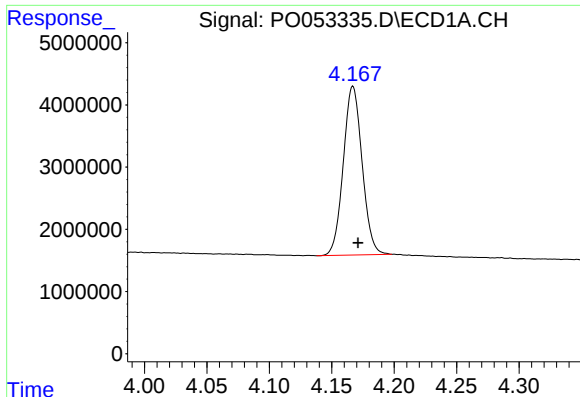

#1 Tetrachloro-m-xylene


R.T.: 4.167 min
Delta R.T.: -0.004 min
Response: 28504092
Conc: 21.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

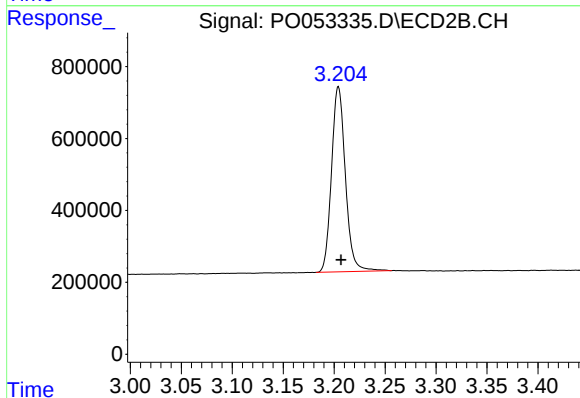


#1 Tetrachloro-m-xylene

R.T.: 3.204 min
Delta R.T.: -0.003 min
Response: 4877059
Conc: 19.50 ng/ml

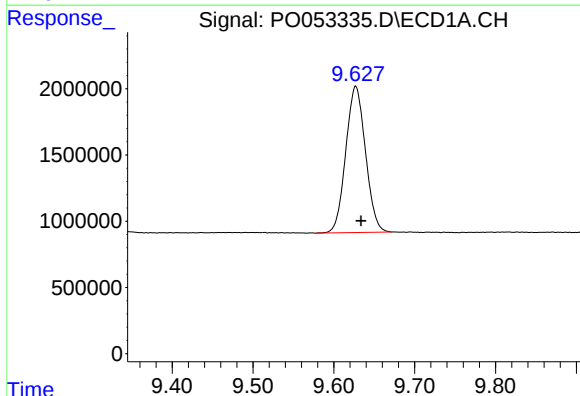

#2 Decachlorobiphenyl

R.T.: 9.627 min
Delta R.T.: -0.007 min
Response: 18704745
Conc: 23.68 ng/ml

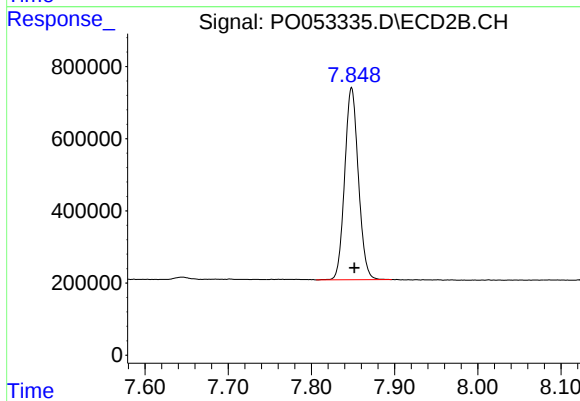

#2 Decachlorobiphenyl

R.T.: 7.848 min
Delta R.T.: -0.003 min
Response: 6079665
Conc: 26.55 ng/ml