

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011019\
 Data File : P0053342.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2019 10:24
 Operator : SM/SJ
 Sample : K1082-11
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SP-1-6

Manual Integrations
 APPROVED

Sohil
 1/11/2019 10:33:13 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 00:42:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 09 03:34:05 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.166	3.204	26109306	3417420	19.539m	13.667 #
2) SA Decachlor...	9.626	7.847	11593404	3488072	14.678	15.232

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011019\
Data File : P0053342.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2019 10:24
Operator : SM/SJ
Sample : K1082-11
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SP-1-6


Manual Integrations
APPROVED

Sohil
1/11/2019 10:33:13 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 00:42:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010819.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 09 03:34:05 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

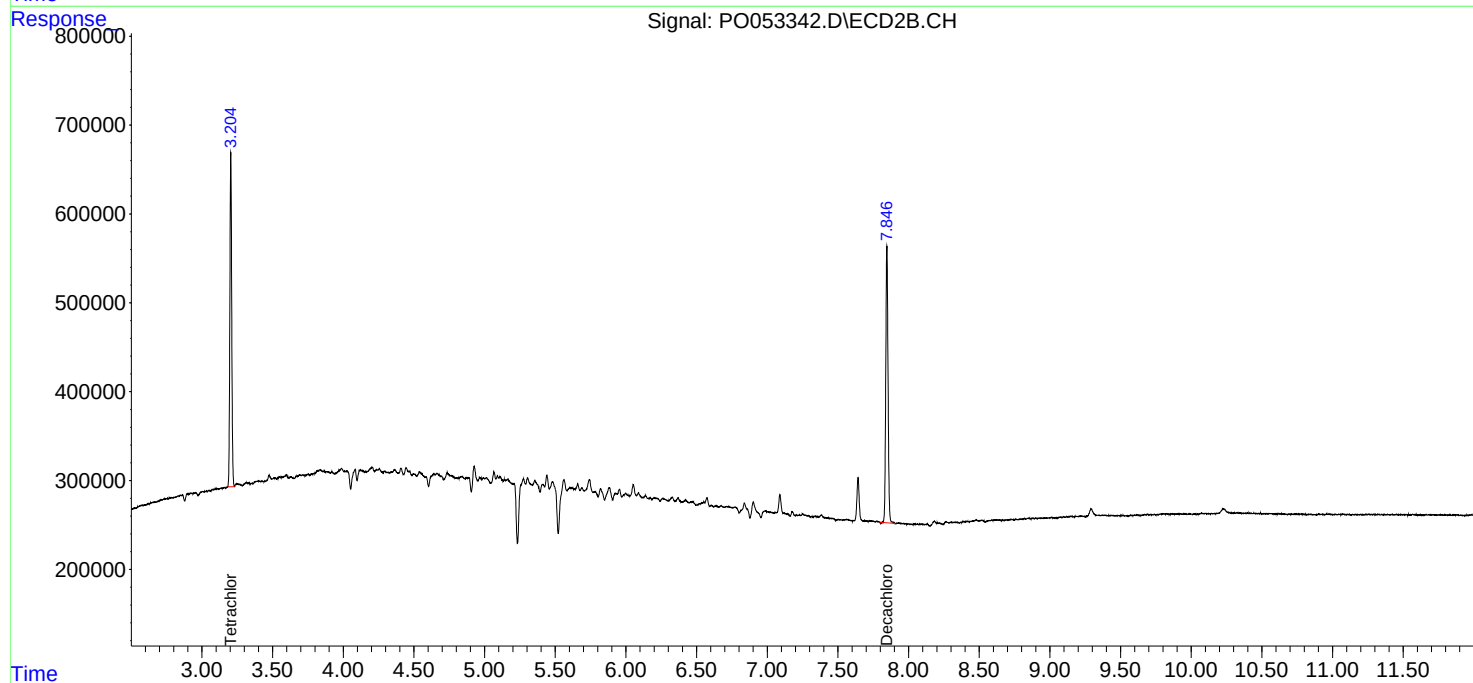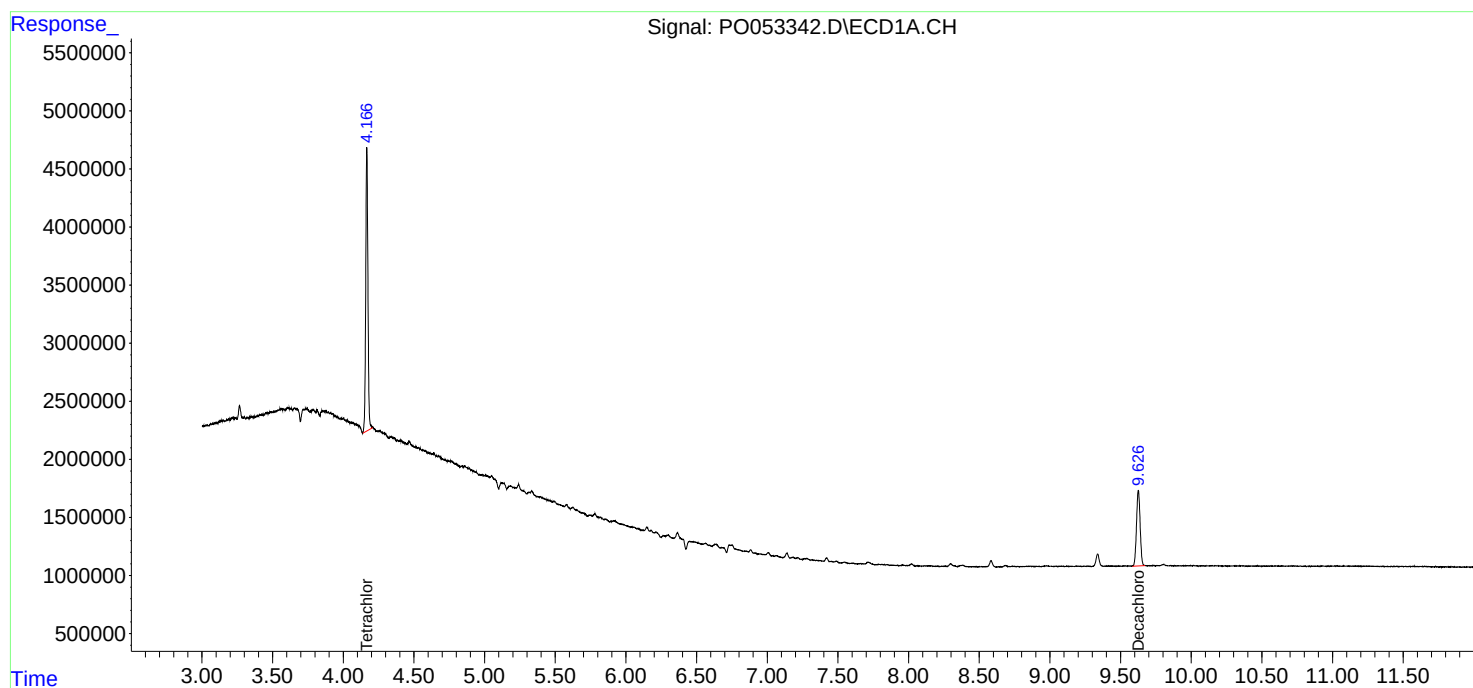

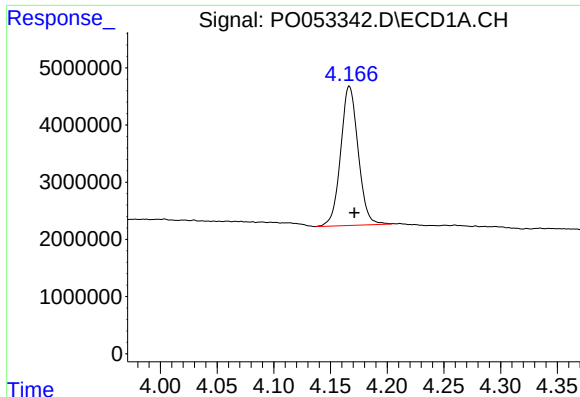


#1 Tetrachloro-m-xylene

R.T.: 4.166 min
Delta R.T.: -0.005 min
Response: 26109306
Conc: 19.54 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SP-1-6


Manual Integrations
APPROVED

Sohil
1/11/2019 10:33:13 AM

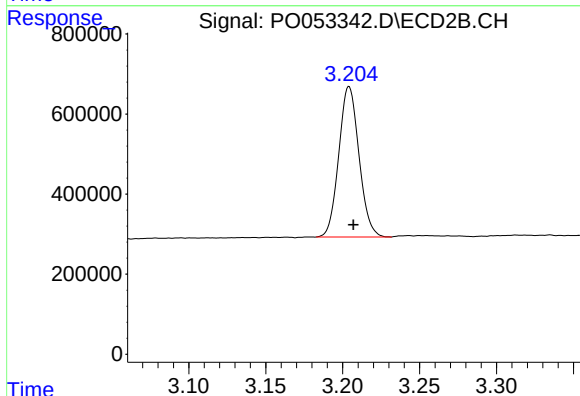


#1 Tetrachloro-m-xylene

R.T.: 3.204 min
Delta R.T.: -0.003 min
Response: 3417420
Conc: 13.67 ng/ml

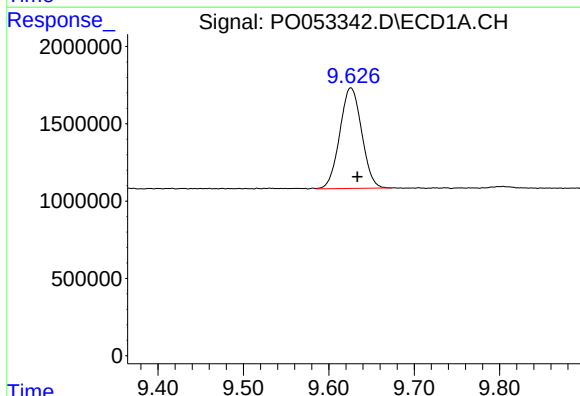

#2 Decachlorobiphenyl

R.T.: 9.626 min
Delta R.T.: -0.008 min
Response: 11593404
Conc: 14.68 ng/ml

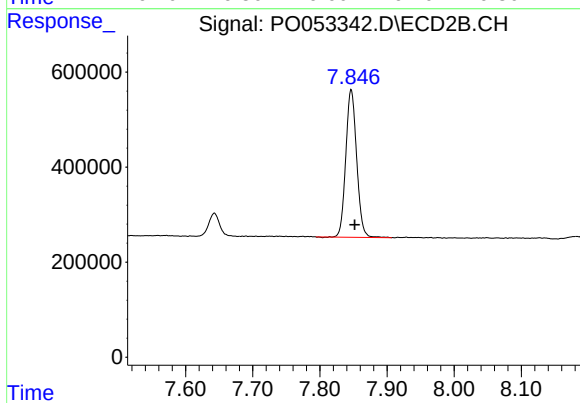

#2 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: -0.005 min
Response: 3488072
Conc: 15.23 ng/ml