

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011020\
 Data File : P0065415.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2020 12:16
 Operator : AJ/MA
 Sample : PB126003BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB126003BL

Manual Integrations
 APPROVED

mohammad
 1/13/2020 10:18:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 13:14:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.183	3.443	416440	460700	22.806m	20.943
2)	SA Decachlor...	9.697	8.354	705980	800150	20.836	19.295

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011020\
Data File : PO065415.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2020 12:16
Operator : AJ/MA
Sample : PB126003BL
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB126003BL


Manual Integrations
APPROVED

mohammad
1/13/2020 10:18:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 13:14:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

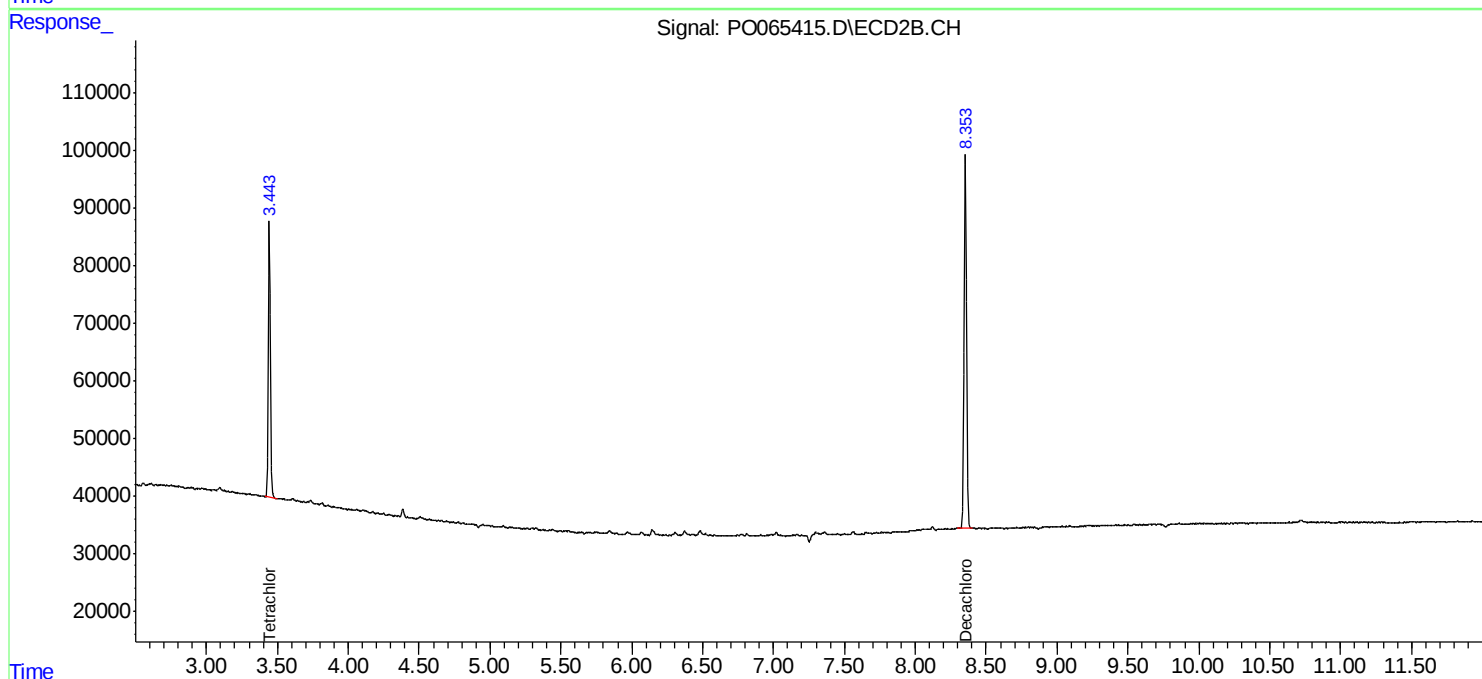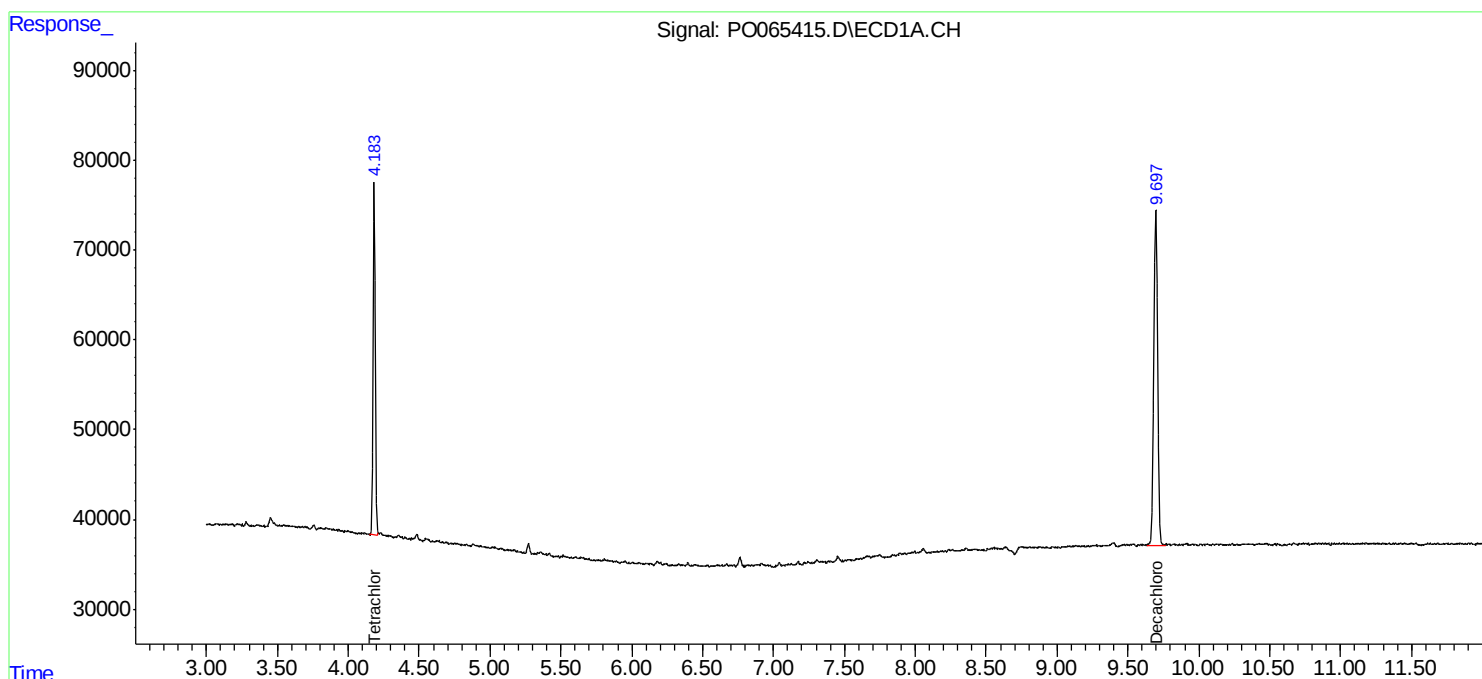

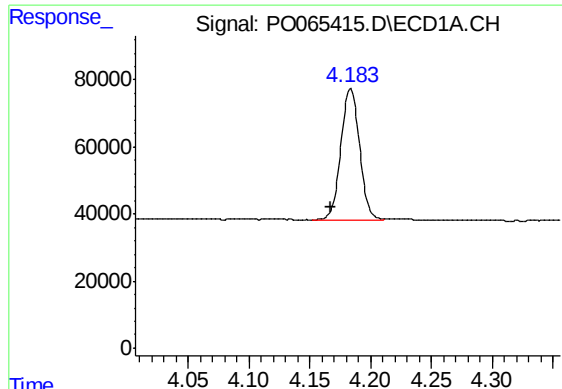


#1 Tetrachloro-m-xylene

R.T.: 4.183 min
Delta R.T.: 0.016 min
Response: 416440
Conc: 22.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB126003BL


Manual Integrations
APPROVED

mohammad
1/13/2020 10:18:49 AM

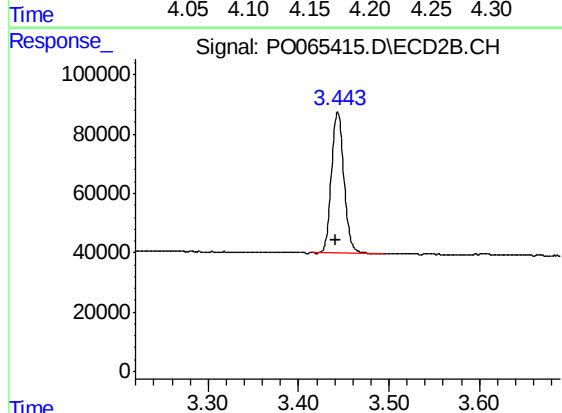


#1 Tetrachloro-m-xylene

R.T.: 3.443 min
Delta R.T.: 0.002 min
Response: 460700
Conc: 20.94 ng/ml

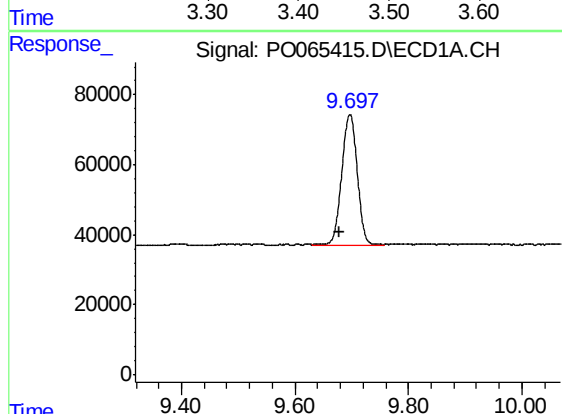

#2 Decachlorobiphenyl

R.T.: 9.697 min
Delta R.T.: 0.019 min
Response: 705980
Conc: 20.84 ng/ml

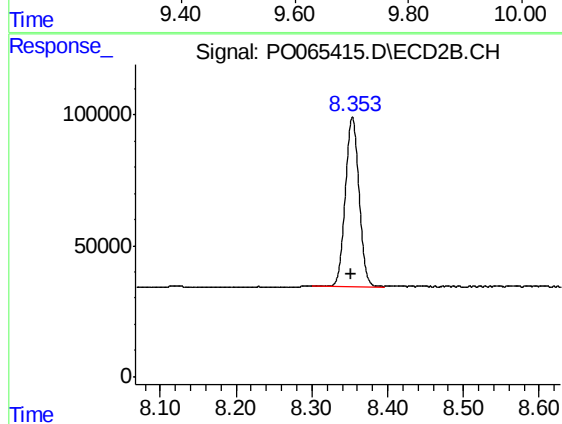

#2 Decachlorobiphenyl

R.T.: 8.354 min
Delta R.T.: 0.000 min
Response: 800150
Conc: 19.29 ng/ml