

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011020\
 Data File : P0065424.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2020 14:45
 Operator : AJ/MA
 Sample : L1064-09RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ODRE

Manual Integrations
 APPROVED

mohammad
 1/13/2020 10:19:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 10 15:26:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jan 04 04:01:28 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.187	3.471	717983	854206	39.319m	38.832m
2)	SA Decachlor...	9.670	8.345	699315	771354	20.639	18.600

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011020\
Data File : PO065424.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2020 14:45
Operator : AJ/MA
Sample : L1064-09RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ODRE


Manual Integrations
APPROVED

mohammad
1/13/2020 10:19:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 10 15:26:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010420.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jan 04 04:01:28 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

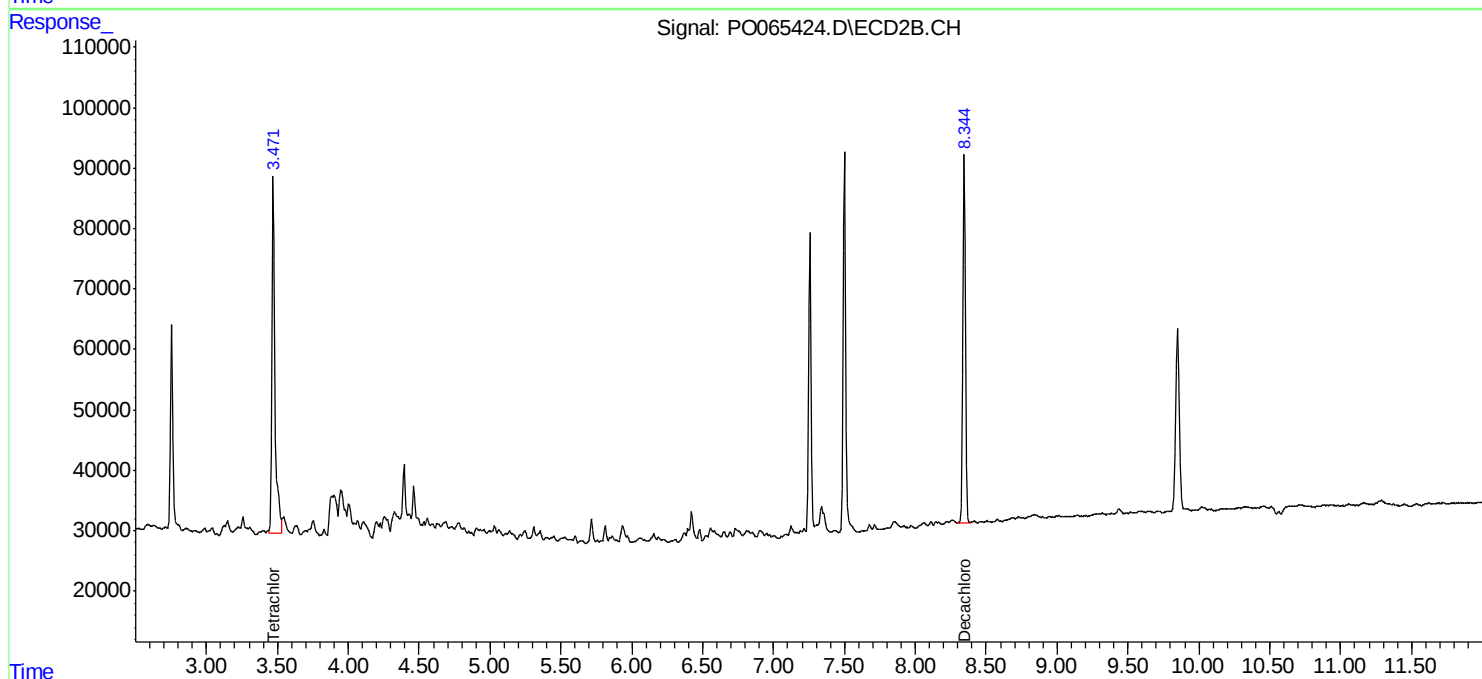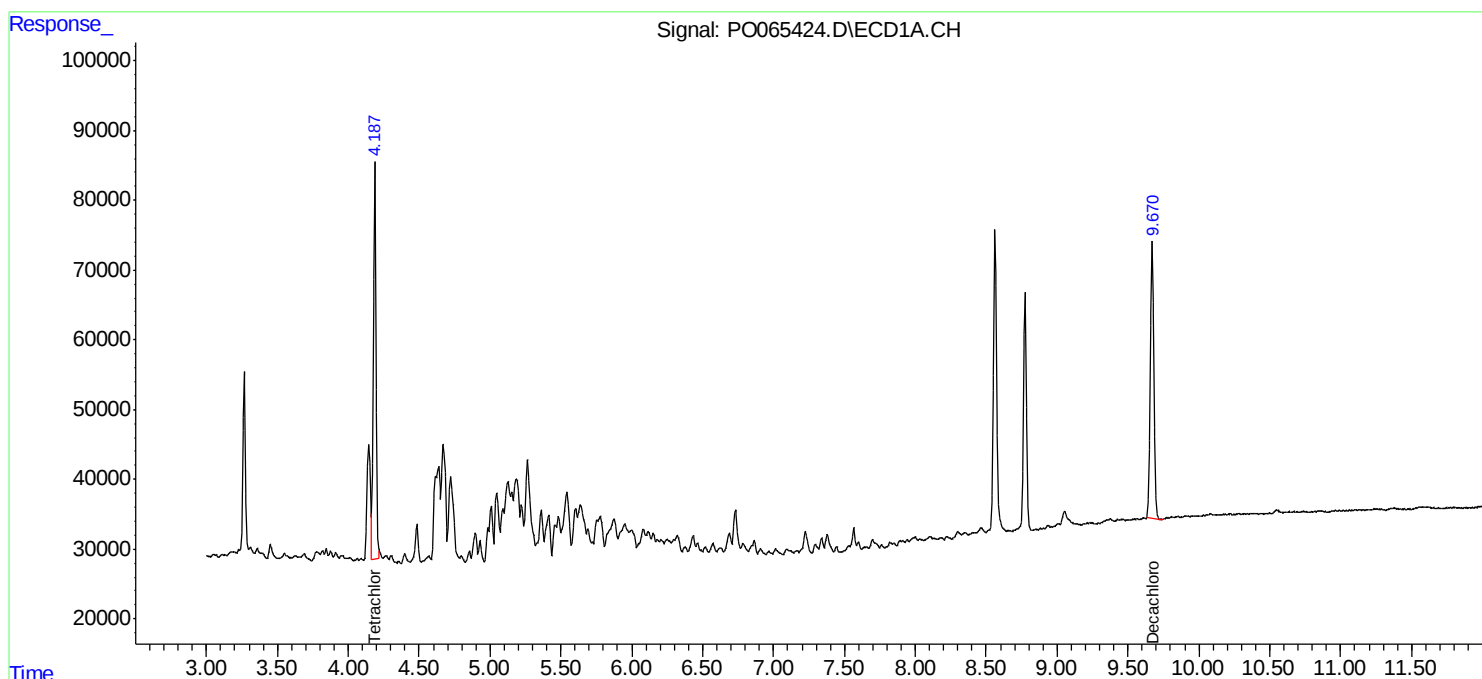

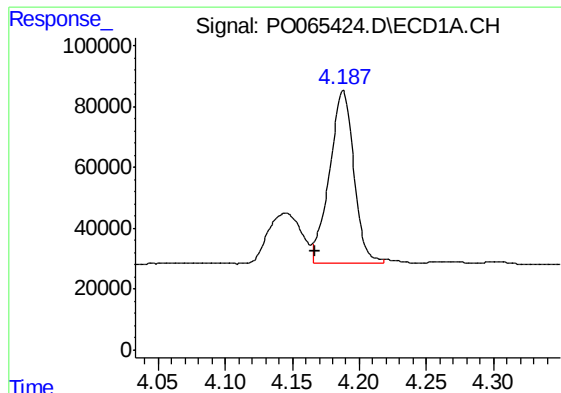


#1 Tetrachloro-m-xylene

R.T.: 4.187 min
Delta R.T.: 0.020 min
Response: 717983
Conc: 39.32 ng/ml m

Instrument :
ECD_O
ClientSampleId :
ODRE


Manual Integrations
APPROVED

mohammad
1/13/2020 10:19:02 AM

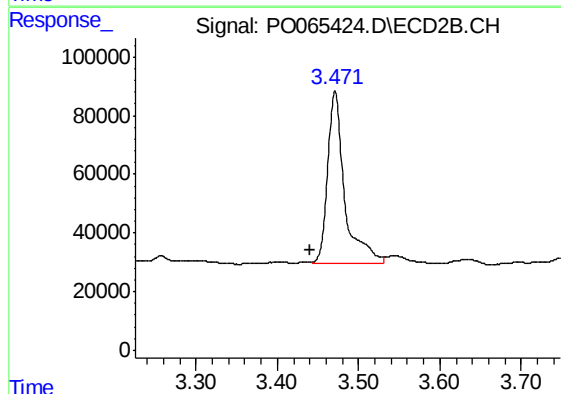


#1 Tetrachloro-m-xylene

R.T.: 3.471 min
Delta R.T.: 0.030 min
Response: 854206
Conc: 38.83 ng/ml m

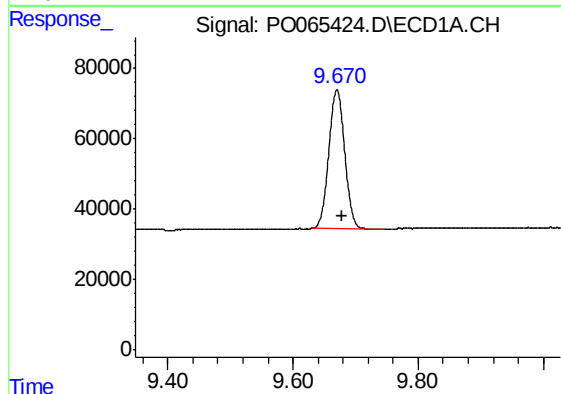

#2 Decachlorobiphenyl

R.T.: 9.670 min
Delta R.T.: -0.008 min
Response: 699315
Conc: 20.64 ng/ml

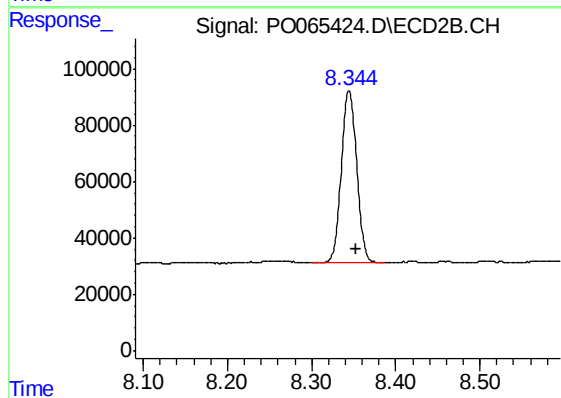

#2 Decachlorobiphenyl

R.T.: 8.345 min
Delta R.T.: -0.008 min
Response: 771354
Conc: 18.60 ng/ml