

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011022\
 Data File : P0084103.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2022 14:32
 Operator : AJ\MA
 Sample : N1054-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20220014-CAPE-1-COMP

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
 Supervised By :mohammad ahmed 01/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 02:41:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 10 11:26:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.043	4.036	1914621	402813	19.390m	19.699
2) SA Decachlor...	11.250	9.444	906161	259291	13.622	13.274

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011022\
Data File : P0084103.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2022 14:32
Operator : AJ\MA
Sample : N1054-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20220014-CAPE-1-COMP


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
Supervised By :mohammad ahmed 01/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 02:41:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 10 11:26:21 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

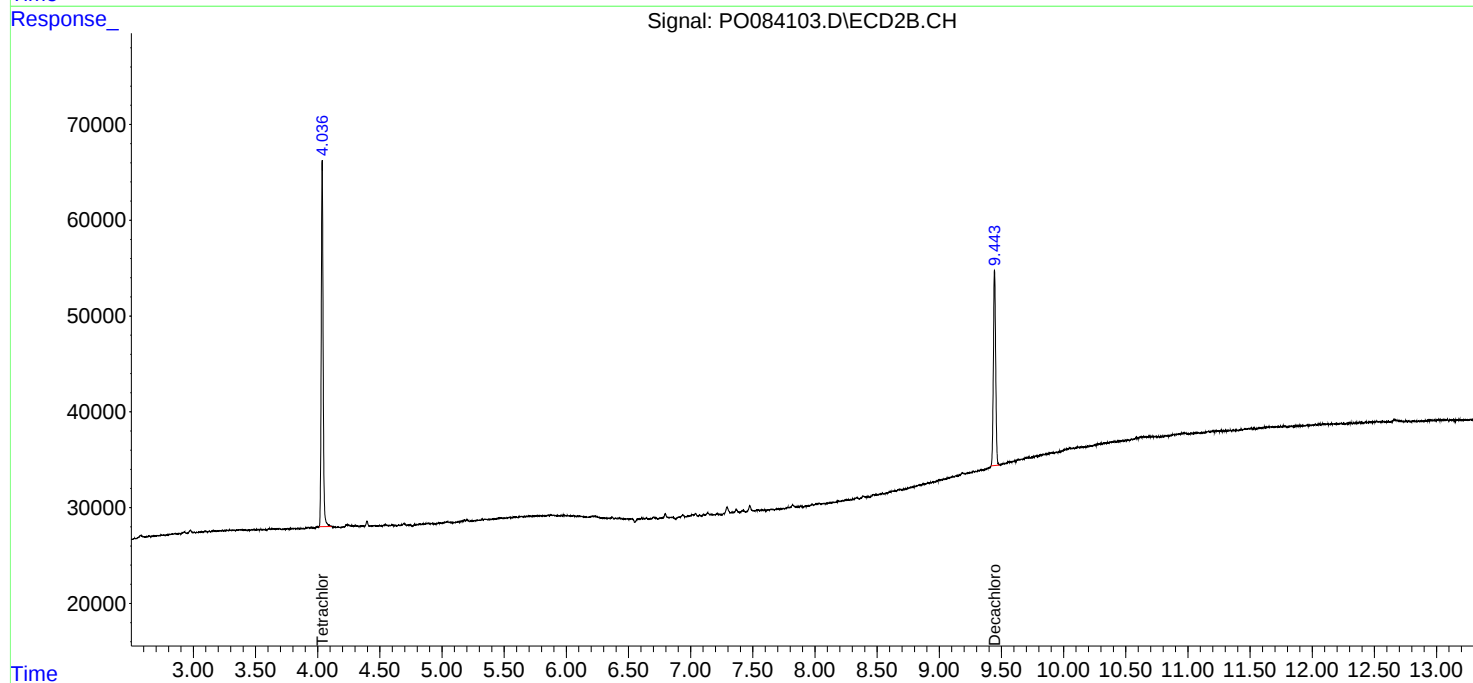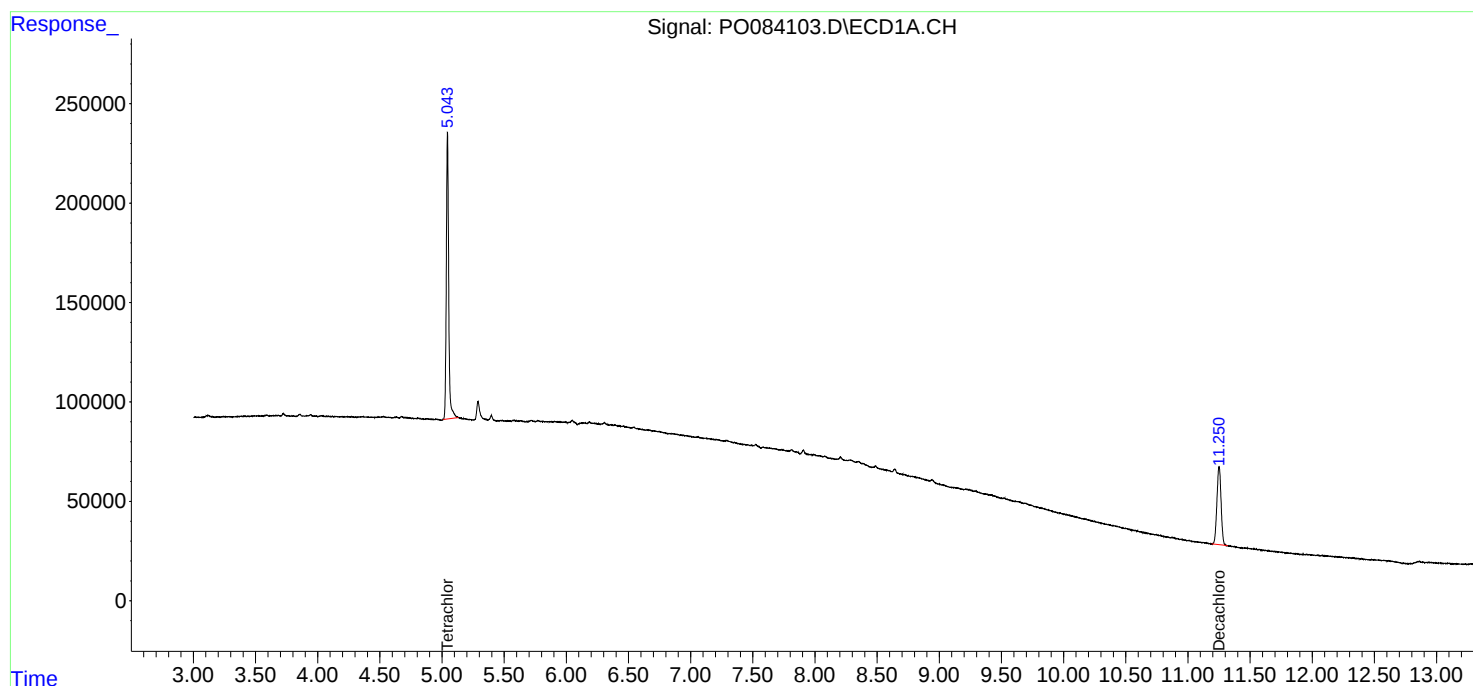

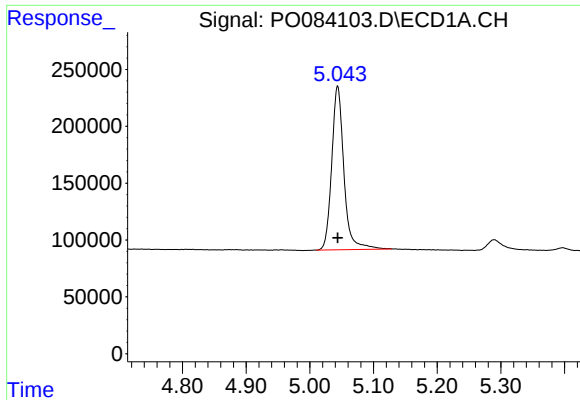


#1 Tetrachloro-m-xylene

R.T.: 5.043 min
Delta R.T.: 0.000 min
Response: 1914621
Conc: 19.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220014-CAPE-1-COMP


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
Supervised By :mohammad ahmed 01/13/2022

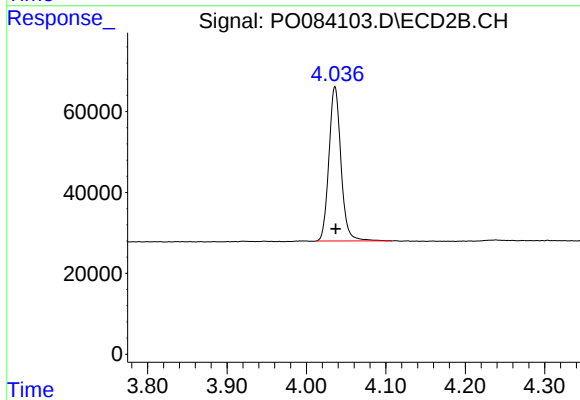


#1 Tetrachloro-m-xylene

R.T.: 4.036 min
Delta R.T.: -0.001 min
Response: 402813
Conc: 19.70 ng/ml

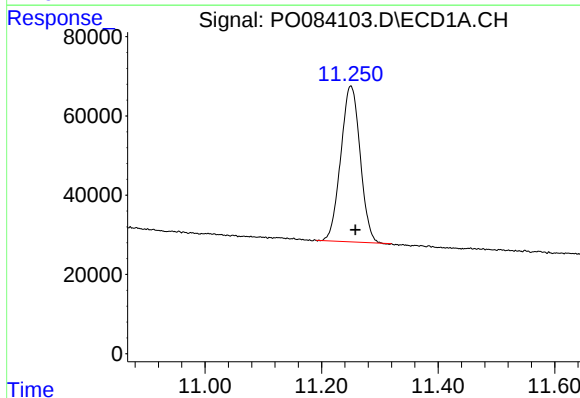

#2 Decachlorobiphenyl

R.T.: 11.250 min
Delta R.T.: -0.008 min
Response: 906161
Conc: 13.62 ng/ml

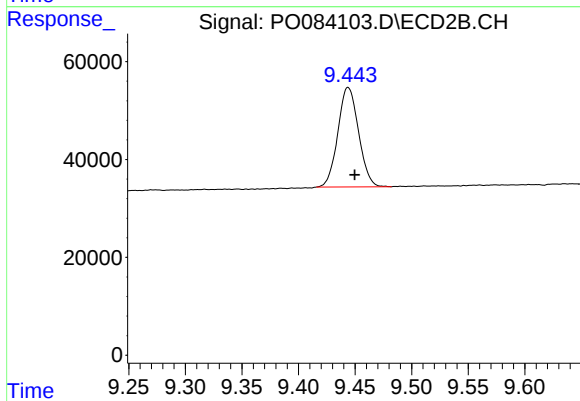

#2 Decachlorobiphenyl

R.T.: 9.444 min
Delta R.T.: -0.006 min
Response: 259291
Conc: 13.27 ng/ml