

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011022\
 Data File : P0084106.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2022 15:21
 Operator : AJ\MA
 Sample : N1054-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20220017-CAPE-4-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 02:42:29 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 10 11:26:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.045	4.036	2073058	424970	20.995	20.783
2) SA Decachlor...	11.249	9.445	1019841	291864	15.331	14.941

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011022\
Data File : P0084106.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2022 15:21
Operator : AJ\MA
Sample : N1054-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20220017-CAPE-4-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 02:42:29 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 10 11:26:21 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

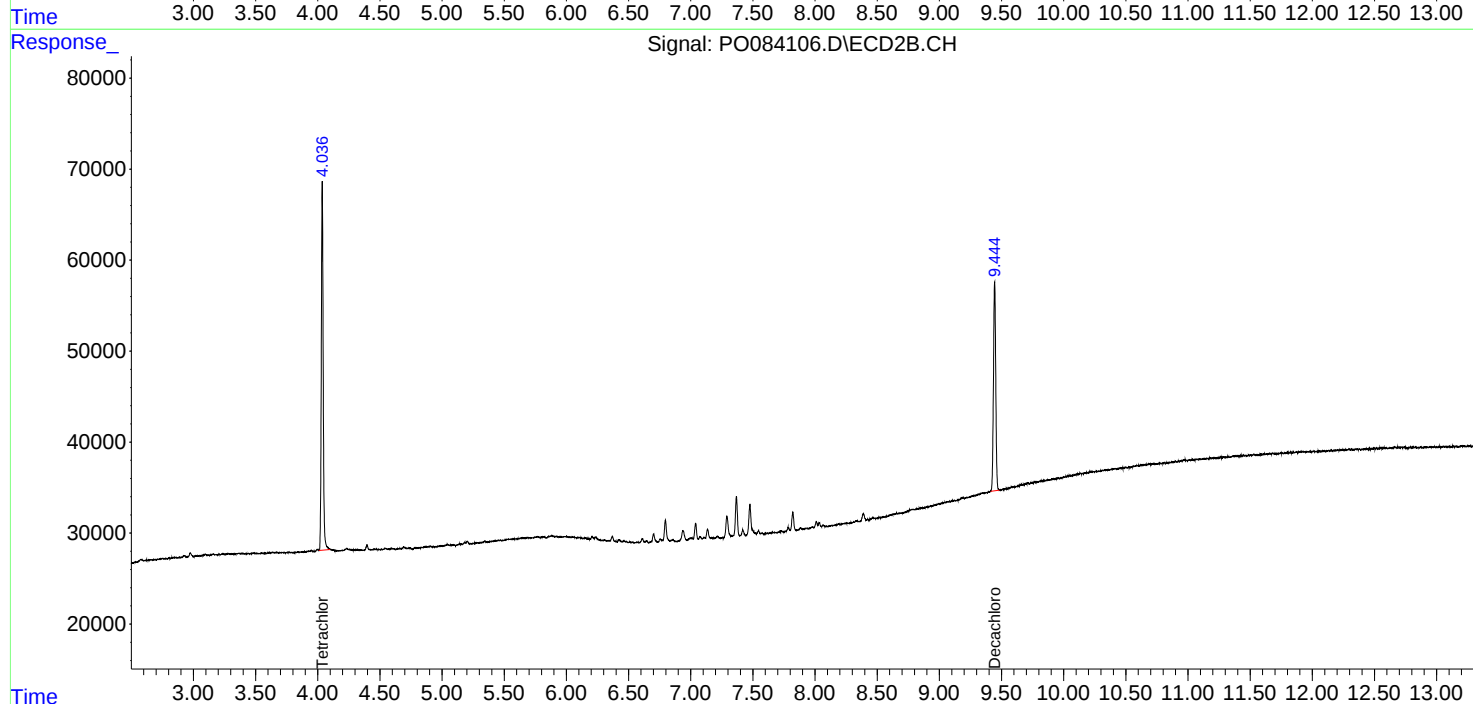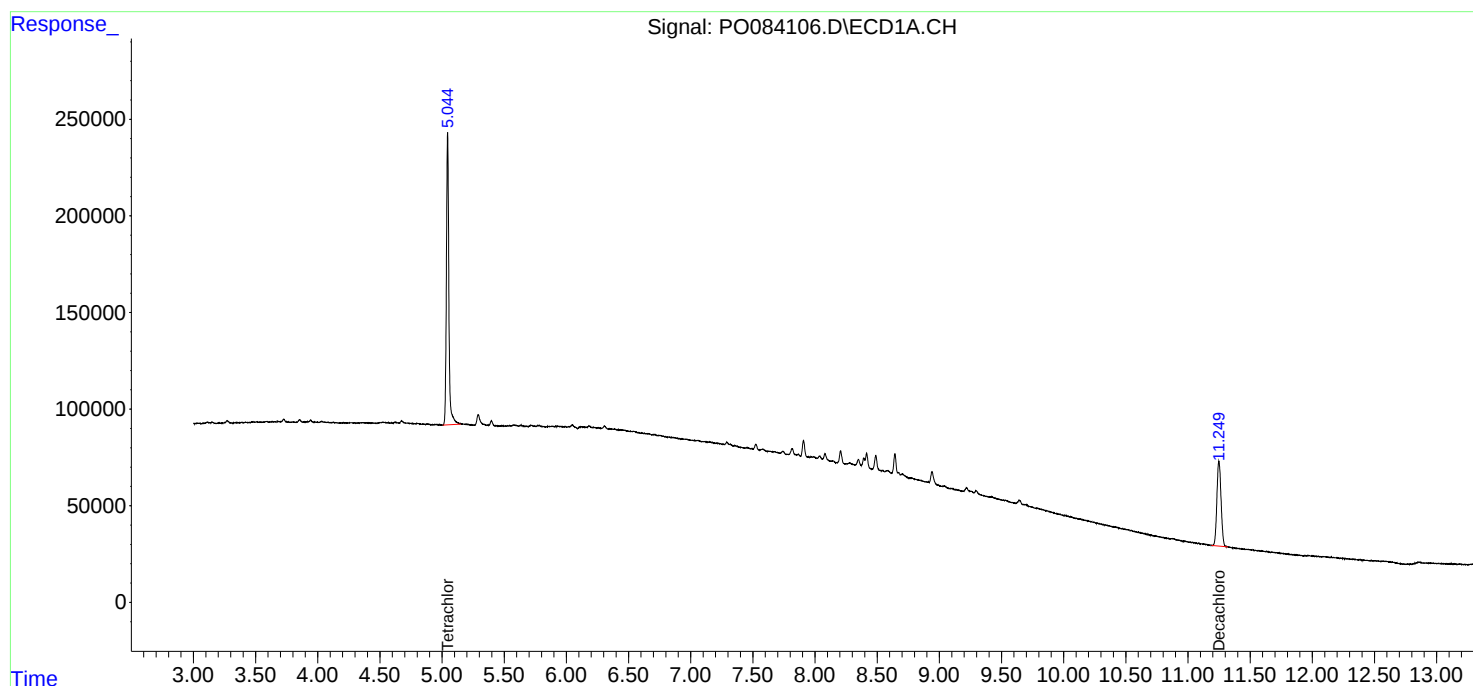


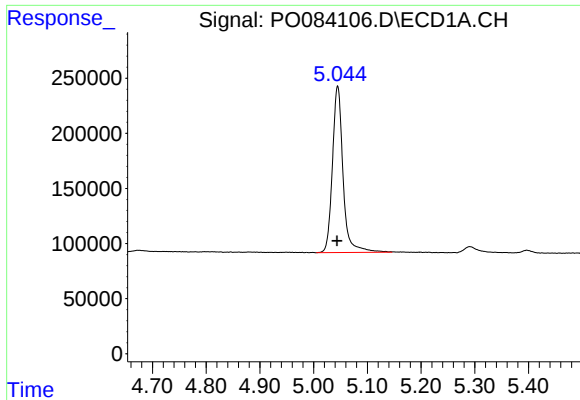

#1 Tetrachloro-m-xylene


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 2073058
Conc: 20.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
20220017-CAPE-4-COMP

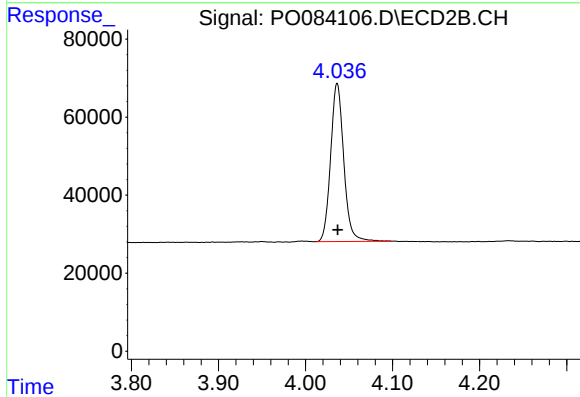


#1 Tetrachloro-m-xylene

R.T.: 4.036 min
Delta R.T.: 0.000 min
Response: 424970
Conc: 20.78 ng/ml

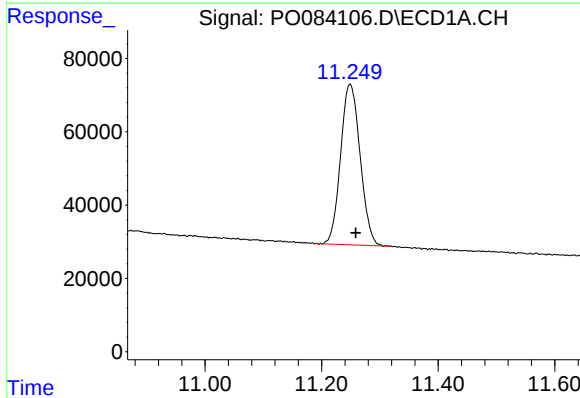

#2 Decachlorobiphenyl

R.T.: 11.249 min
Delta R.T.: -0.010 min
Response: 1019841
Conc: 15.33 ng/ml

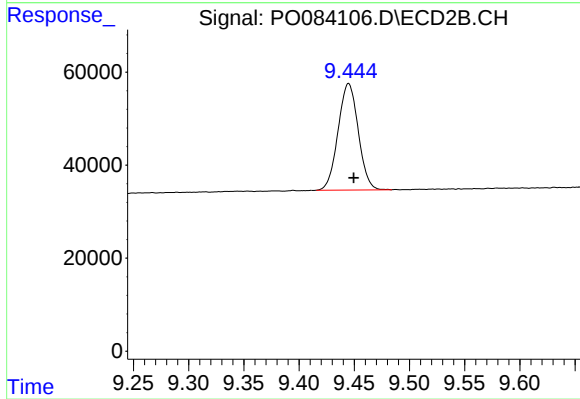

#2 Decachlorobiphenyl

R.T.: 9.445 min
Delta R.T.: -0.005 min
Response: 291864
Conc: 14.94 ng/ml