

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011022\
 Data File : P0084107.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2022 15:38
 Operator : AJ\MA
 Sample : N1054-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20211303-CAPE-5-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 02:42:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 10 11:26:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.045	4.037	1936979	396180	19.617	19.375
2) SA Decachlor...	11.249	9.445	902131	253315	13.562	12.968

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011022\
Data File : PO084107.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2022 15:38
Operator : AJ\MA
Sample : N1054-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20211303-CAPE-5-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 02:42:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 10 11:26:21 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

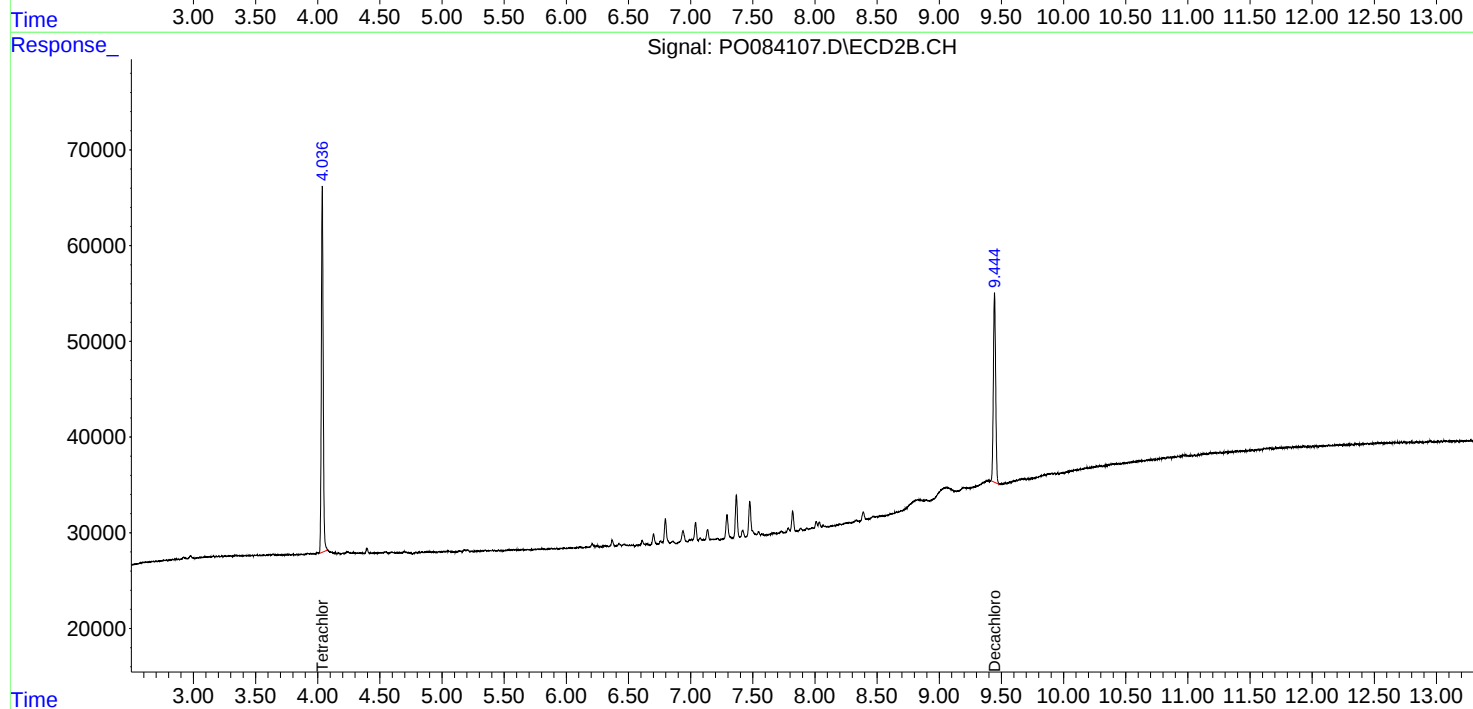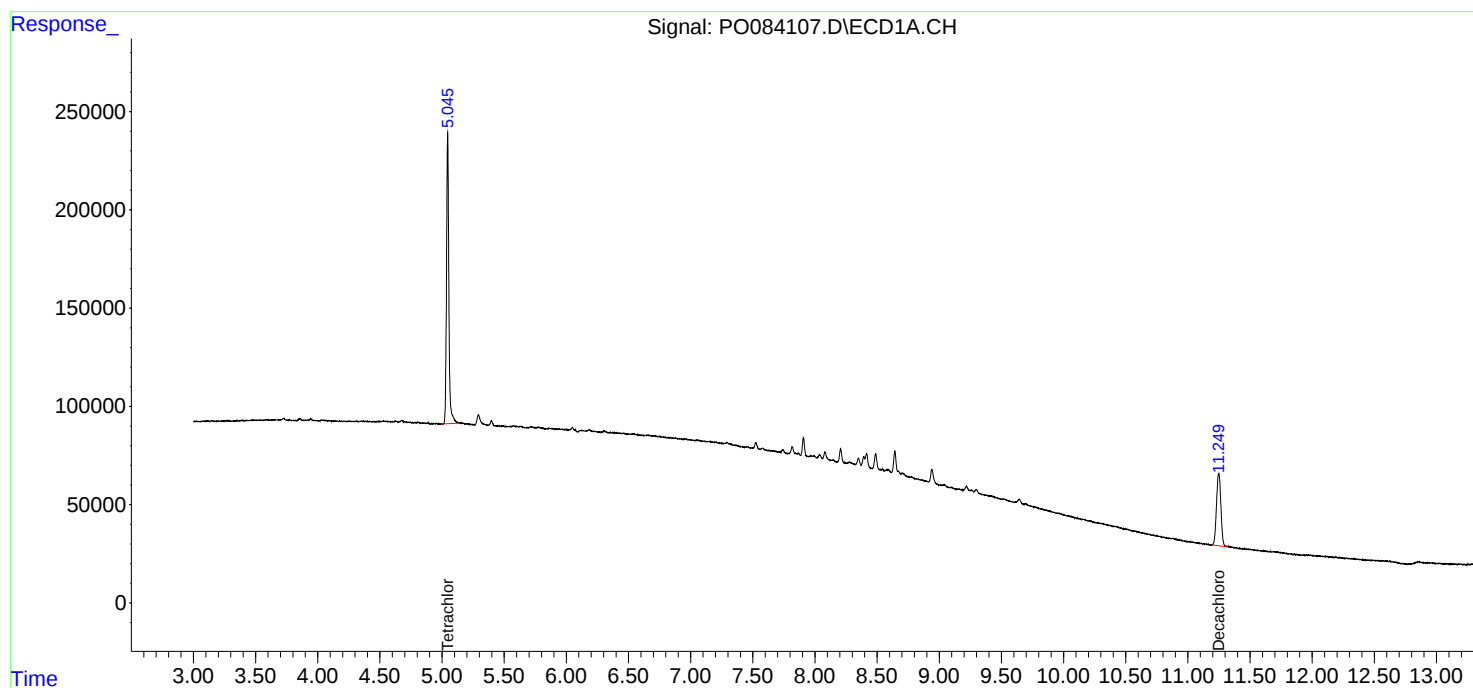


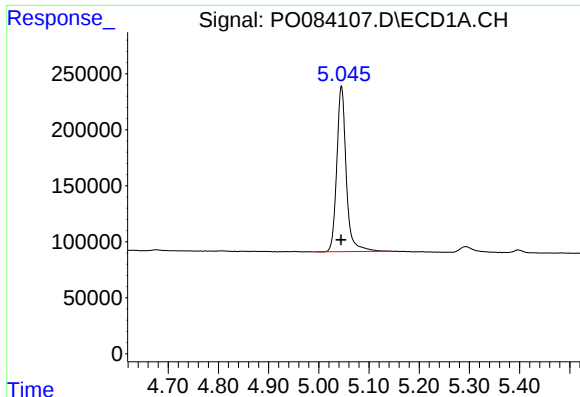

#1 Tetrachloro-m-xylene


R.T.: 5.045 min
Delta R.T.: 0.001 min
Response: 1936979
Conc: 19.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
20211303-CAPE-5-COMP

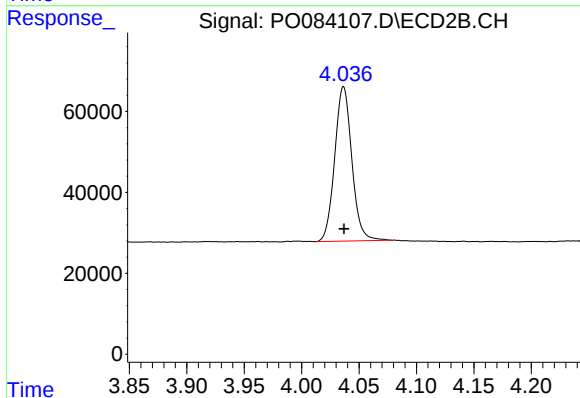


#1 Tetrachloro-m-xylene

R.T.: 4.037 min
Delta R.T.: 0.000 min
Response: 396180
Conc: 19.37 ng/ml

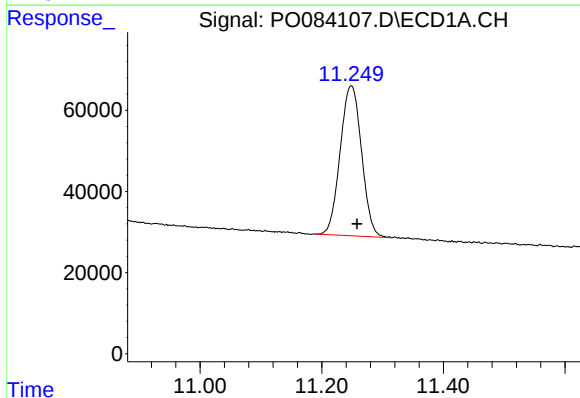

#2 Decachlorobiphenyl

R.T.: 11.249 min
Delta R.T.: -0.010 min
Response: 902131
Conc: 13.56 ng/ml

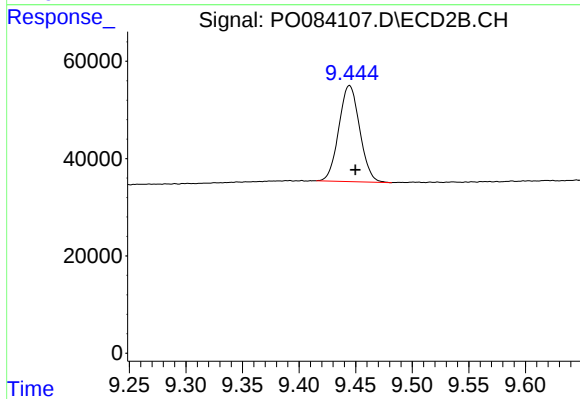

#2 Decachlorobiphenyl

R.T.: 9.445 min
Delta R.T.: -0.005 min
Response: 253315
Conc: 12.97 ng/ml