

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011022\
 Data File : P0084113.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jan 2022 17:51
 Operator : AJ\MA
 Sample : PB141940BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB141940BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 02:45:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 10 11:26:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.045	4.037	2043740	419597	20.698	20.520
2)	SA Decachlor...	11.248	9.444	1390683	406875	20.906	20.829

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011022\
Data File : PO084113.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jan 2022 17:51
Operator : AJ\MA
Sample : PB141940BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB141940BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 02:45:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 10 11:26:21 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

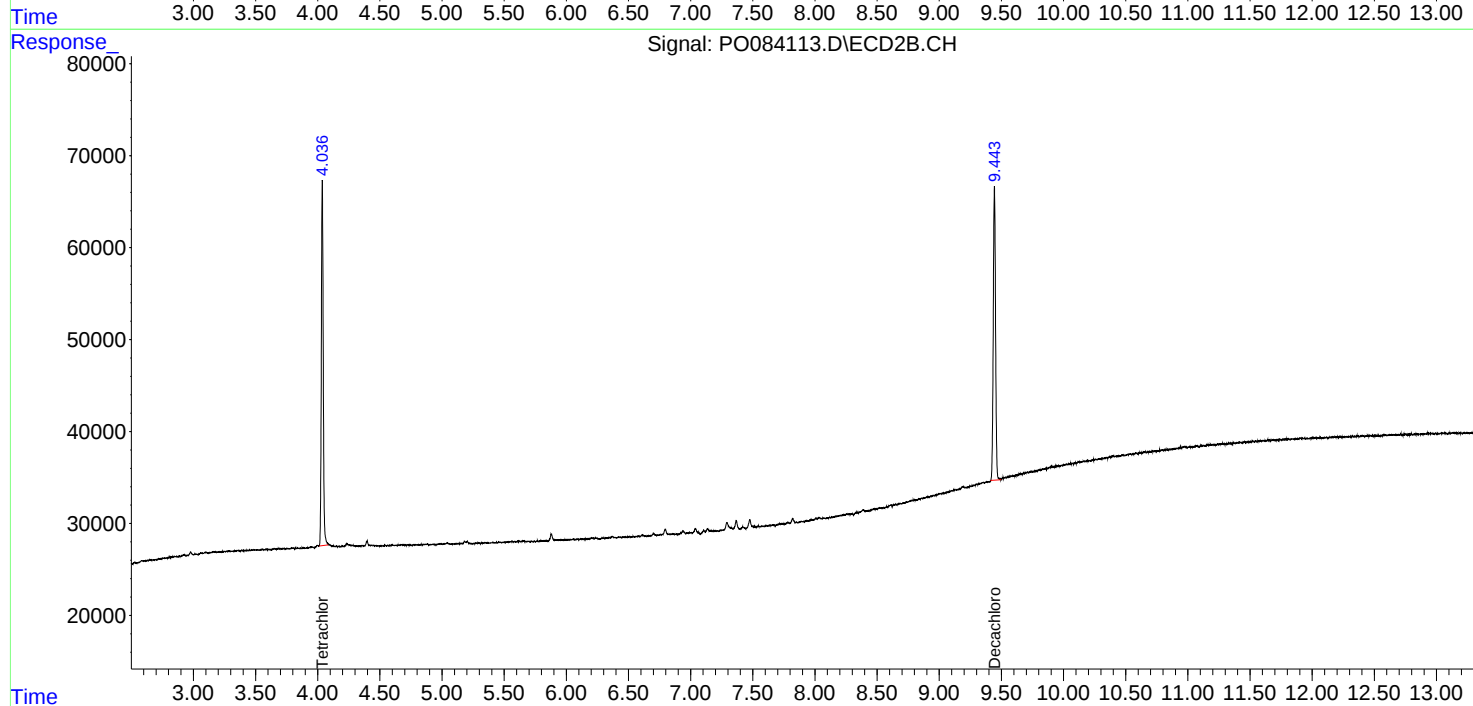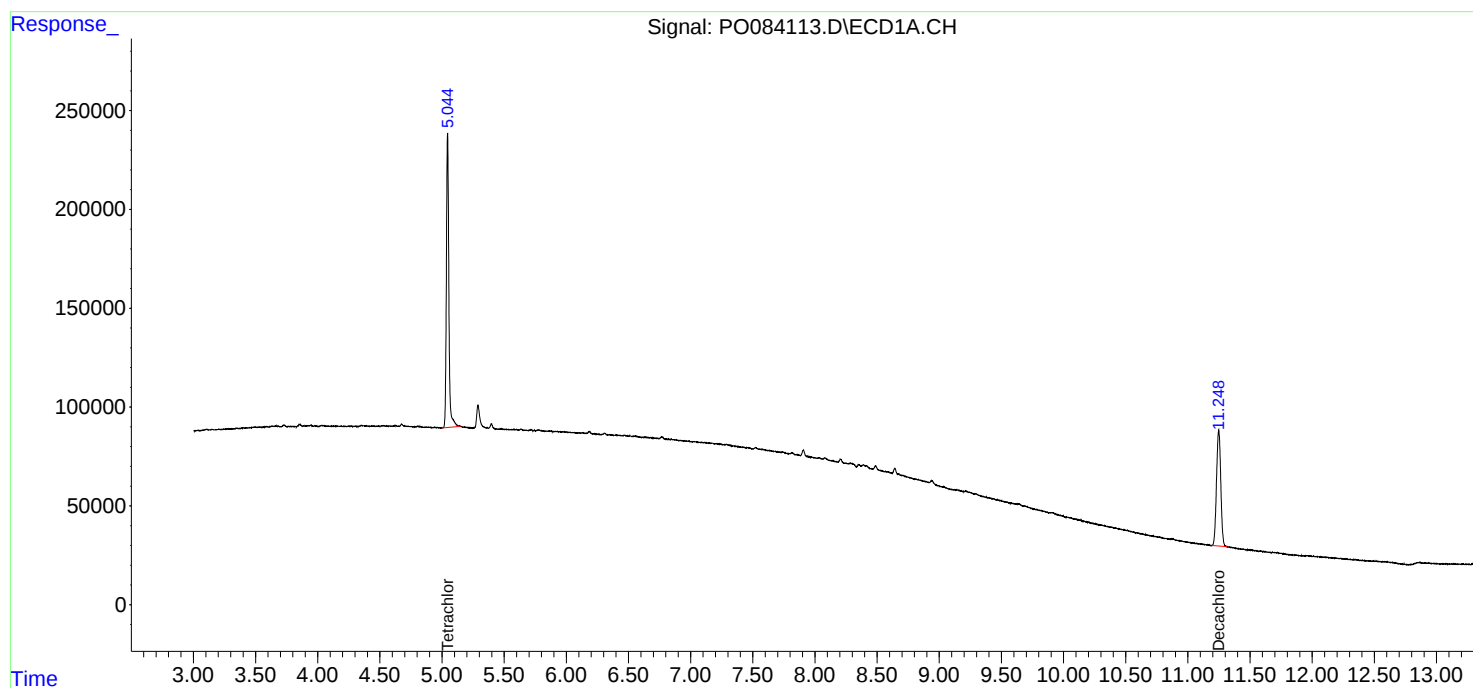


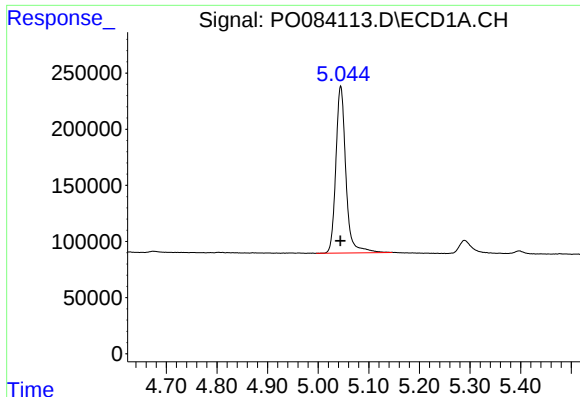

#1 Tetrachloro-m-xylene


R.T.: 5.045 min
Delta R.T.: 0.000 min
Response: 2043740
Conc: 20.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB141940BL

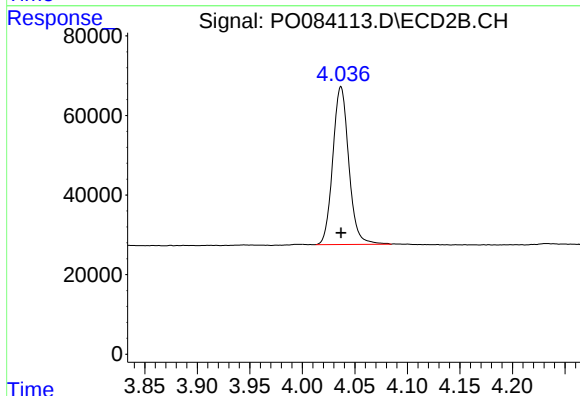


#1 Tetrachloro-m-xylene

R.T.: 4.037 min
Delta R.T.: 0.000 min
Response: 419597
Conc: 20.52 ng/ml

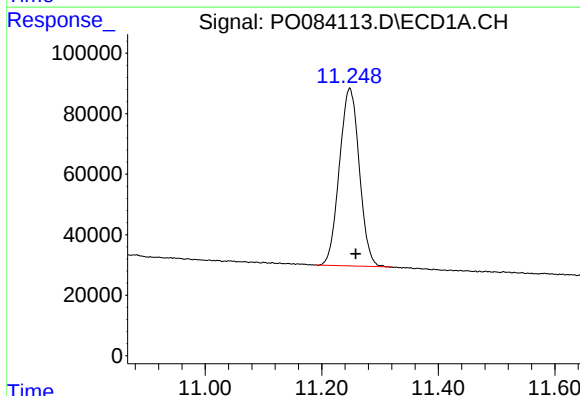

#2 Decachlorobiphenyl

R.T.: 11.248 min
Delta R.T.: -0.010 min
Response: 1390683
Conc: 20.91 ng/ml

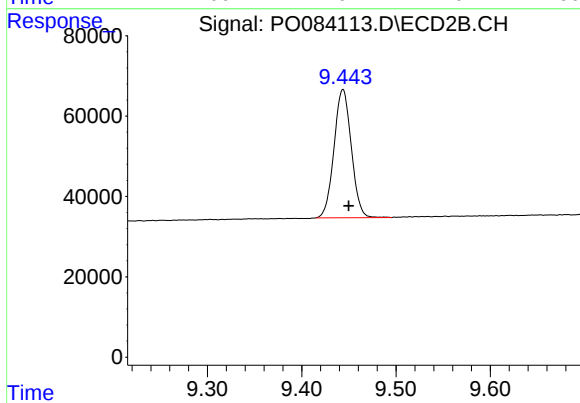

#2 Decachlorobiphenyl

R.T.: 9.444 min
Delta R.T.: -0.006 min
Response: 406875
Conc: 20.83 ng/ml