

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011022\
 Data File : P0084136.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jan 2022 00:43
 Operator : AJ\MA
 Sample : N1081-03
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OB-CS-13

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
 Supervised By :mohammad ahmed 01/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 02:55:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 10 11:26:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.045	4.036	1899194	420074	19.234m	20.543m
2) SA Decachlor...	11.255	9.445	1298229	329520	19.516	16.869

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011022\
Data File : PO084136.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jan 2022 00:43
Operator : AJ\MA
Sample : N1081-03
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OB-CS-13


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
Supervised By :mohammad ahmed 01/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 02:55:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO010722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 10 11:26:21 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

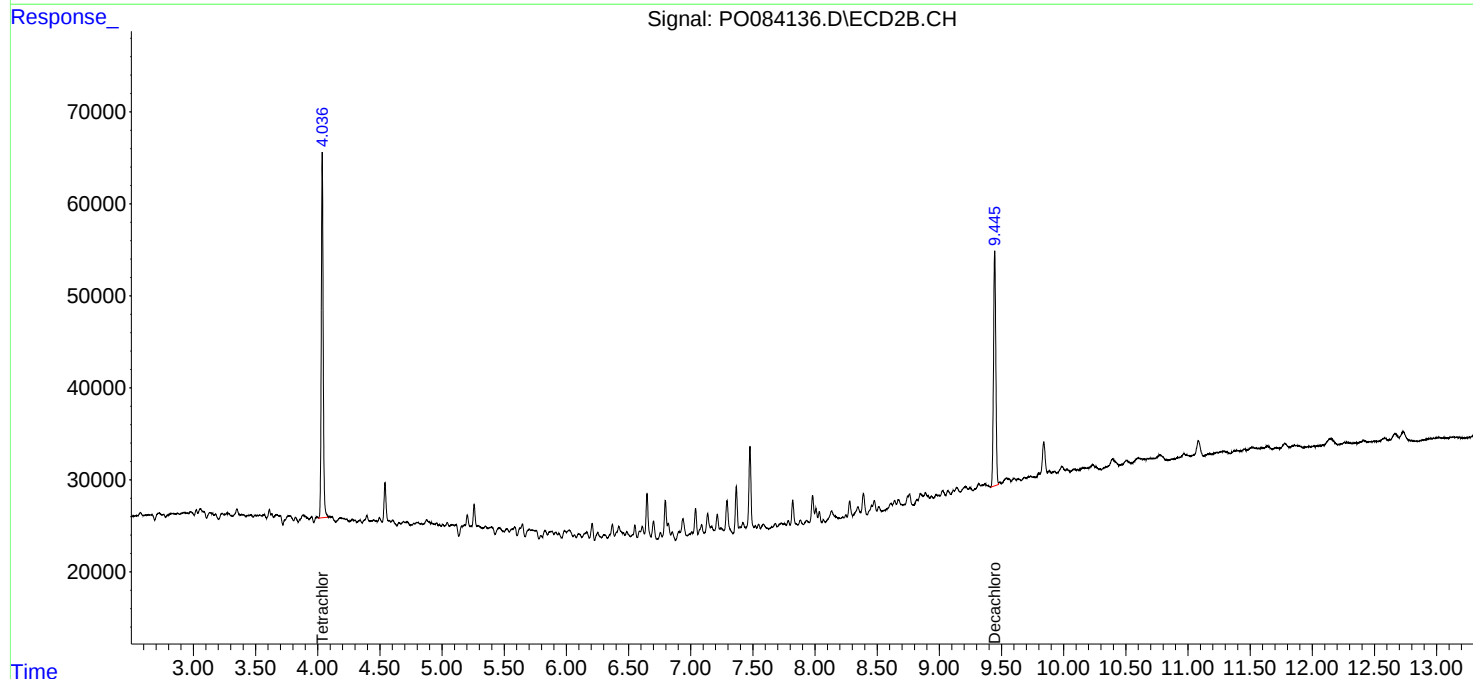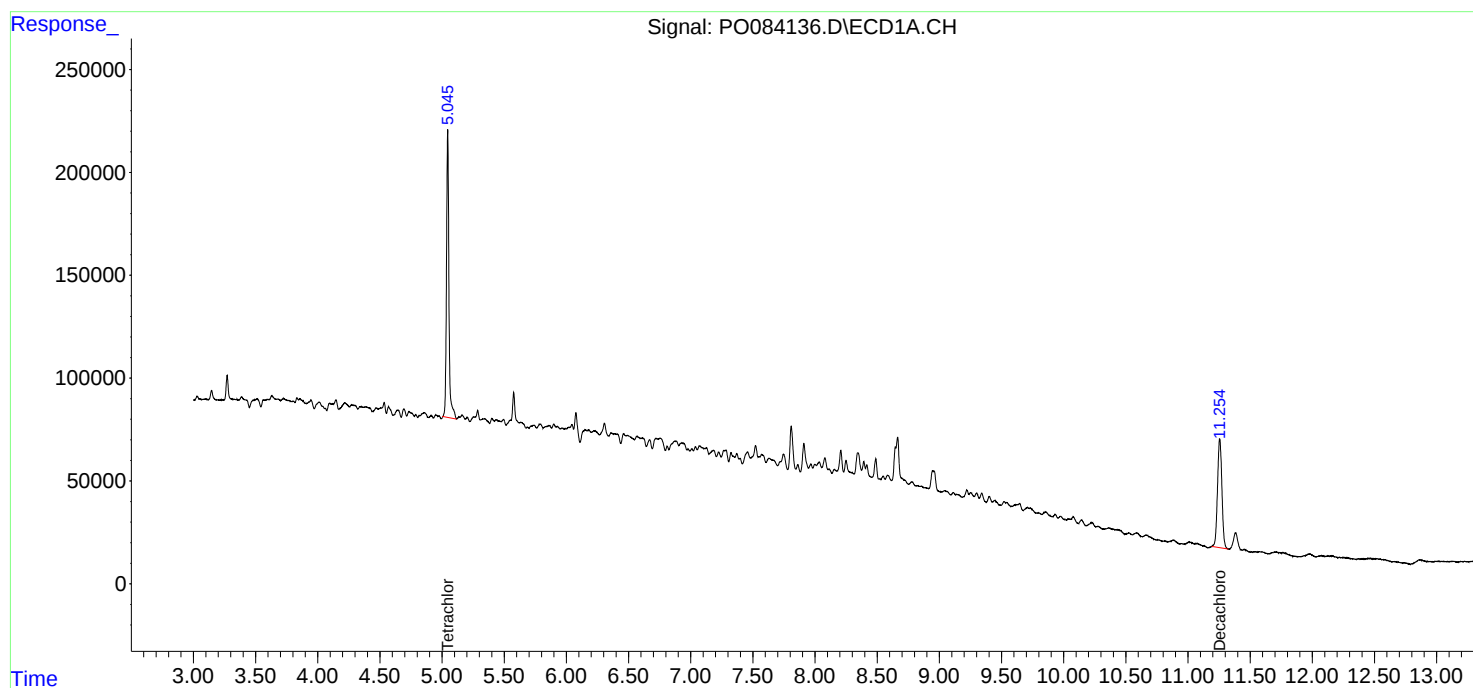

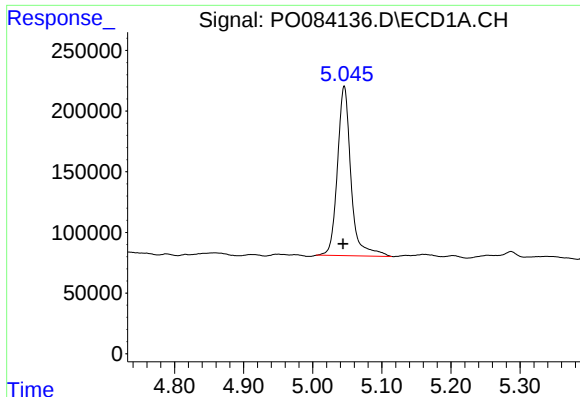


#1 Tetrachloro-m-xylene

R.T.: 5.045 min
Delta R.T.: 0.001 min
Response: 1899194
Conc: 19.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
OB-CS-13


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
Supervised By :mohammad ahmed 01/13/2022

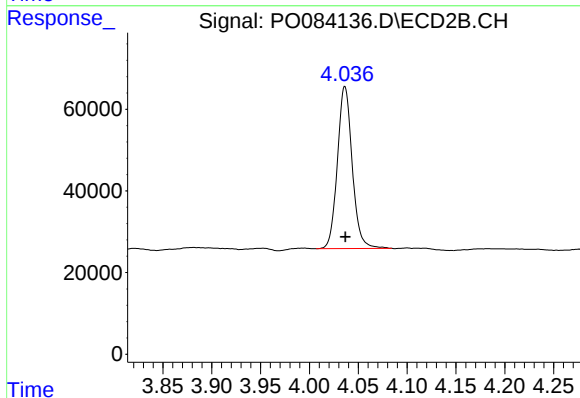


#1 Tetrachloro-m-xylene

R.T.: 4.036 min
Delta R.T.: -0.001 min
Response: 420074
Conc: 20.54 ng/ml m

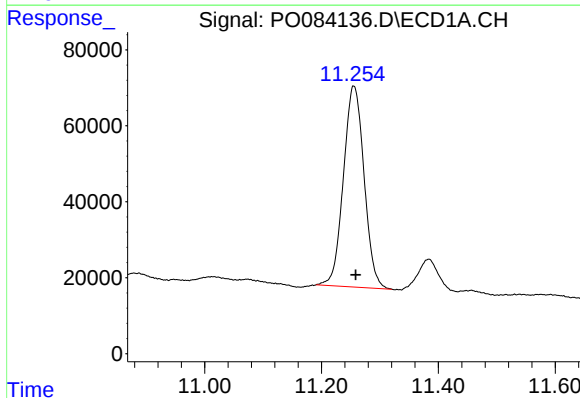

#2 Decachlorobiphenyl

R.T.: 11.255 min
Delta R.T.: -0.003 min
Response: 1298229
Conc: 19.52 ng/ml

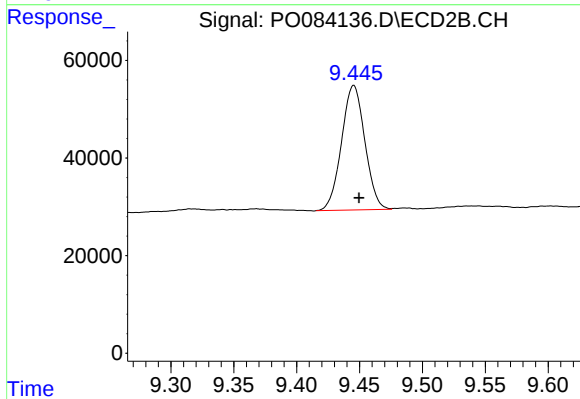

#2 Decachlorobiphenyl

R.T.: 9.445 min
Delta R.T.: -0.004 min
Response: 329520
Conc: 16.87 ng/ml