

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011022\
 Data File : P0084137.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jan 2022 00:59
 Operator : AJ\MA
 Sample : N1081-04
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OB-CS-14

Manual Integrations
 APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
 Supervised By :mohammad ahmed 01/13/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 11 02:55:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jan 10 11:26:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.044	4.036	1962644	436601	19.876	21.352
2) SA Decachlor...	11.255	9.444	1338755	340389	20.126	17.426
Target Compounds						
26) L6 AR-1254-1	7.290	6.207	46484	26404	13.261m	22.135 #
27) L6 AR-1254-2	7.523	6.369	105936	26695	19.827m	25.217m#
28) L6 AR-1254-3	7.909	6.796	227261	57317	40.362m	33.553m
29) L6 AR-1254-4	8.206	7.038	181252	40108	44.233m	37.185m
30) L6 AR-1254-5	8.645	7.476	253961	77601	59.191m	51.979m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011022\
Data File : P0084137.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jan 2022 00:59
Operator : AJ\MA
Sample : N1081-04
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OB-CS-14


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
Supervised By :mohammad ahmed 01/13/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 11 02:55:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0010722.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jan 10 11:26:21 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

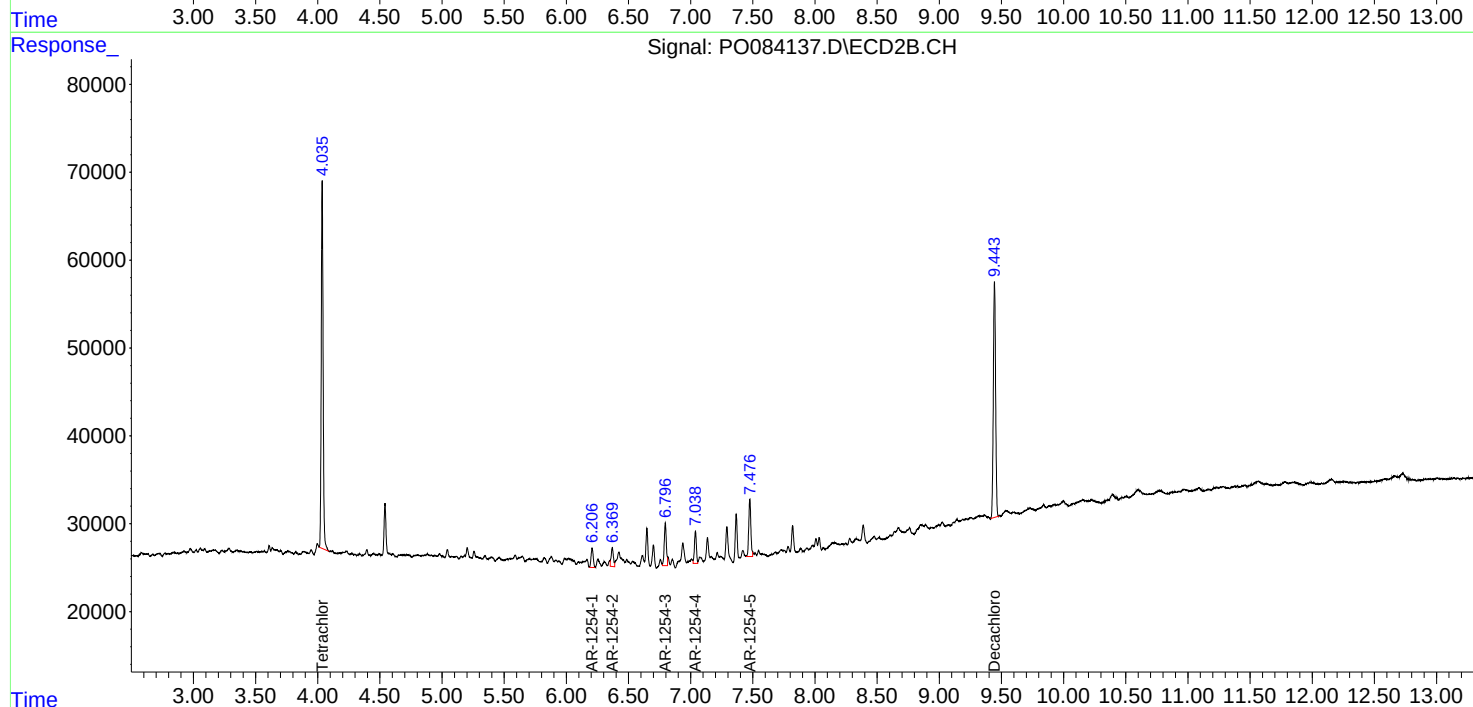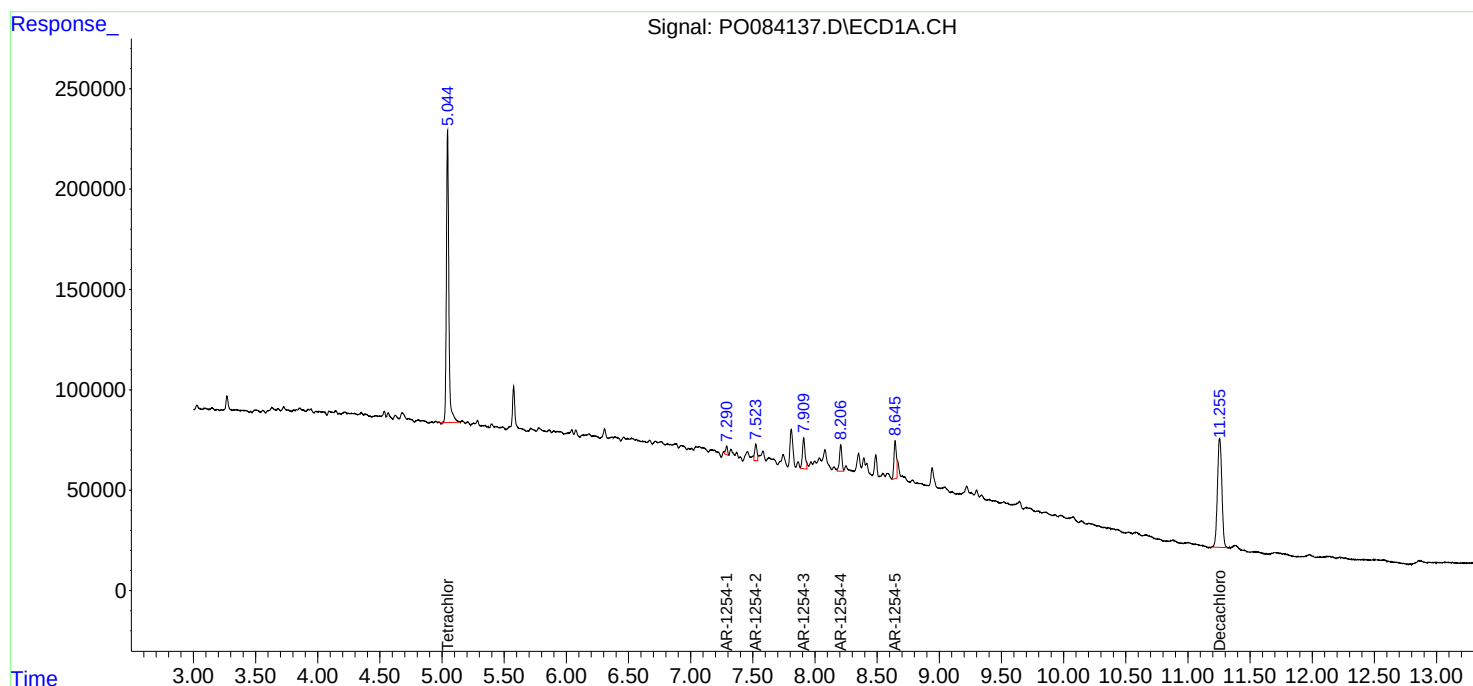

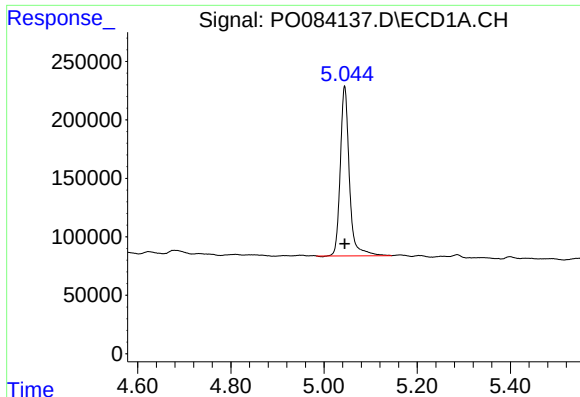


#1 Tetrachloro-m-xylene

R.T.: 5.044 min
Delta R.T.: 0.000 min
Response: 1962644
Conc: 19.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
OB-CS-14


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
Supervised By :mohammad ahmed 01/13/2022

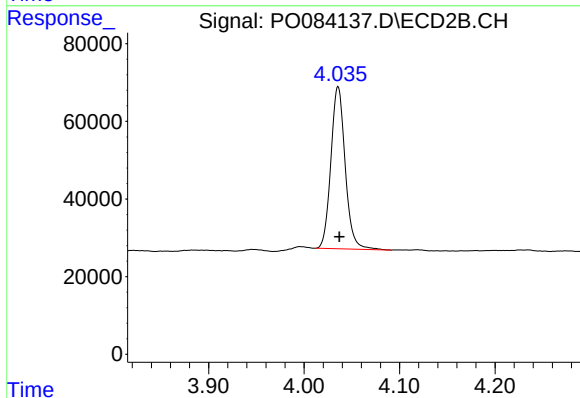


#1 Tetrachloro-m-xylene

R.T.: 4.036 min
Delta R.T.: -0.001 min
Response: 436601
Conc: 21.35 ng/ml

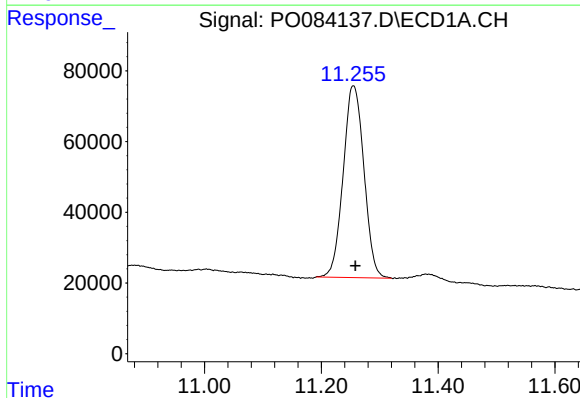


#2 Decachlorobiphenyl

R.T.: 11.255 min
Delta R.T.: -0.004 min
Response: 1338755
Conc: 20.13 ng/ml

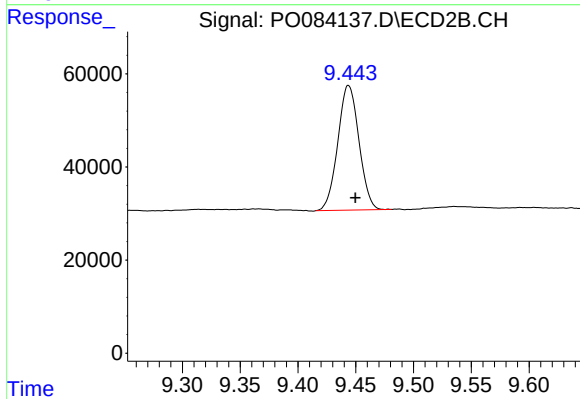

#2 Decachlorobiphenyl

R.T.: 9.444 min
Delta R.T.: -0.006 min
Response: 340389
Conc: 17.43 ng/ml

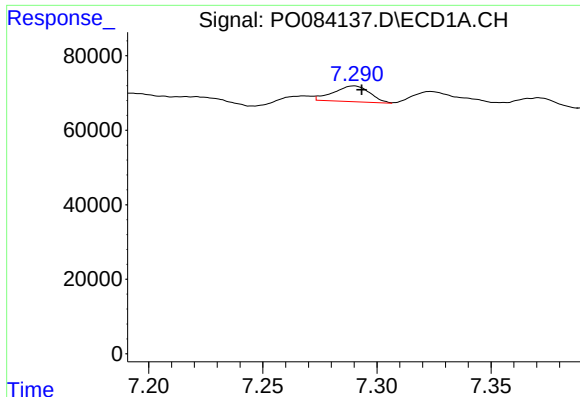


#26 AR-1254-1

R.T.: 7.290 min
Delta R.T.: -0.003 min
Response: 46484
Conc: 13.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
OB-CS-14


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
Supervised By :mohammad ahmed 01/13/2022

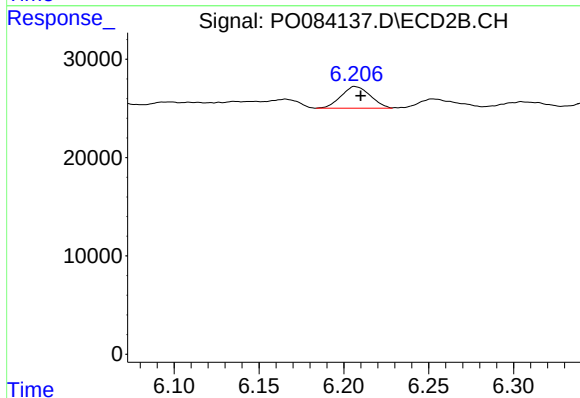


#26 AR-1254-1

R.T.: 6.207 min
Delta R.T.: -0.003 min
Response: 26404
Conc: 22.14 ng/ml

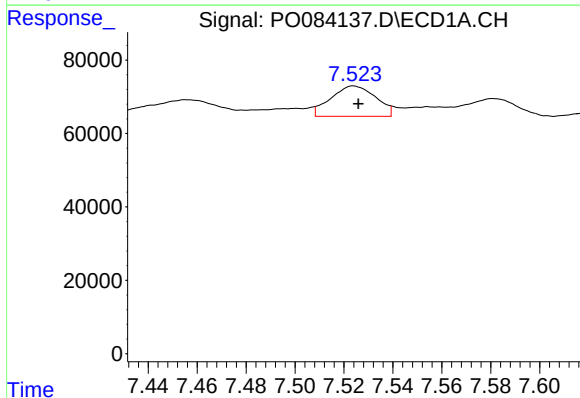


#27 AR-1254-2

R.T.: 7.523 min
Delta R.T.: -0.003 min
Response: 105936
Conc: 19.83 ng/ml m

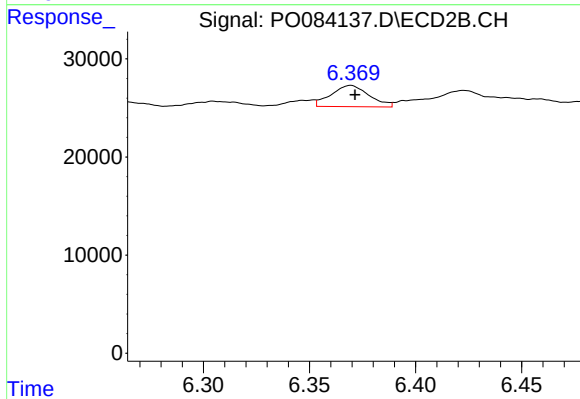

#27 AR-1254-2

R.T.: 6.369 min
Delta R.T.: -0.002 min
Response: 26695
Conc: 25.22 ng/ml m

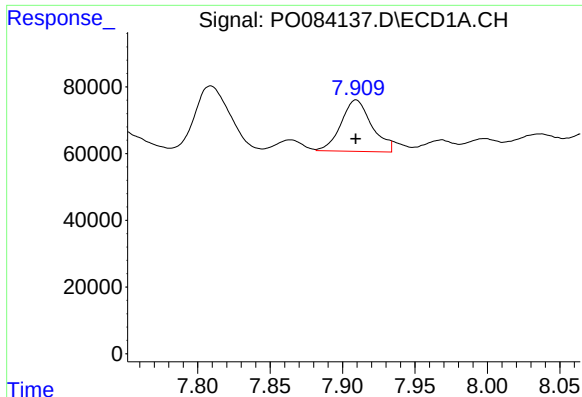


#28 AR-1254-3

R.T.: 7.909 min
Delta R.T.: 0.000 min
Response: 227261
Conc: 40.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
OB-CS-14


Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
Supervised By :mohammad ahmed 01/13/2022

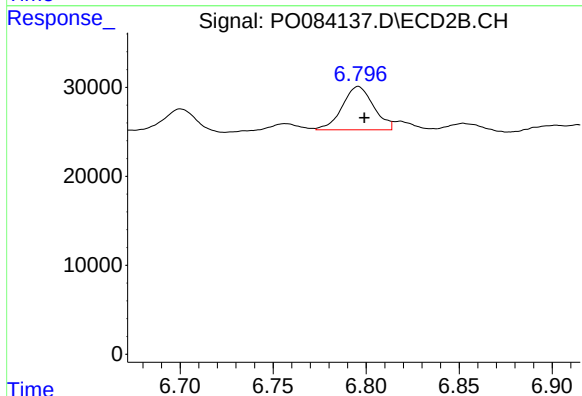


#28 AR-1254-3

R.T.: 6.796 min
Delta R.T.: -0.004 min
Response: 57317
Conc: 33.55 ng/ml m

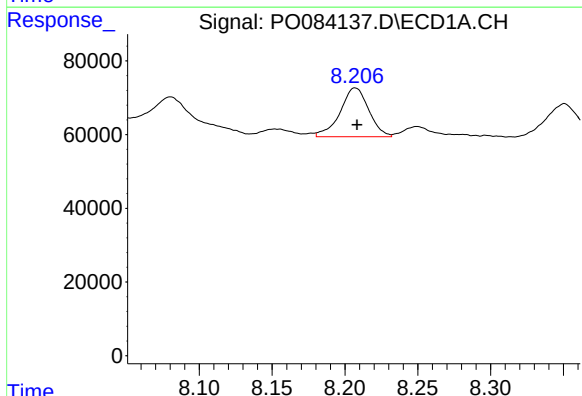


#29 AR-1254-4

R.T.: 8.206 min
Delta R.T.: -0.002 min
Response: 181252
Conc: 44.23 ng/ml m

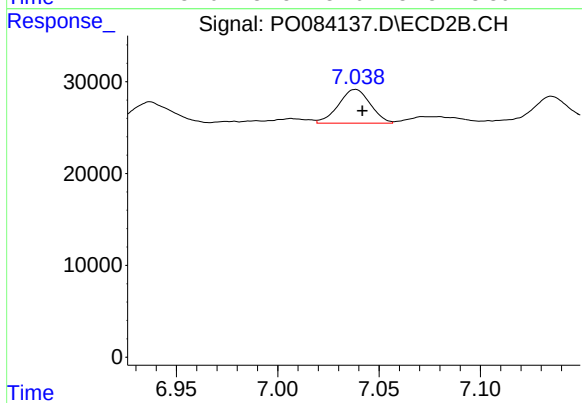

#29 AR-1254-4

R.T.: 7.038 min
Delta R.T.: -0.004 min
Response: 40108
Conc: 37.18 ng/ml m

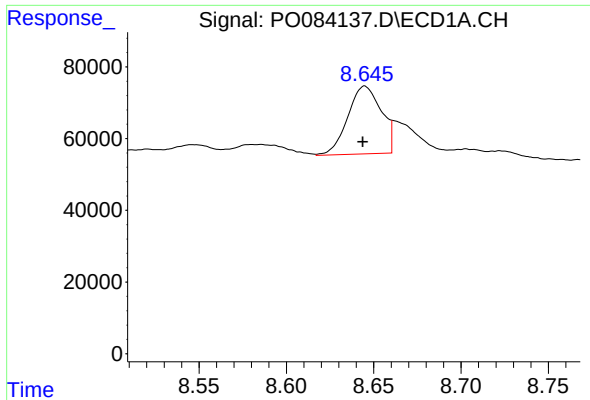


#30 AR-1254-5

R.T.: 8.645 min
Delta R.T.: 0.000 min
Response: 253961
Conc: 59.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
OB-CS-14

Manual Integrations
APPROVED

Reviewed By :Ankita Jodhani 01/13/2022
Supervised By :mohammad ahmed 01/13/2022

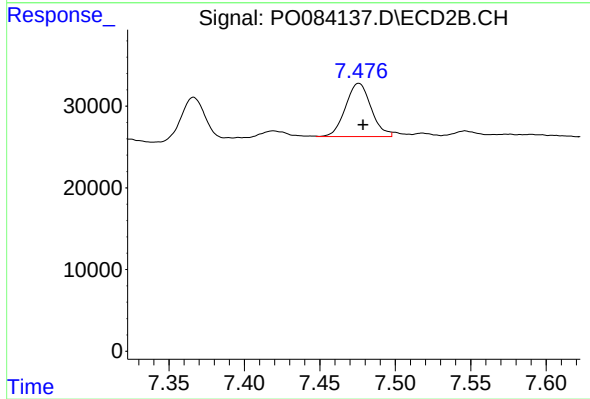

#30 AR-1254-5

R.T.: 7.476 min
Delta R.T.: -0.003 min
Response: 77601
Conc: 51.98 ng/ml m