

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011121\
 Data File : P0074470.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Jan 2021 15:28
 Operator : AJ/MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 06:08:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3)	L1	AR-1016-1	6.261	0.000	22863	0	5.592 N.D. #
4)	L1	AR-1016-2	6.261f	0.000	22863	0	4.015 N.D. #
13)	L3	AR-1232-3	6.261f	0.000	22863	0	9.475 N.D. #
16)	L4	AR-1242-1	6.261	0.000	22863	0	7.100 N.D. #
17)	L4	AR-1242-2	6.261f	0.000	22863	0	5.066 N.D. #
21)	L5	AR-1248-1	6.261	0.000	22863	0	9.497 N.D. #
30)	L6	AR-1254-5	8.533f	0.000	1249	0	0.215 N.D. #
32)	L7	AR-1260-2	8.233f	0.000	45506	0	6.690 N.D. #
33)	L7	AR-1260-3	0.000	7.171	0	48182	N.D. 13.371 #
34)	L7	AR-1260-4	8.812	0.000	5718	0	1.045 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011121\
Data File : P0074470.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jan 2021 15:28
Operator : AJ/MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 06:08:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

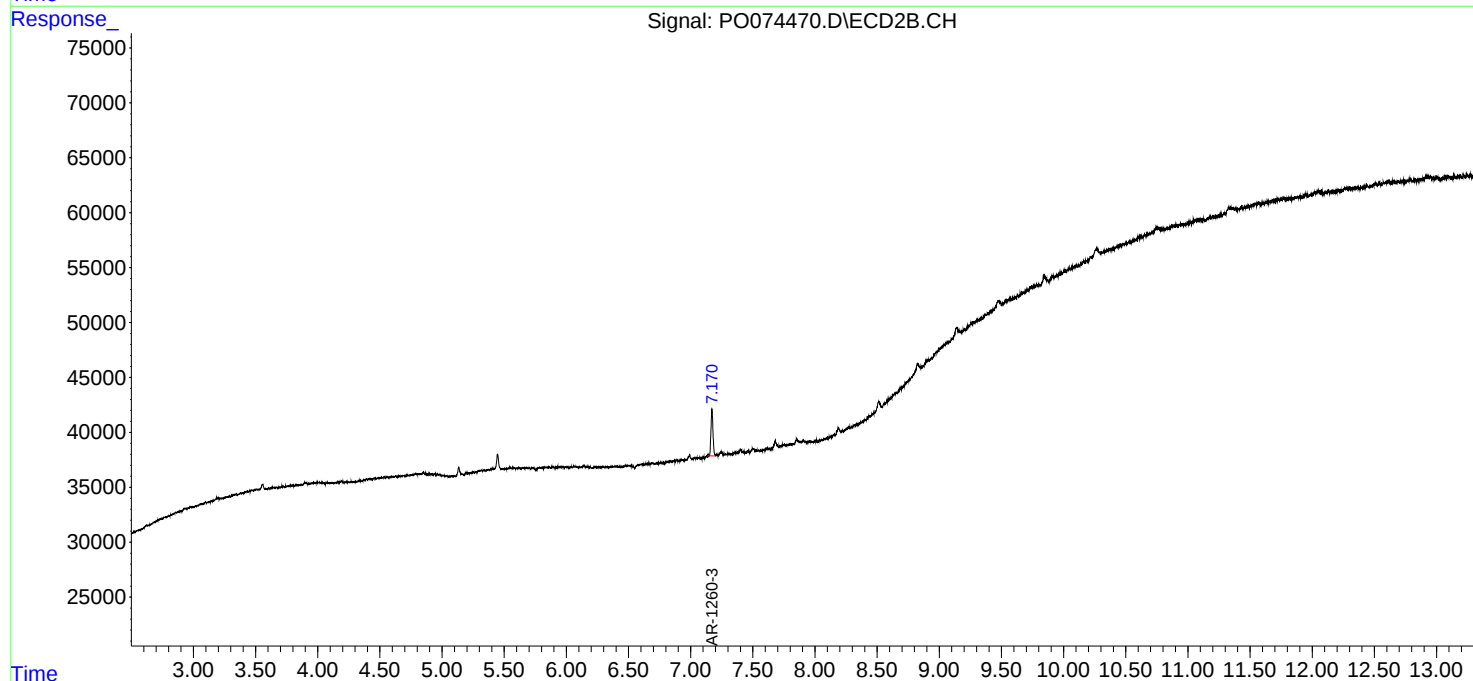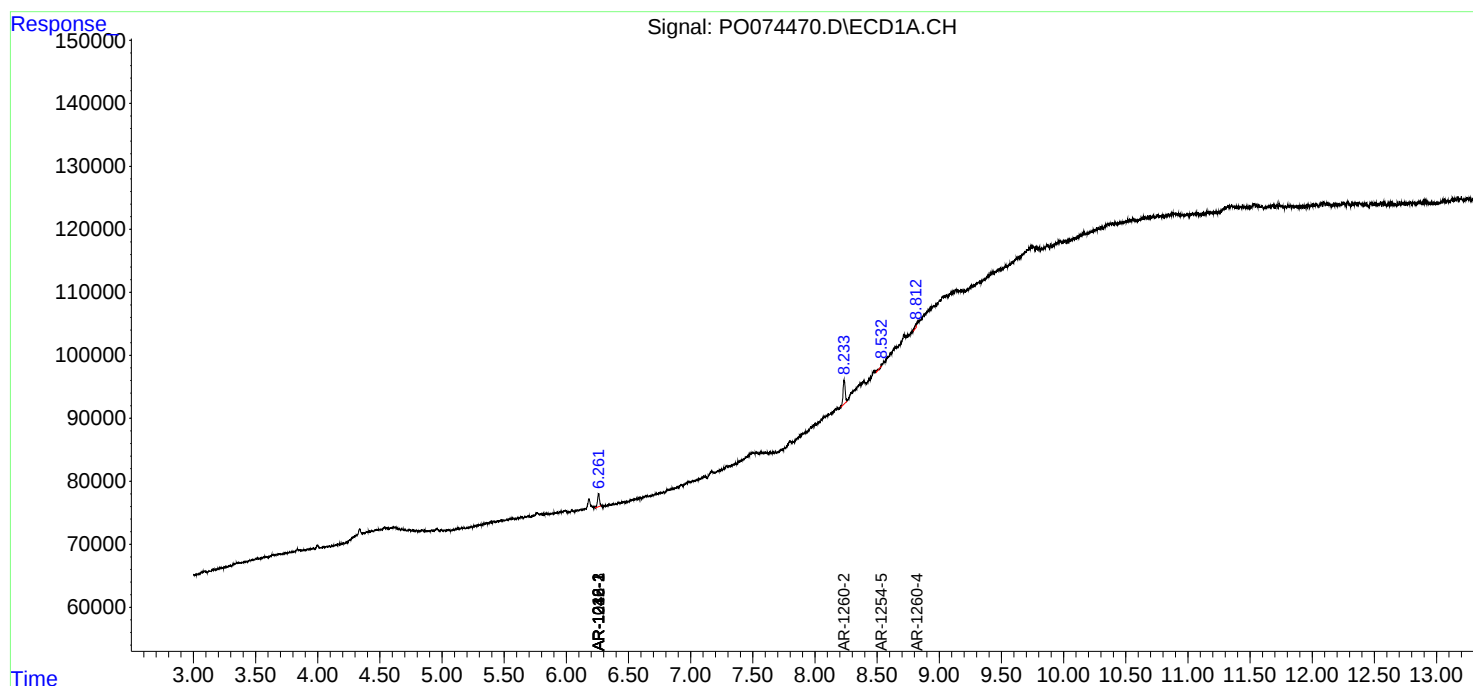


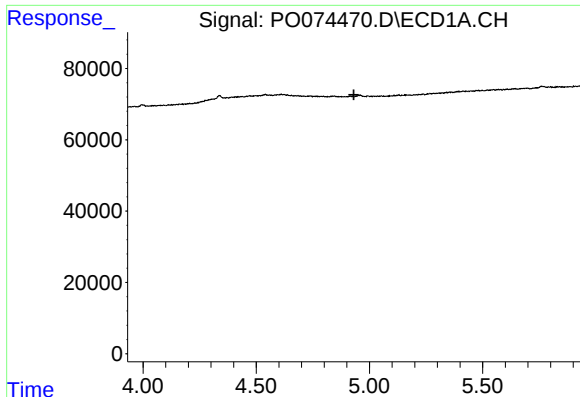

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

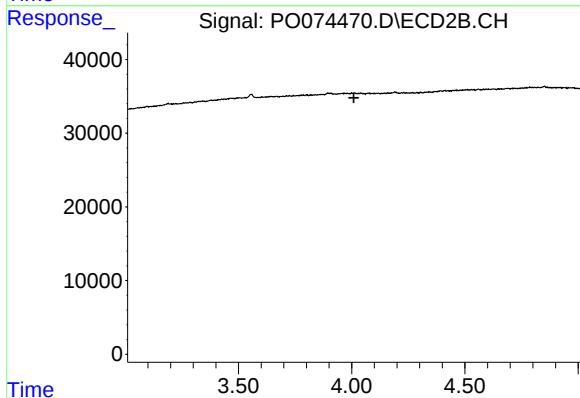


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.010 min
Response: 0
Conc: N.D.

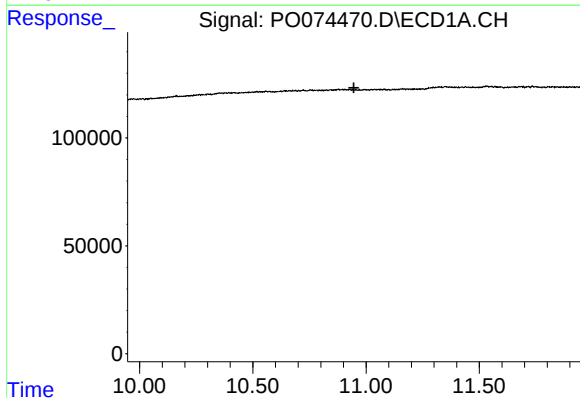


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.946 min
Response: 0
Conc: N.D.

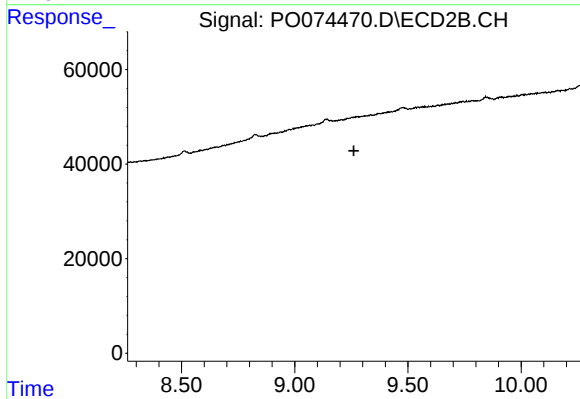

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 9.261 min
Response: 0
Conc: N.D.

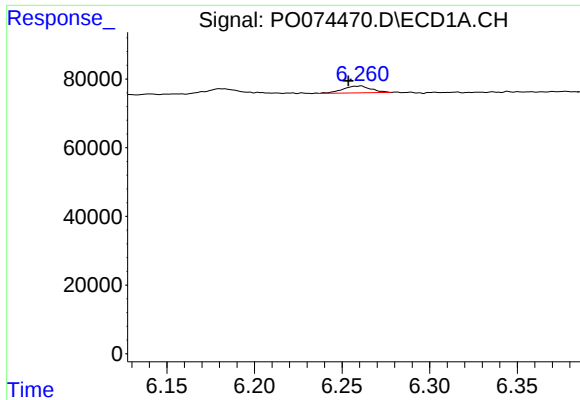

#3 AR-1016-1


R.T.: 6.261 min
Delta R.T.: 0.007 min
Response: 22863
Conc: 5.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

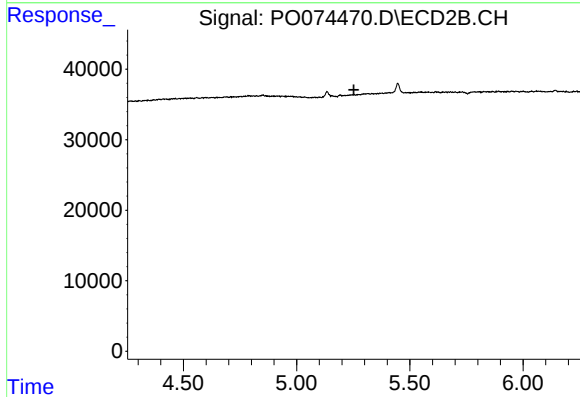


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 5.253 min
Response: 0
Conc: N.D.

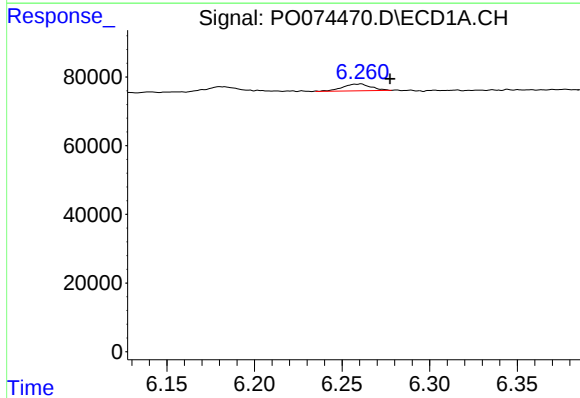


#4 AR-1016-2

R.T.: 6.261 min
Delta R.T.: -0.017 min
Response: 22863
Conc: 4.01 ng/ml

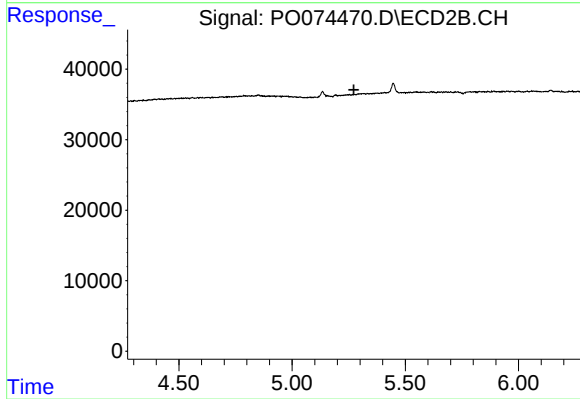

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 5.273 min
Response: 0
Conc: N.D.

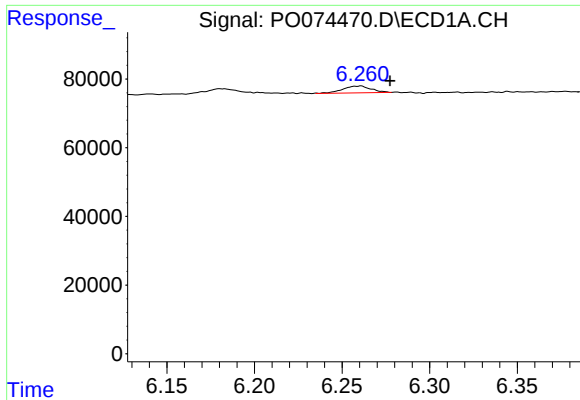

#13 AR-1232-3


R.T.: 6.261 min
Delta R.T.: -0.016 min
Response: 22863
Conc: 9.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

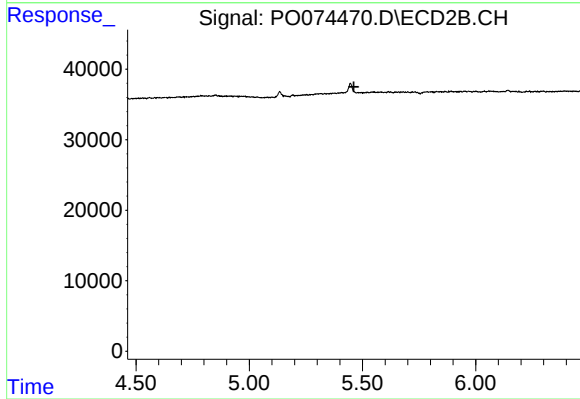


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 5.462 min
Response: 0
Conc: N.D.

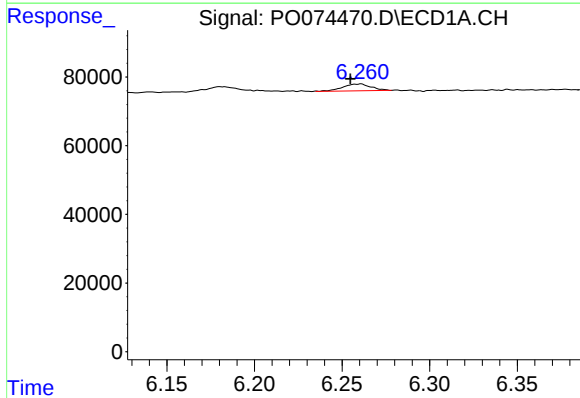


#16 AR-1242-1

R.T.: 6.261 min
Delta R.T.: 0.006 min
Response: 22863
Conc: 7.10 ng/ml

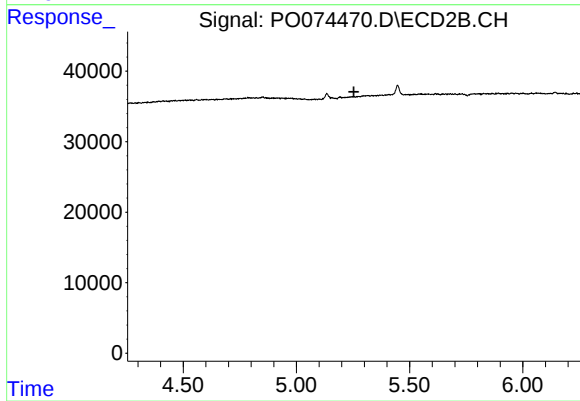

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 5.254 min
Response: 0
Conc: N.D.

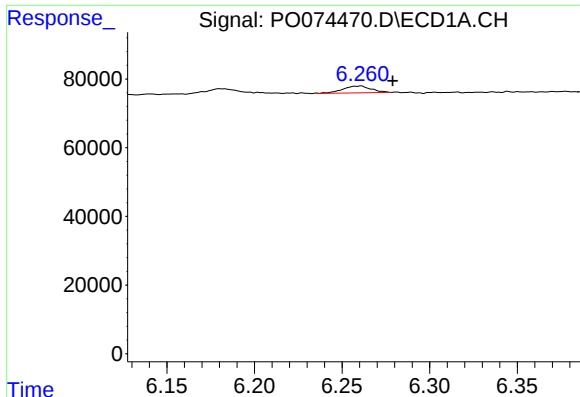

#17 AR-1242-2


R.T.: 6.261 min
Delta R.T.: -0.018 min
Response: 22863
Conc: 5.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

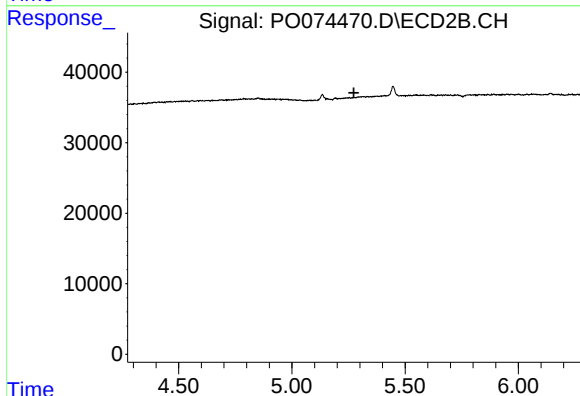


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 5.274 min
Response: 0
Conc: N.D.

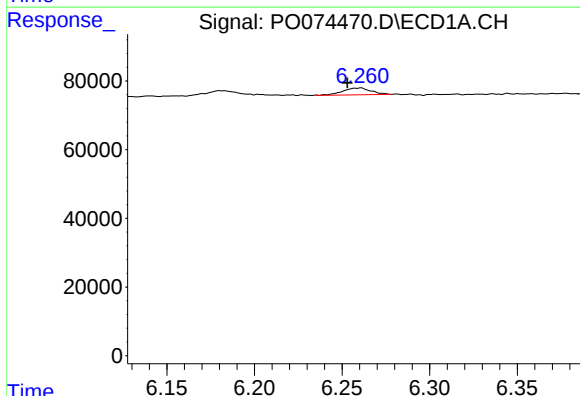


#21 AR-1248-1

R.T.: 6.261 min
Delta R.T.: 0.008 min
Response: 22863
Conc: 9.50 ng/ml

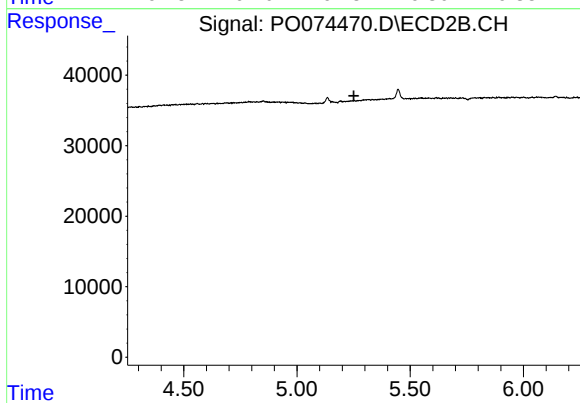

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 5.252 min
Response: 0
Conc: N.D.

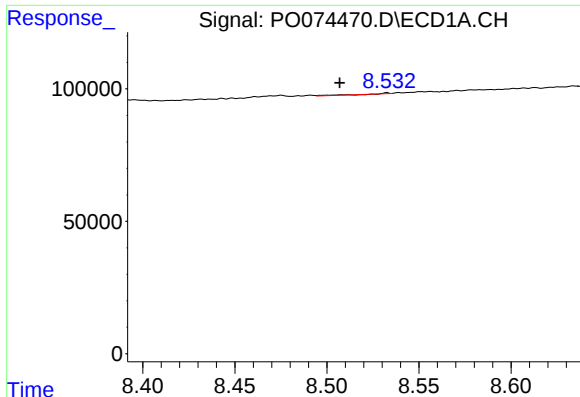

#30 AR-1254-5


R.T.: 8.533 min
Delta R.T.: 0.026 min
Response: 1249
Conc: 0.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
HEXANE

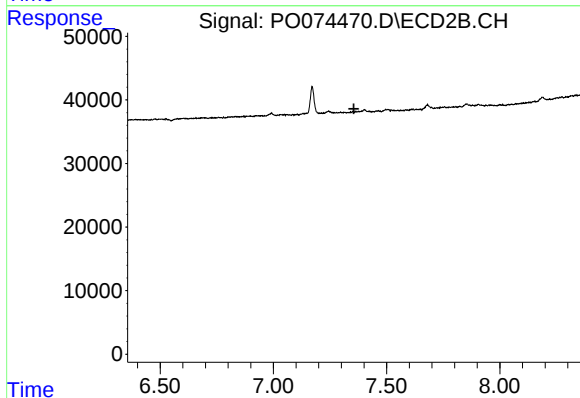


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.356 min
Response: 0
Conc: N.D.

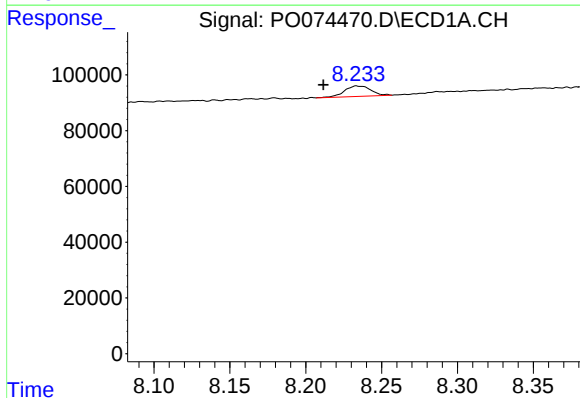


#32 AR-1260-2

R.T.: 8.233 min
Delta R.T.: 0.022 min
Response: 45506
Conc: 6.69 ng/ml

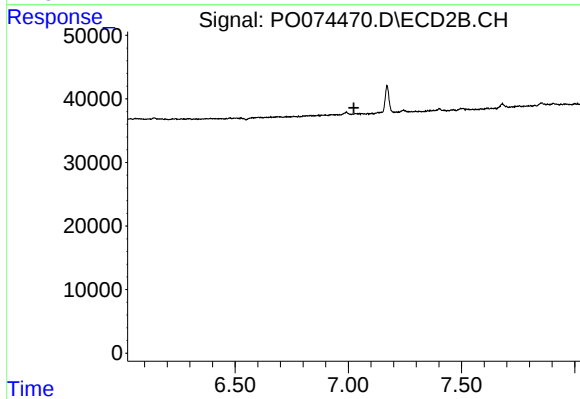

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.025 min
Response: 0
Conc: N.D.

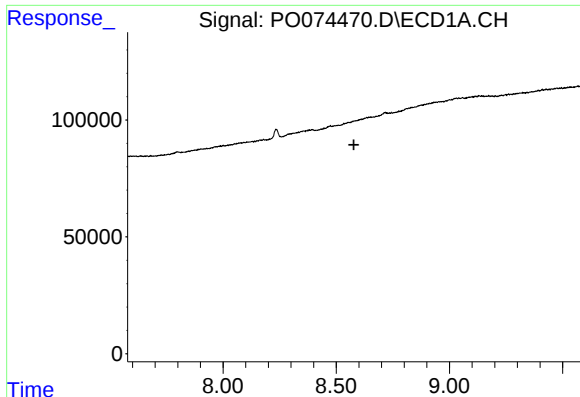

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.578 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
HEXANE

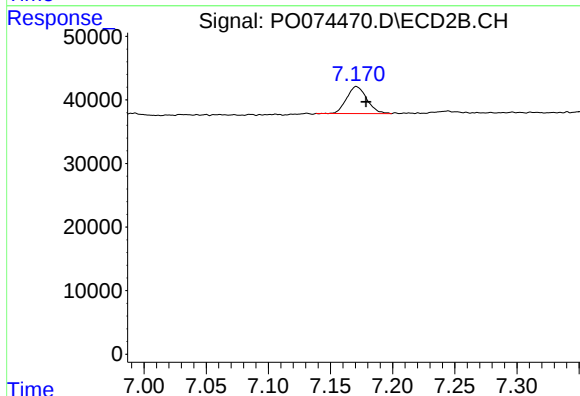


#33 AR-1260-3

R.T.: 7.171 min
Delta R.T.: -0.008 min
Response: 48182
Conc: 13.37 ng/ml

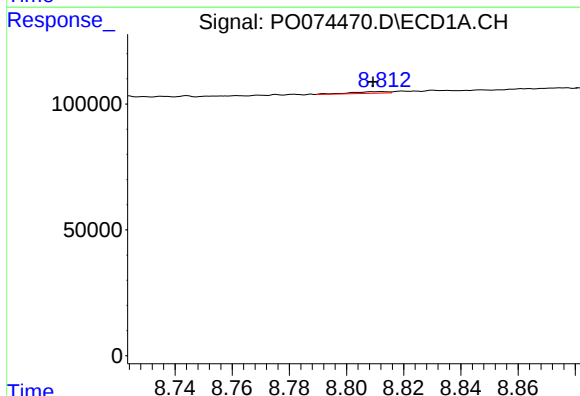

#34 AR-1260-4

R.T.: 8.812 min
Delta R.T.: 0.003 min
Response: 5718
Conc: 1.04 ng/ml

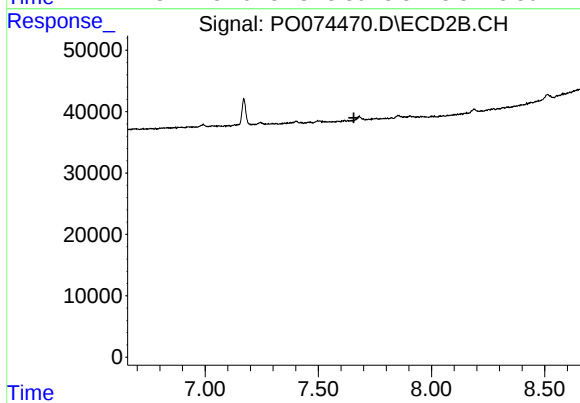

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 7.657 min
Response: 0
Conc: N.D.