

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011123\
 Data File : P0091952.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Jan 2023 13:59
 Operator : YP/AJ
 Sample : 01082-02
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 1556

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/12/2023
 Supervised By :Ankita Jodhani 01/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 01:24:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.443	3.649	39365004	21208651	14.113m	15.276m
2) SA Decachlor...	10.353	8.705	35734049	16244908	18.253	18.321

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011123\
Data File : PO091952.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Jan 2023 13:59
Operator : YP/AJ
Sample : 01082-02
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
1556


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/12/2023
Supervised By :Ankita Jodhani 01/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 01:24:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

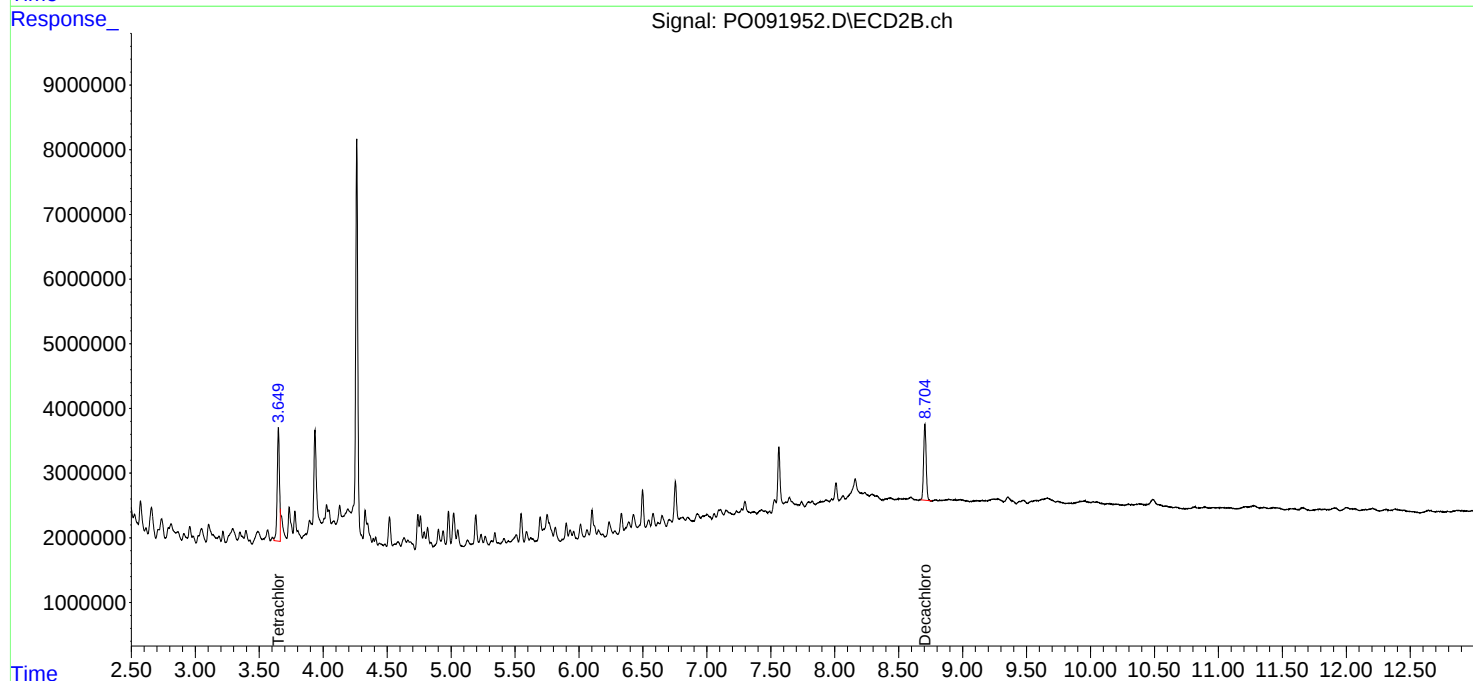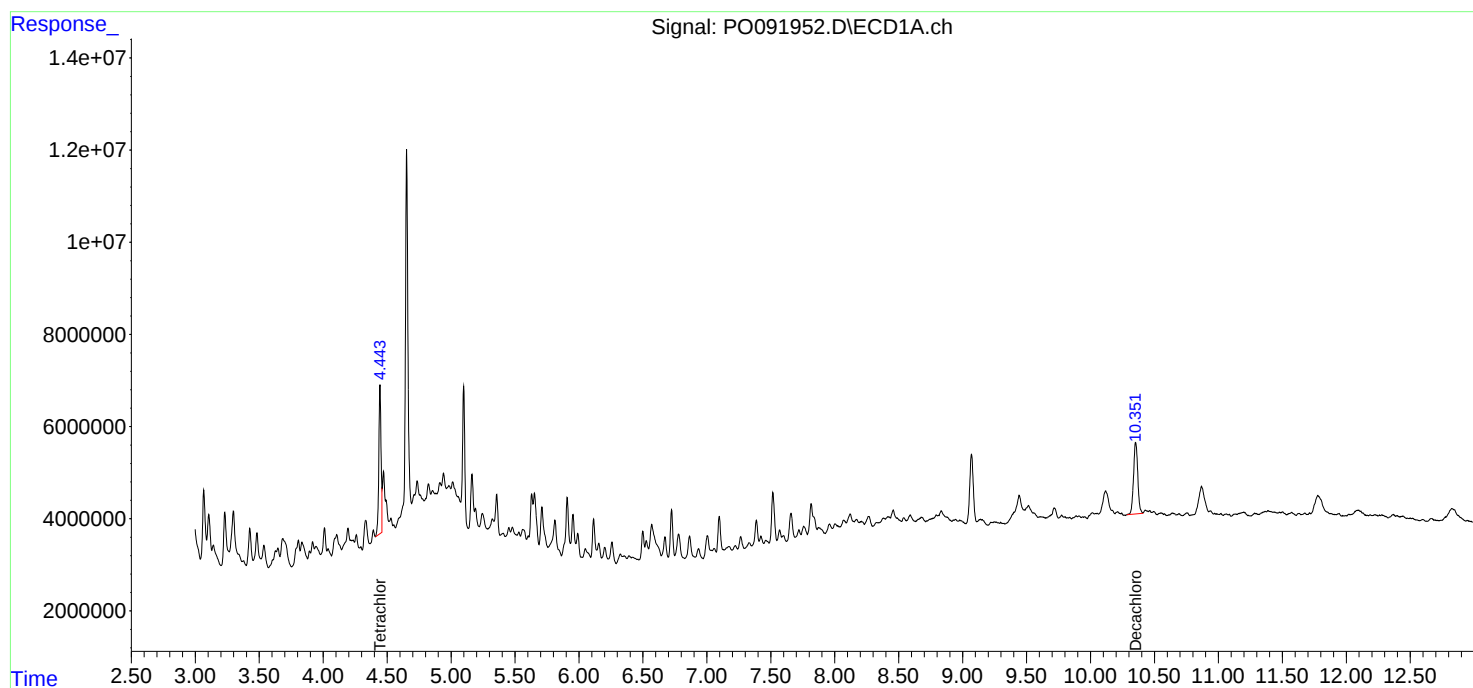

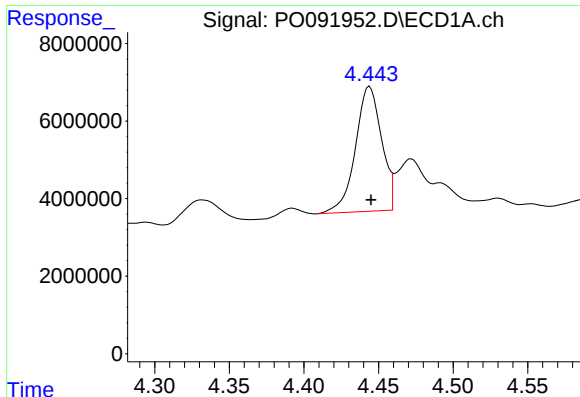


#1 Tetrachloro-m-xylene

R.T.: 4.443 min
Delta R.T.: -0.002 min
Response: 39365004
Conc: 14.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
1556


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/12/2023
Supervised By :Ankita Jodhani 01/12/2023

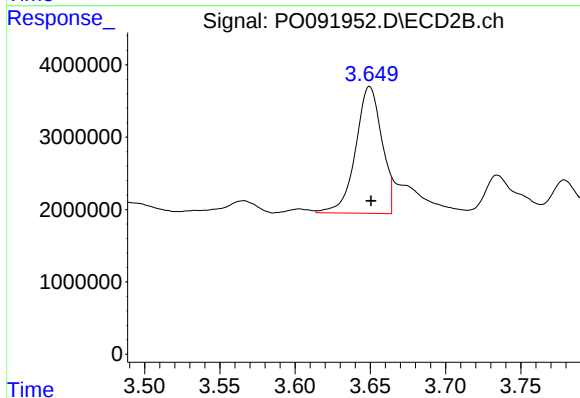


#1 Tetrachloro-m-xylene

R.T.: 3.649 min
Delta R.T.: -0.002 min
Response: 21208651
Conc: 15.28 ng/ml m

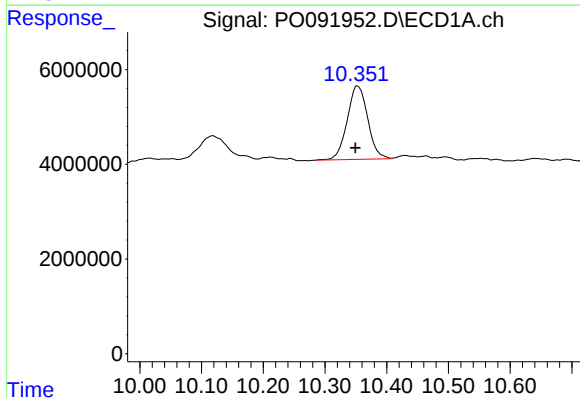

#2 Decachlorobiphenyl

R.T.: 10.353 min
Delta R.T.: 0.003 min
Response: 35734049
Conc: 18.25 ng/ml

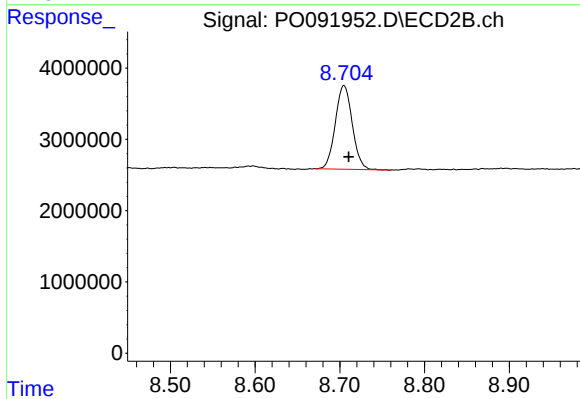

#2 Decachlorobiphenyl

R.T.: 8.705 min
Delta R.T.: -0.005 min
Response: 16244908
Conc: 18.32 ng/ml