

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011221\
 Data File : P0074520.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jan 2021 12:26
 Operator : AJ/MA
 Sample : PB134066BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB134066BL

Manual Integrations
 APPROVED

Ankita
 1/13/2021 11:27:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 17:00:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.946	4.007	2095825	1098744	19.862	19.532
2) SA Decachlor...	10.965f	9.262	2192717	1167832	21.605m	21.270

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011221\
Data File : P0074520.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jan 2021 12:26
Operator : AJ/MA
Sample : PB134066BL
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB134066BL


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 17:00:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

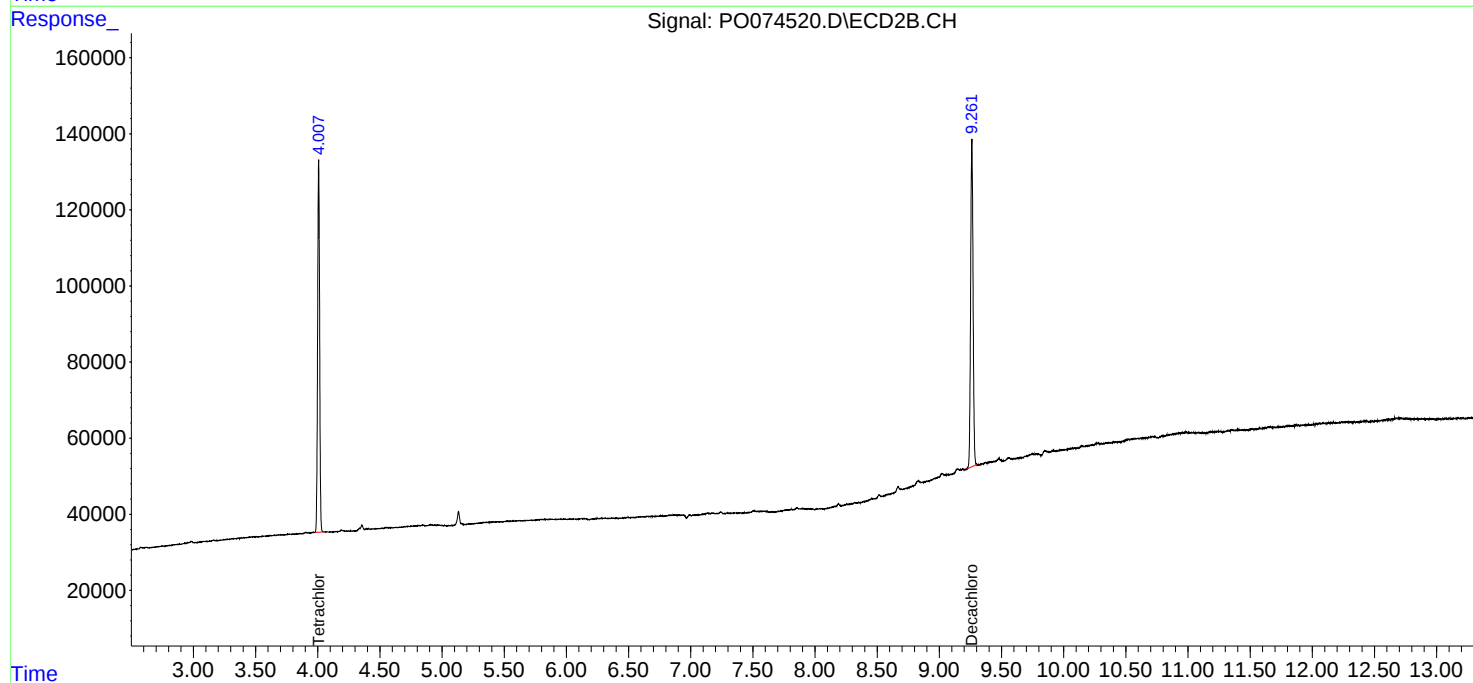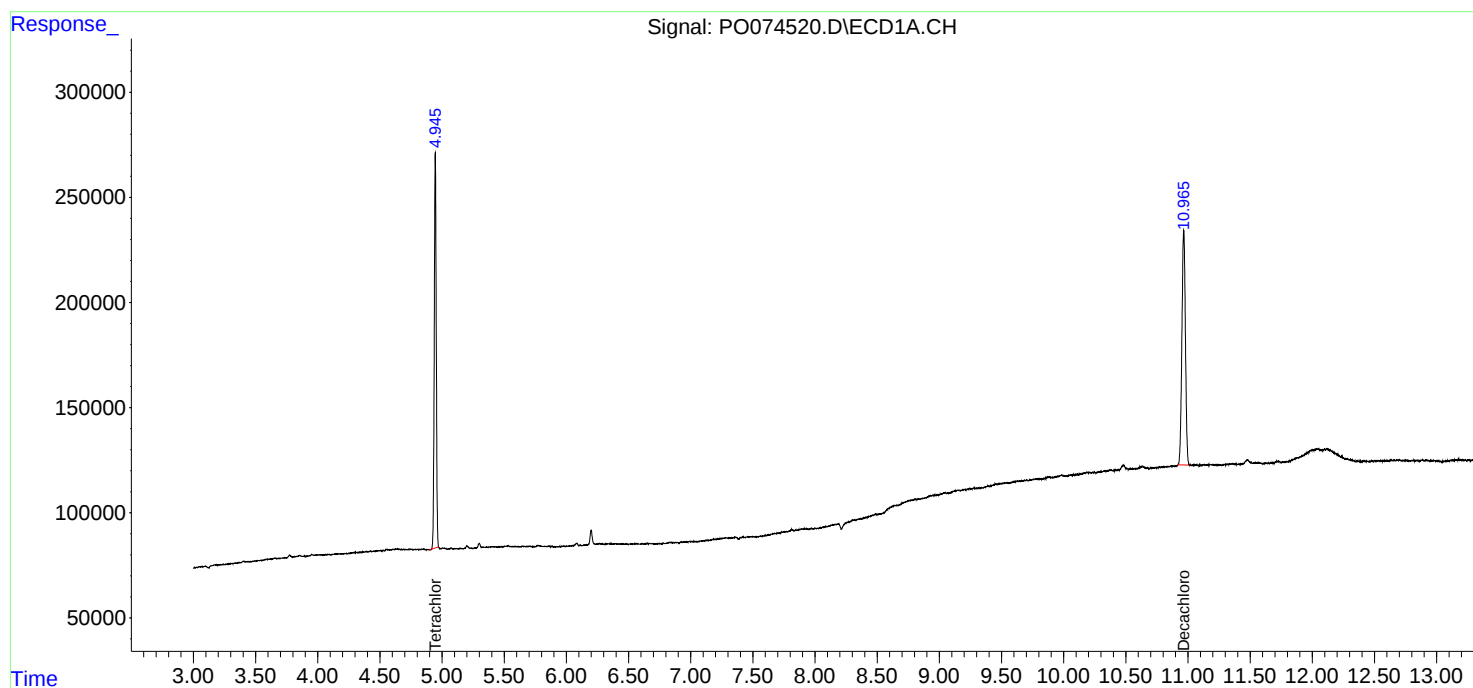

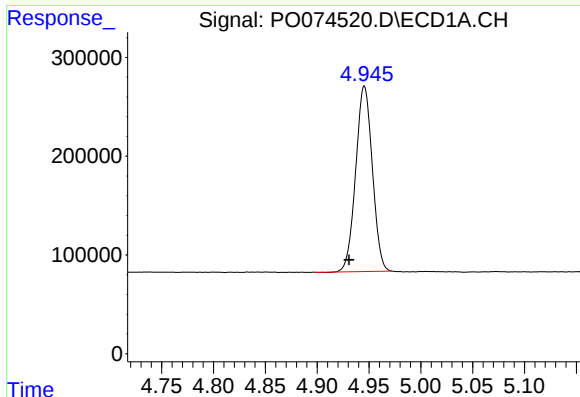


#1 Tetrachloro-m-xylene

R.T.: 4.946 min
Delta R.T.: 0.015 min
Response: 2095825
Conc: 19.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB134066BL


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:38 AM

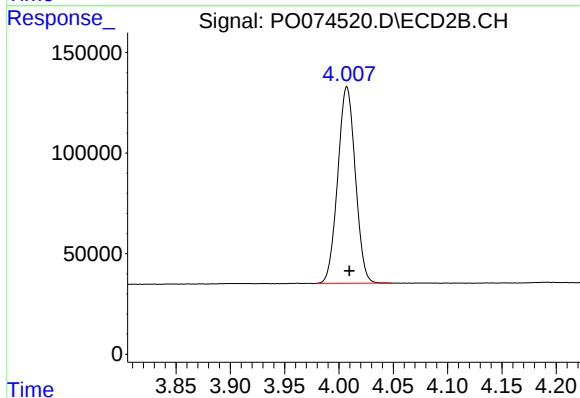


#1 Tetrachloro-m-xylene

R.T.: 4.007 min
Delta R.T.: -0.002 min
Response: 1098744
Conc: 19.53 ng/ml

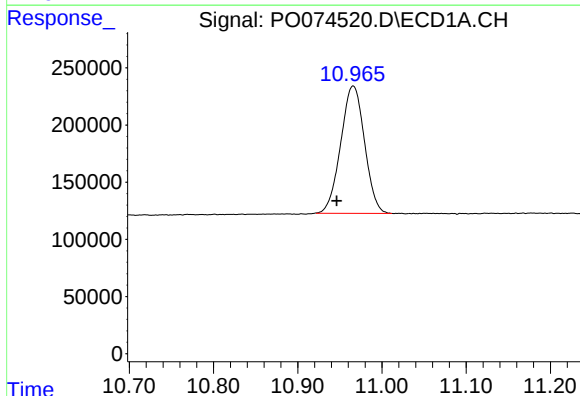

#2 Decachlorobiphenyl

R.T.: 10.965 min
Delta R.T.: 0.019 min
Response: 2192717
Conc: 21.60 ng/ml m

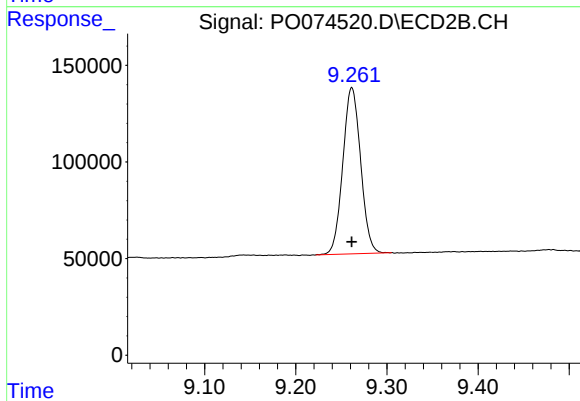

#2 Decachlorobiphenyl

R.T.: 9.262 min
Delta R.T.: 0.000 min
Response: 1167832
Conc: 21.27 ng/ml