

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011221\
 Data File : P0074546.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jan 2021 19:49
 Operator : AJ/MA
 Sample : M1087-01 5X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S4-01-B

Manual Integrations
 APPROVED

Ankita
 1/13/2021 11:27:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 01:07:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.005	472514	269612	4.478	4.793
2) SA Decachlor...	10.947	9.259	413645	231359	4.076	4.214
Target Compounds						
26) L6 AR-1254-1	7.166	6.115	355224	271175	80.767m	75.076
27) L6 AR-1254-2	7.396	6.274	830796	461910	121.983	148.212
28) L6 AR-1254-3	7.779	6.690	1293049	940858	184.344	191.858
29) L6 AR-1254-4	8.077	6.928	1174696	672252	193.695	193.857
30) L6 AR-1254-5	8.507	7.354	1974930	4923386	339.981	1087.815 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011221\
Data File : PO074546.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jan 2021 19:49
Operator : AJ/MA
Sample : M1087-01 5X
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S4-01-B


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 01:07:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

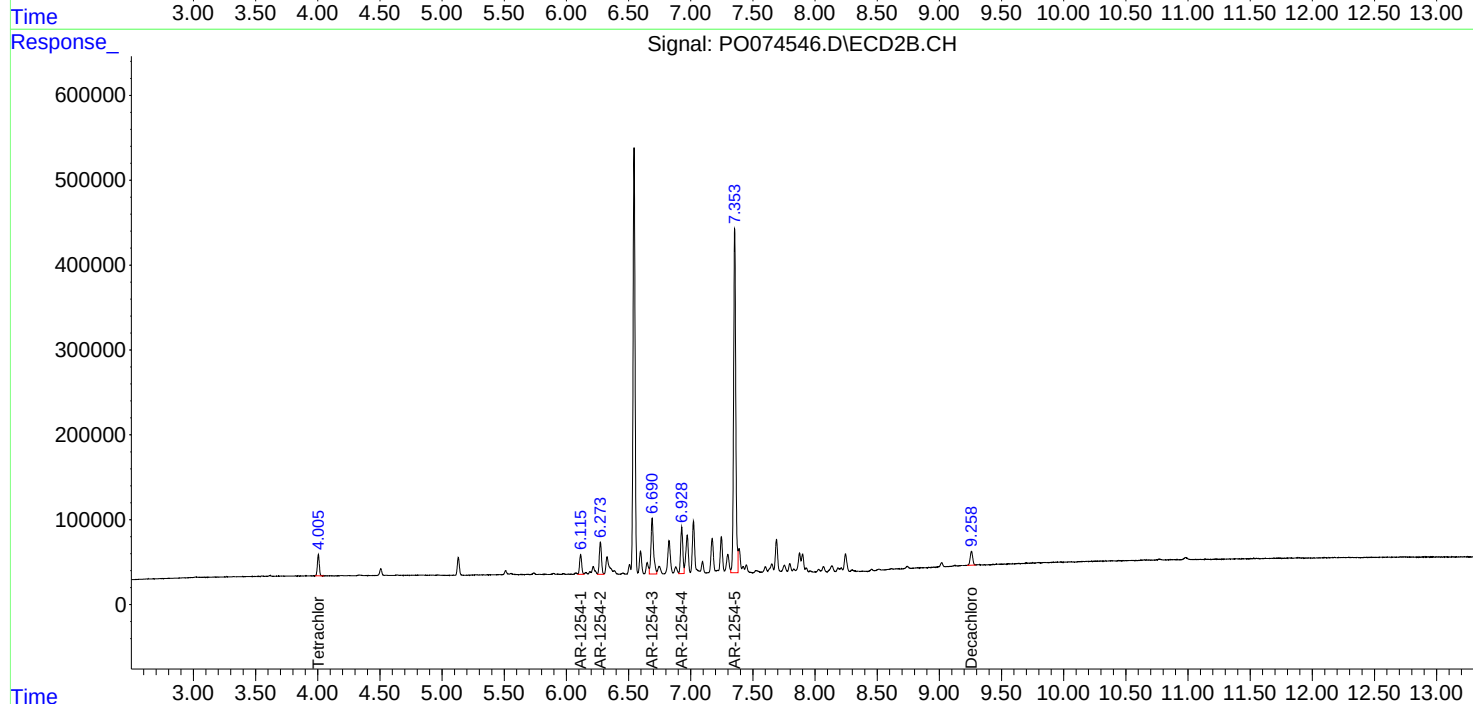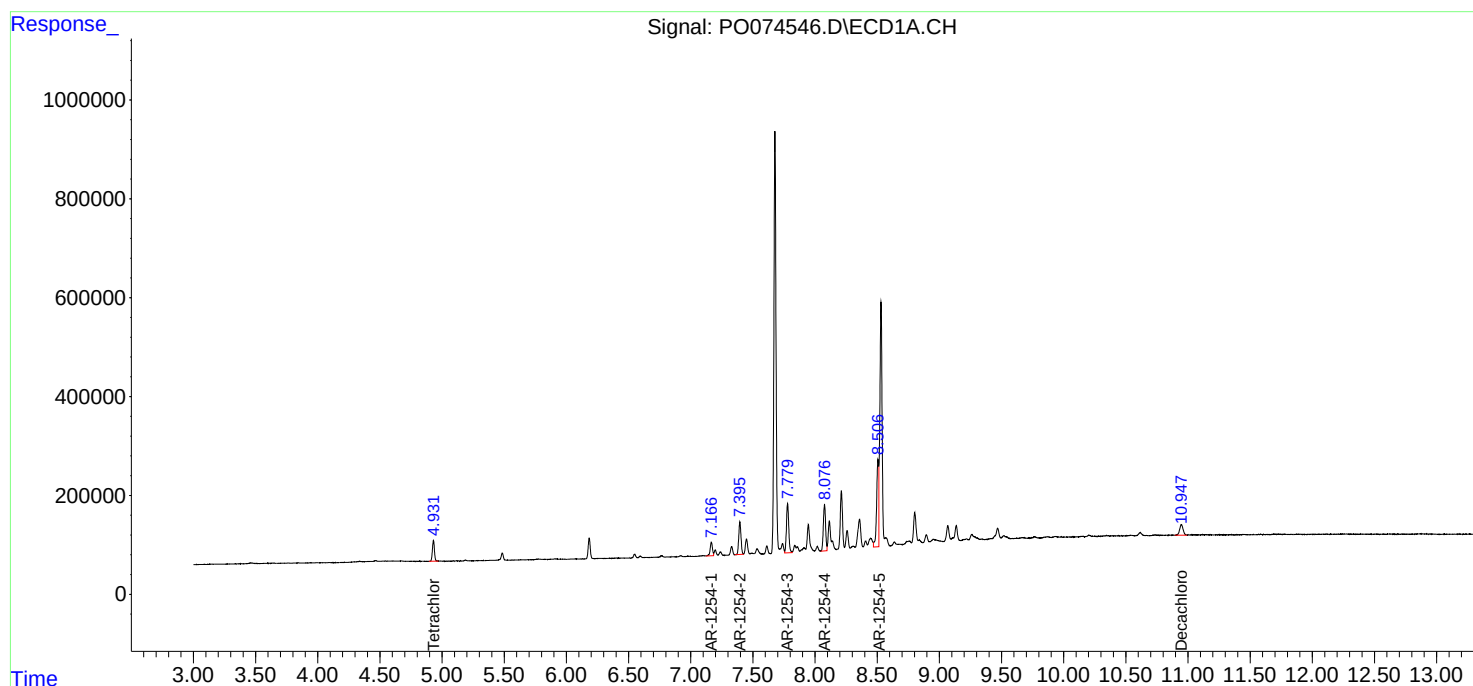

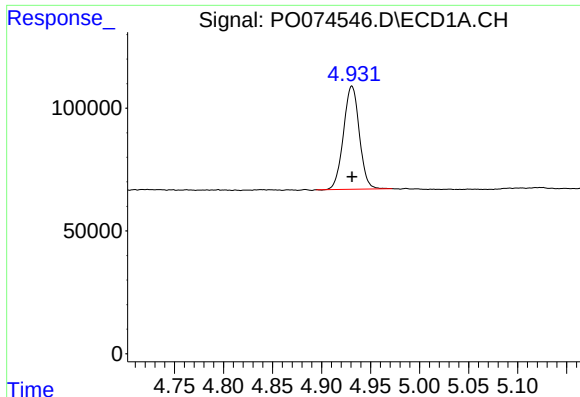


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 472514
Conc: 4.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
S4-01-B


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:46 AM

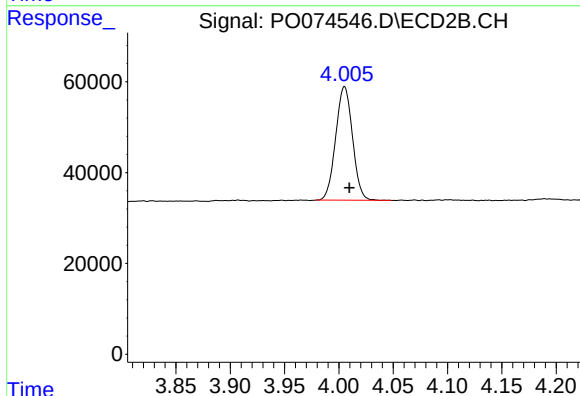


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.005 min
Response: 269612
Conc: 4.79 ng/ml

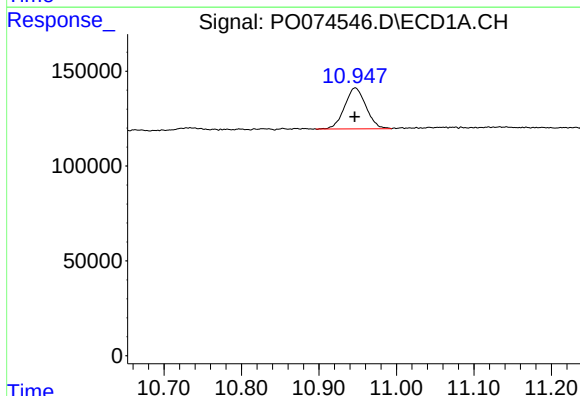


#2 Decachlorobiphenyl

R.T.: 10.947 min
Delta R.T.: 0.000 min
Response: 413645
Conc: 4.08 ng/ml

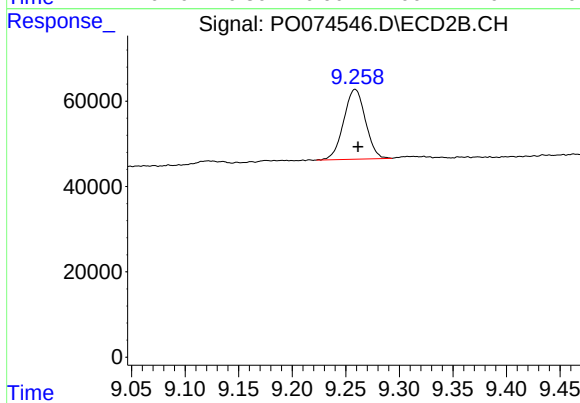

#2 Decachlorobiphenyl

R.T.: 9.259 min
Delta R.T.: -0.003 min
Response: 231359
Conc: 4.21 ng/ml

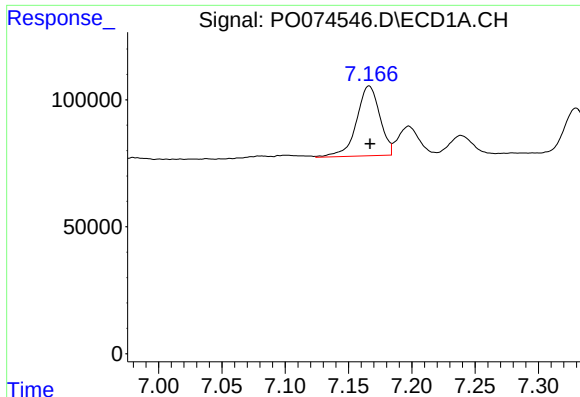


#26 AR-1254-1

R.T.: 7.166 min
Delta R.T.: -0.001 min
Response: 355224
Conc: 80.77 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S4-01-B


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:46 AM

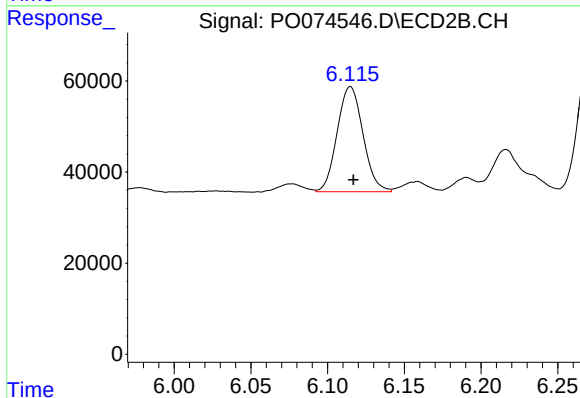


#26 AR-1254-1

R.T.: 6.115 min
Delta R.T.: -0.002 min
Response: 271175
Conc: 75.08 ng/ml

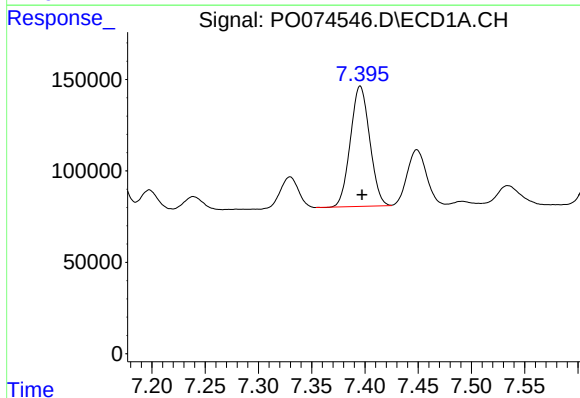


#27 AR-1254-2

R.T.: 7.396 min
Delta R.T.: -0.002 min
Response: 830796
Conc: 121.98 ng/ml

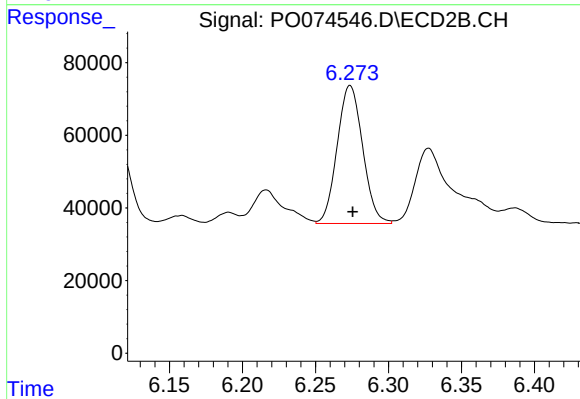

#27 AR-1254-2

R.T.: 6.274 min
Delta R.T.: -0.002 min
Response: 461910
Conc: 148.21 ng/ml

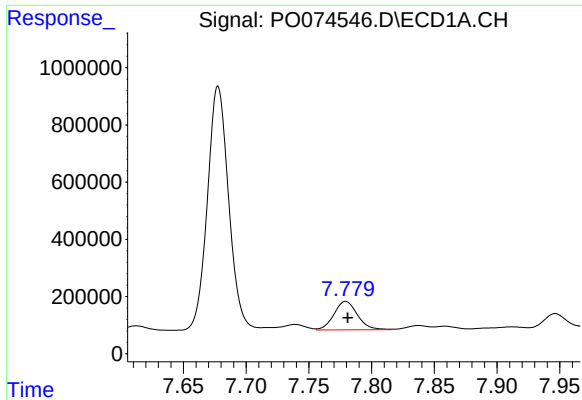


#28 AR-1254-3

R.T.: 7.779 min
Delta R.T.: -0.002 min
Response: 1293049
Conc: 184.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
S4-01-B


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:46 AM

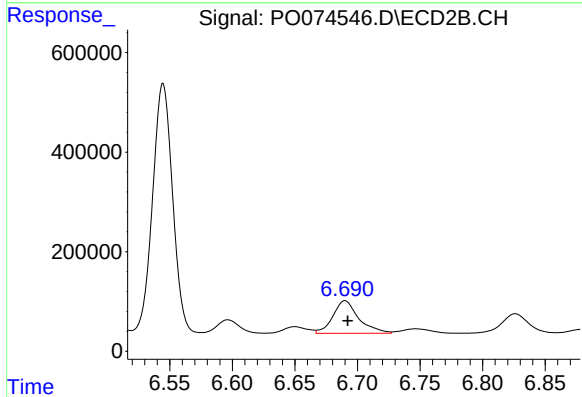


#28 AR-1254-3

R.T.: 6.690 min
Delta R.T.: -0.002 min
Response: 940858
Conc: 191.86 ng/ml

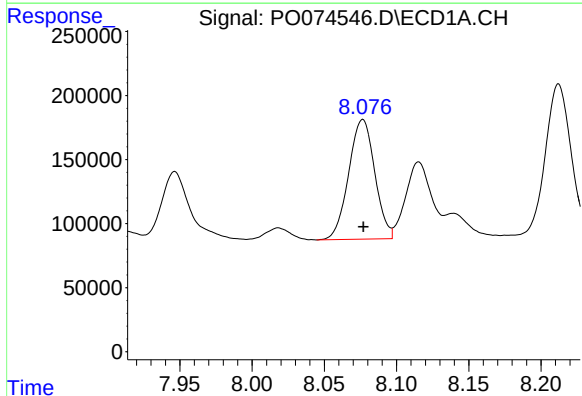


#29 AR-1254-4

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 1174696
Conc: 193.69 ng/ml

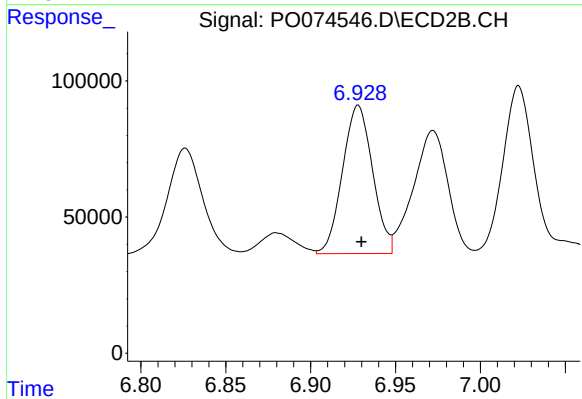

#29 AR-1254-4

R.T.: 6.928 min
Delta R.T.: -0.002 min
Response: 672252
Conc: 193.86 ng/ml

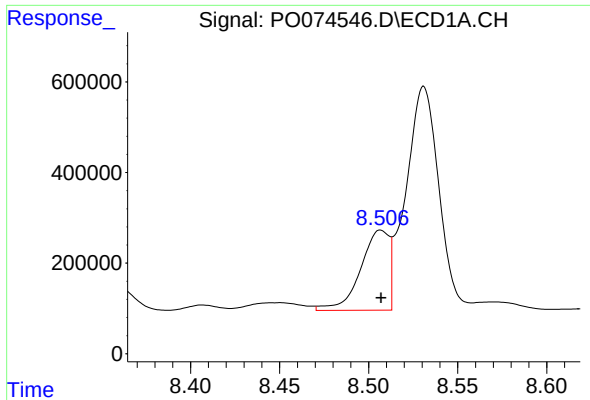


#30 AR-1254-5

R.T.: 8.507 min
Delta R.T.: 0.000 min
Response: 1974930
Conc: 339.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
S4-01-B

Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:46 AM

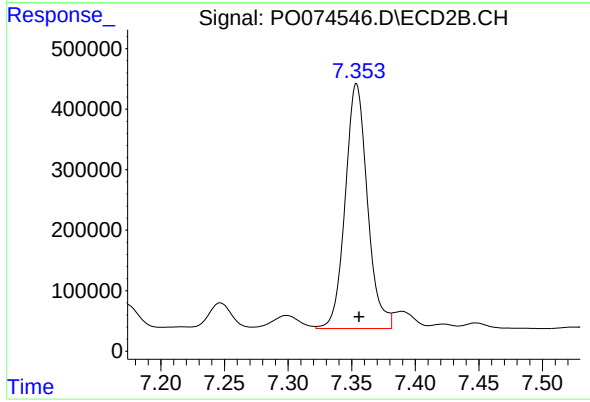

#30 AR-1254-5

R.T.: 7.354 min
Delta R.T.: -0.002 min
Response: 4923386
Conc: 1087.81 ng/ml