

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011221\
 Data File : P0074549.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Jan 2021 20:40
 Operator : AJ/MA
 Sample : M1087-04 5X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-5

Manual Integrations
 APPROVED

Ankita
 1/13/2021 11:27:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 01:08:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.930	4.005	463223	280504	4.390m	4.987
2) SA Decachlor...	10.946	9.257	364296	202718	3.589	3.692
Target Compounds						
26) L6 AR-1254-1	7.166	6.115	2408920	1837232	547.713	508.646
27) L6 AR-1254-2	7.396	6.273	3975853	1833534	583.760	588.324
28) L6 AR-1254-3	7.779	6.690	4458637	3123098	635.647	636.857
29) L6 AR-1254-4	8.076	6.928	3602653	1969868	594.039	568.049
30) L6 AR-1254-5	8.506	7.354	4478247	6549117	770.924	1447.018 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011221\
Data File : PO074549.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Jan 2021 20:40
Operator : AJ/MA
Sample : M1087-04 5X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
DUP-5


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 01:08:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

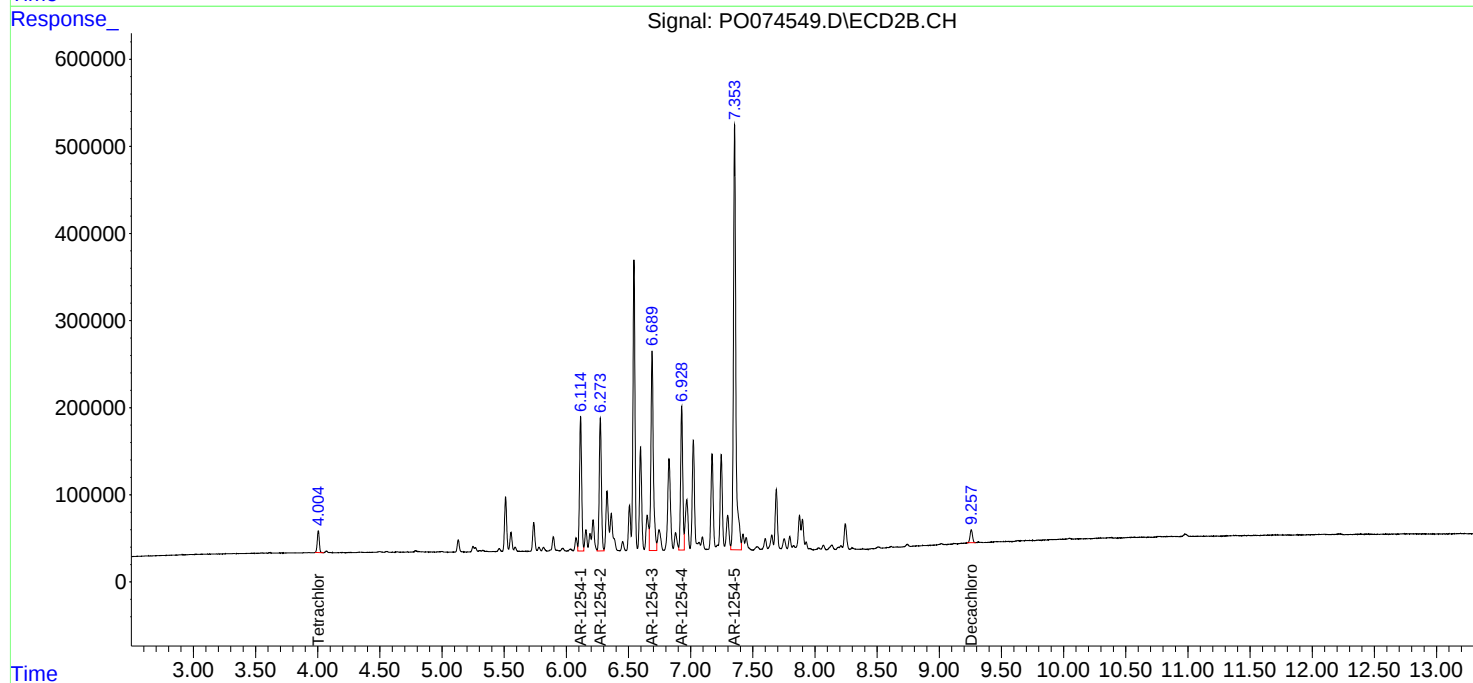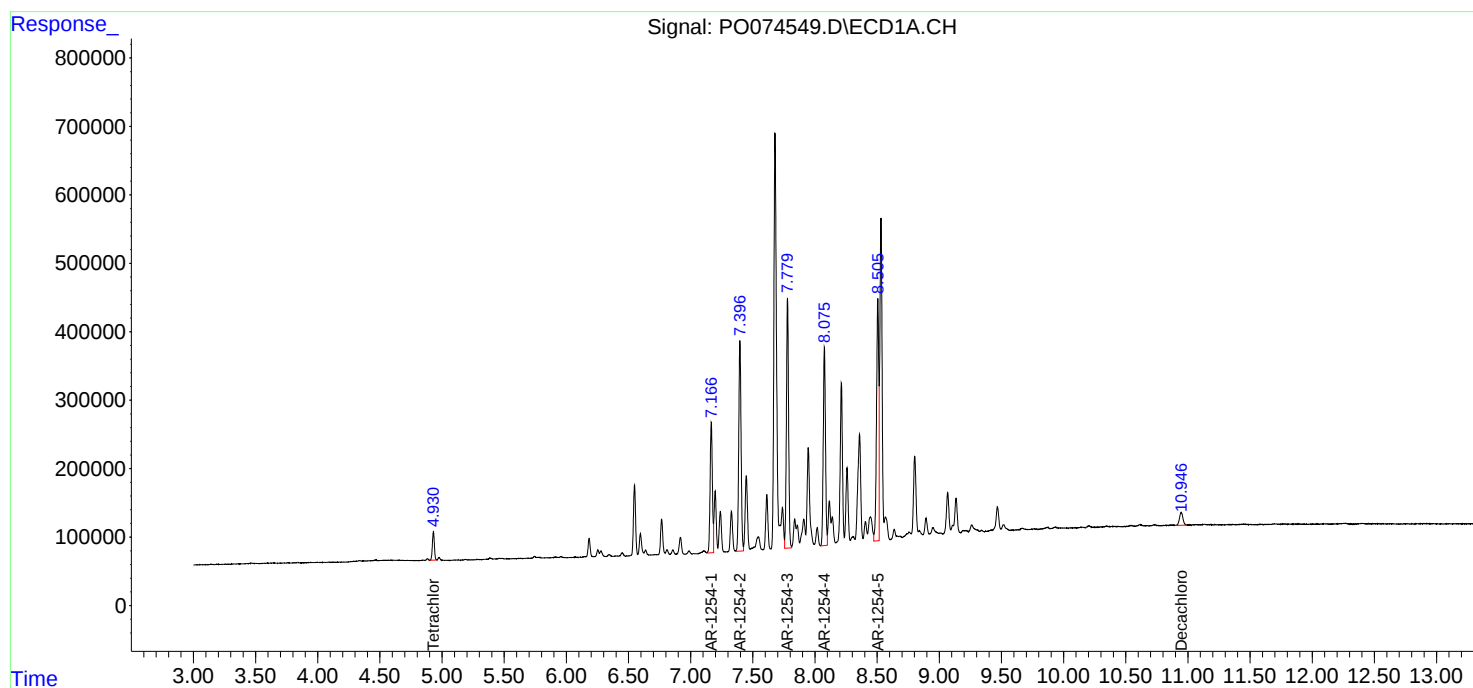

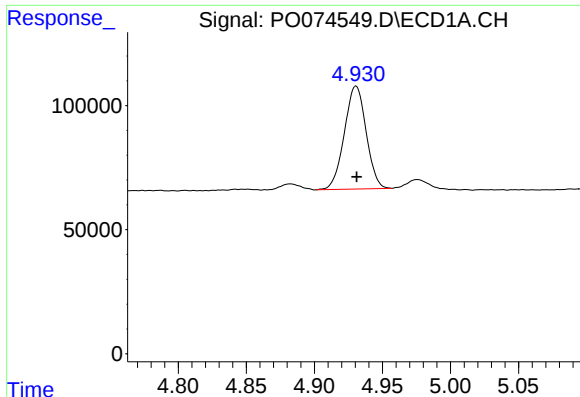


#1 Tetrachloro-m-xylene

R.T.: 4.930 min
Delta R.T.: 0.000 min
Response: 463223
Conc: 4.39 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DUP-5


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:51 AM

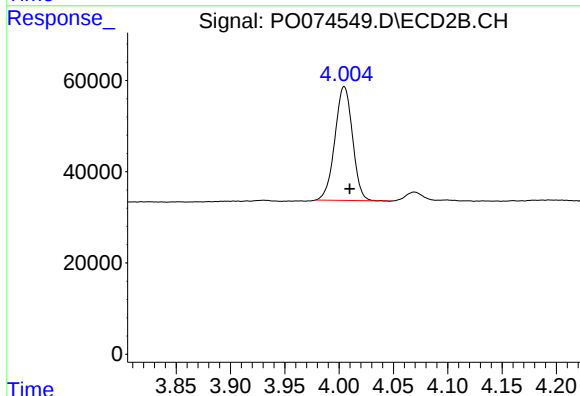


#1 Tetrachloro-m-xylene

R.T.: 4.005 min
Delta R.T.: -0.005 min
Response: 280504
Conc: 4.99 ng/ml

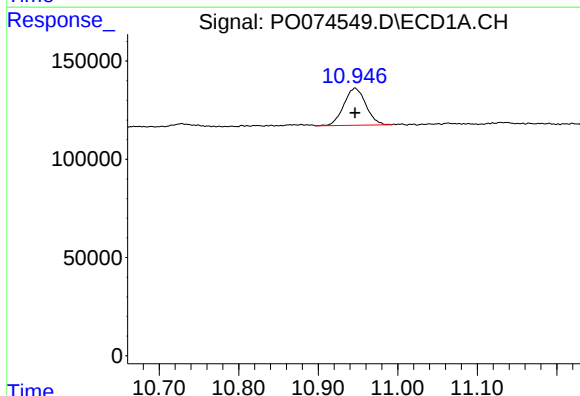


#2 Decachlorobiphenyl

R.T.: 10.946 min
Delta R.T.: 0.000 min
Response: 364296
Conc: 3.59 ng/ml

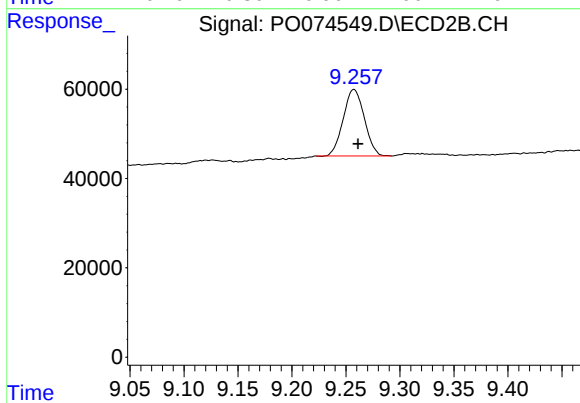

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.004 min
Response: 202718
Conc: 3.69 ng/ml

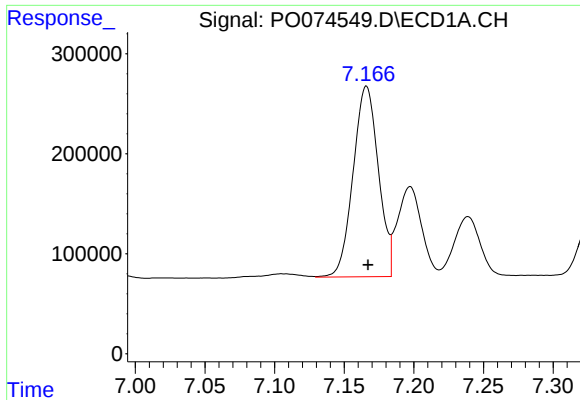


#26 AR-1254-1

R.T.: 7.166 min
Delta R.T.: -0.001 min
Response: 2408920
Conc: 547.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-5


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:51 AM

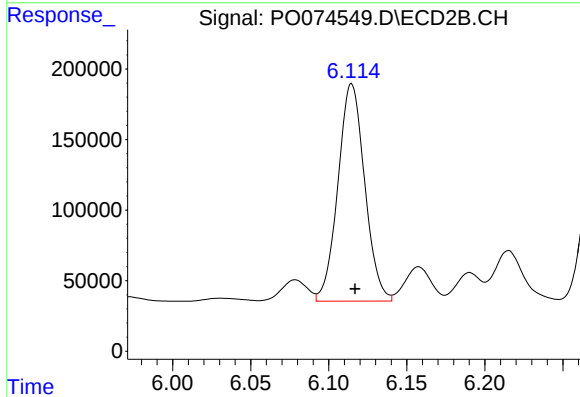


#26 AR-1254-1

R.T.: 6.115 min
Delta R.T.: -0.002 min
Response: 1837232
Conc: 508.65 ng/ml

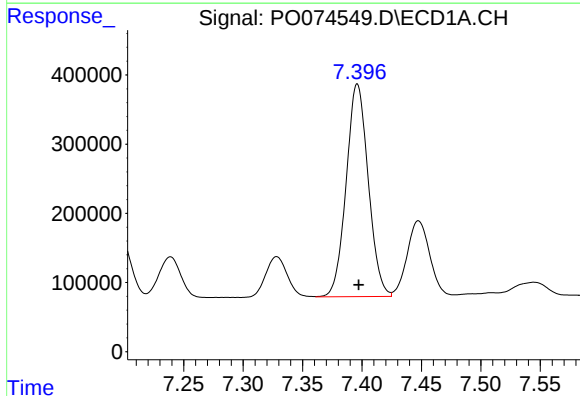


#27 AR-1254-2

R.T.: 7.396 min
Delta R.T.: -0.001 min
Response: 3975853
Conc: 583.76 ng/ml

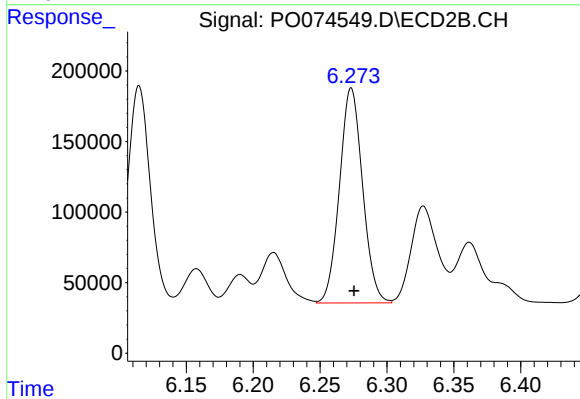

#27 AR-1254-2

R.T.: 6.273 min
Delta R.T.: -0.002 min
Response: 1833534
Conc: 588.32 ng/ml

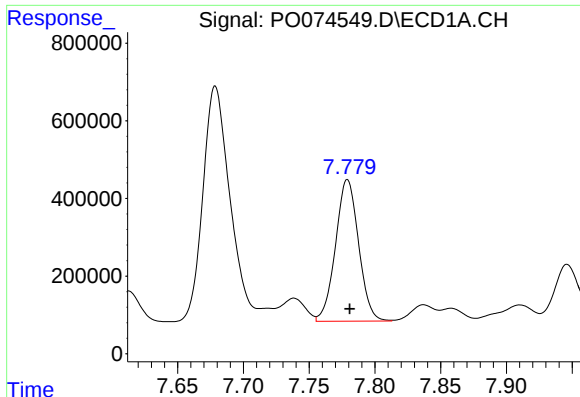


#28 AR-1254-3

R.T.: 7.779 min
Delta R.T.: -0.002 min
Response: 4458637
Conc: 635.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-5


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:51 AM

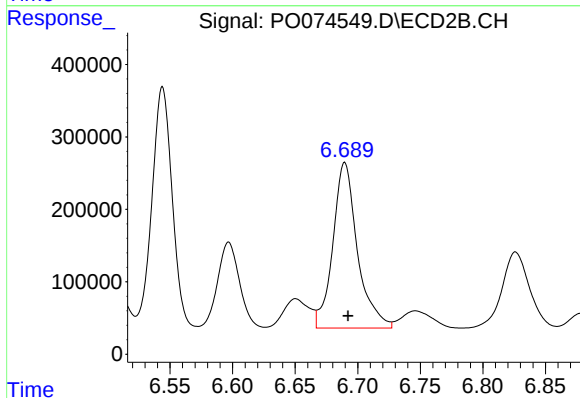


#28 AR-1254-3

R.T.: 6.690 min
Delta R.T.: -0.003 min
Response: 3123098
Conc: 636.86 ng/ml

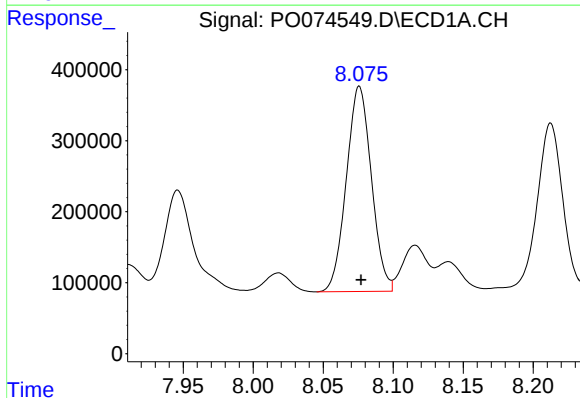


#29 AR-1254-4

R.T.: 8.076 min
Delta R.T.: -0.001 min
Response: 3602653
Conc: 594.04 ng/ml

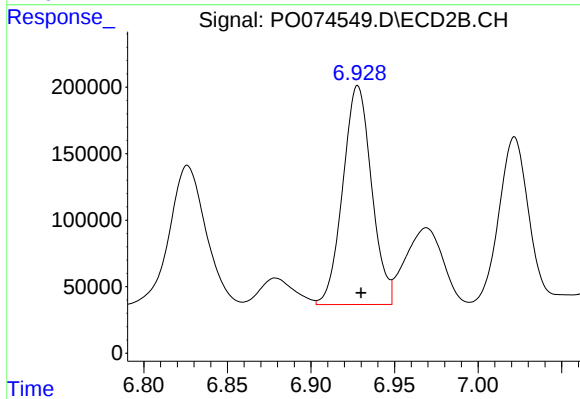

#29 AR-1254-4

R.T.: 6.928 min
Delta R.T.: -0.002 min
Response: 1969868
Conc: 568.05 ng/ml

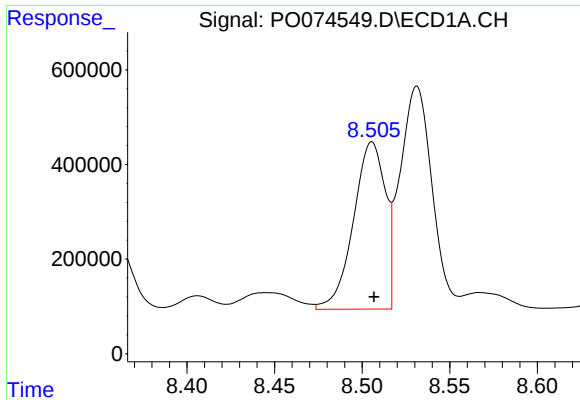


#30 AR-1254-5

R.T.: 8.506 min
Delta R.T.: -0.001 min
Response: 4478247
Conc: 770.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-5

Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:51 AM

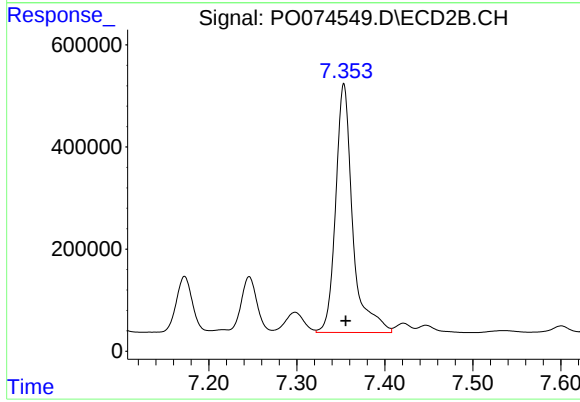

#30 AR-1254-5

R.T.: 7.354 min
Delta R.T.: -0.002 min
Response: 6549117
Conc: 1447.02 ng/ml