

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011221\
 Data File : P0074560.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 00:06
 Operator : AJ/MA
 Sample : M1095-18
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-28A

Manual Integrations
 APPROVED

Ankita
 1/13/2021 11:27:59 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 01:10:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.932	4.006	1815070	1047872	17.202m	18.628
2) SA Decachlor...	10.950	9.258	1252886	729471	12.345	13.286
Target Compounds						
26) L6 AR-1254-1	7.167	6.115	72608	116938	16.509	32.375m#
27) L6 AR-1254-2	7.399	6.274	380117	245646	55.811	78.820 #
28) L6 AR-1254-3	7.782	6.690	823996	604709	117.473	123.311
29) L6 AR-1254-4	8.077	6.928	614871	317687	101.386	91.611
30) L6 AR-1254-5	8.507	7.353	2041024	2911577	351.359	643.309 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011221\
Data File : PO074560.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 00:06
Operator : AJ/MA
Sample : M1095-18
Misc :
ALS Vial : 44 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-28A


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:59 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 01:10:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

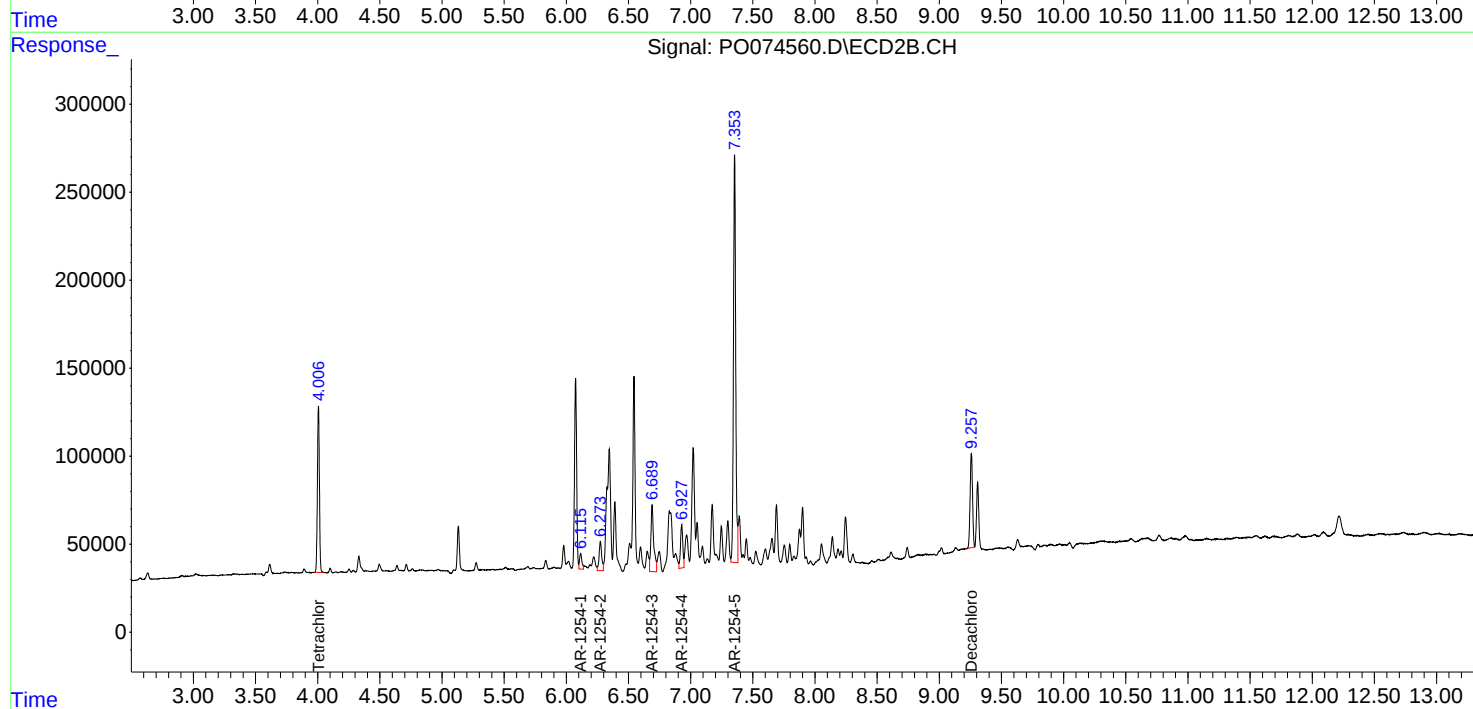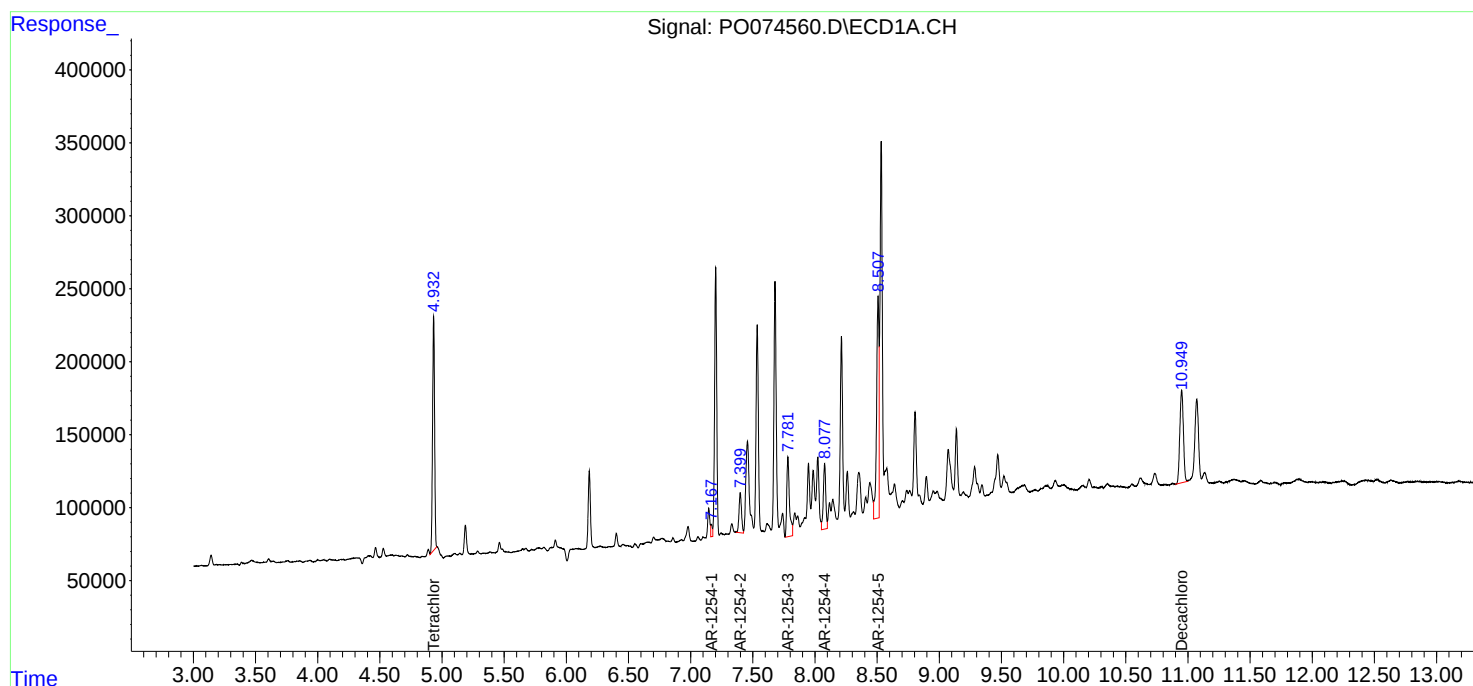

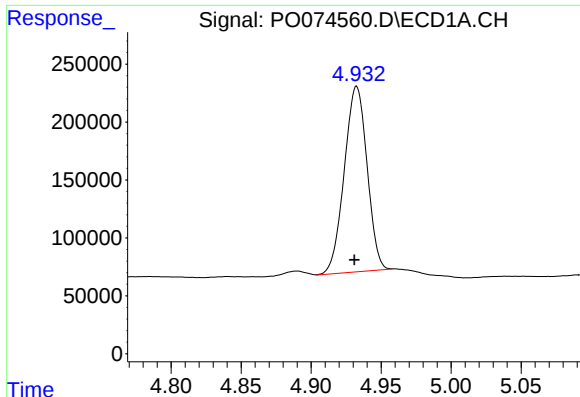


#1 Tetrachloro-m-xylene

R.T.: 4.932 min
Delta R.T.: 0.001 min
Response: 1815070
Conc: 17.20 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-28A


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:59 AM

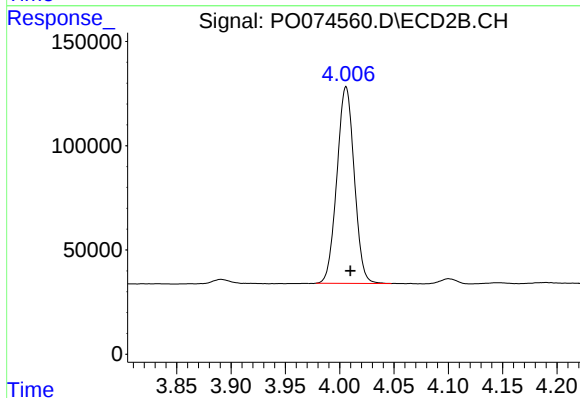


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: -0.004 min
Response: 1047872
Conc: 18.63 ng/ml

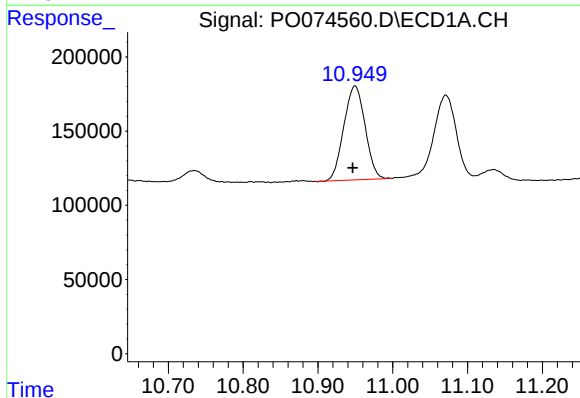


#2 Decachlorobiphenyl

R.T.: 10.950 min
Delta R.T.: 0.003 min
Response: 1252886
Conc: 12.34 ng/ml

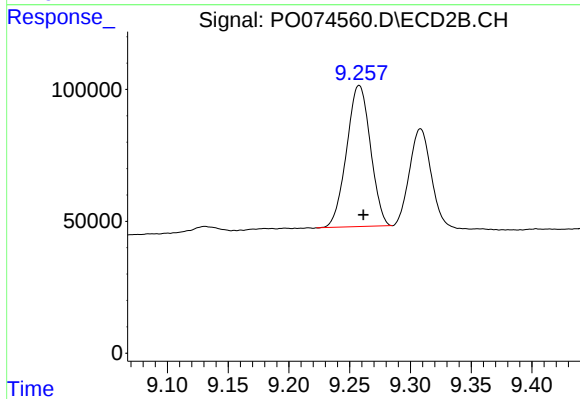

#2 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.004 min
Response: 729471
Conc: 13.29 ng/ml

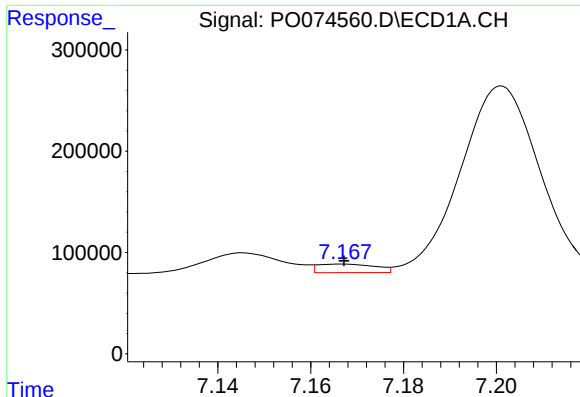


#26 AR-1254-1

R.T.: 7.167 min
Delta R.T.: 0.000 min
Response: 72608
Conc: 16.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-28A


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:59 AM

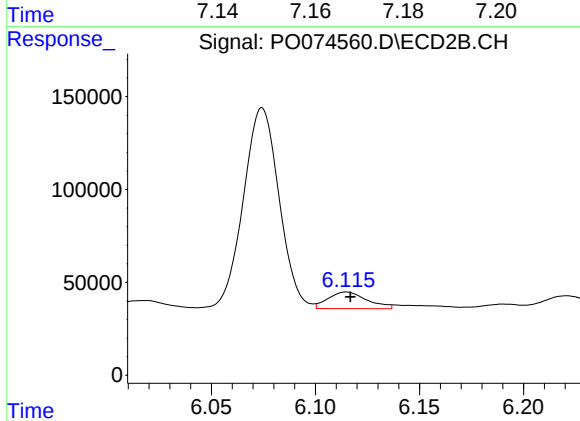


#26 AR-1254-1

R.T.: 6.115 min
Delta R.T.: -0.002 min
Response: 116938
Conc: 32.37 ng/ml m

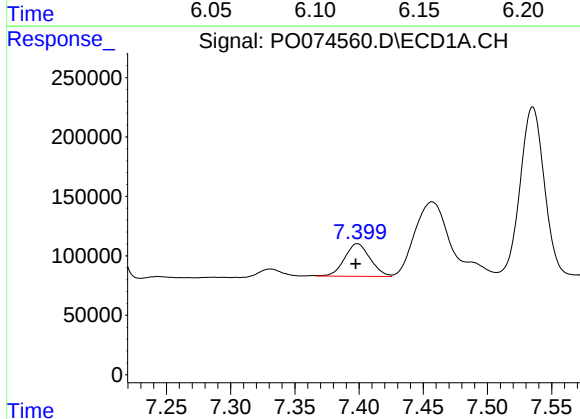


#27 AR-1254-2

R.T.: 7.399 min
Delta R.T.: 0.001 min
Response: 380117
Conc: 55.81 ng/ml

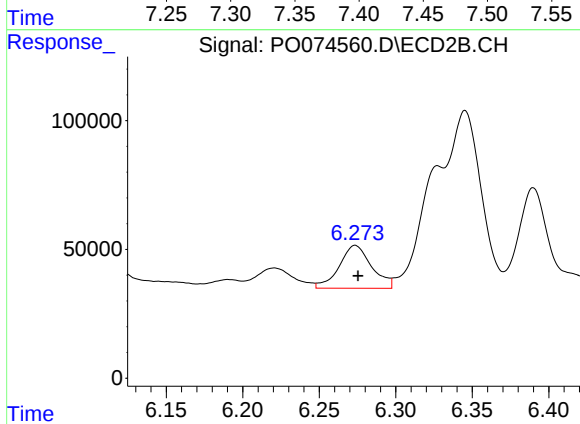

#27 AR-1254-2

R.T.: 6.274 min
Delta R.T.: -0.002 min
Response: 245646
Conc: 78.82 ng/ml

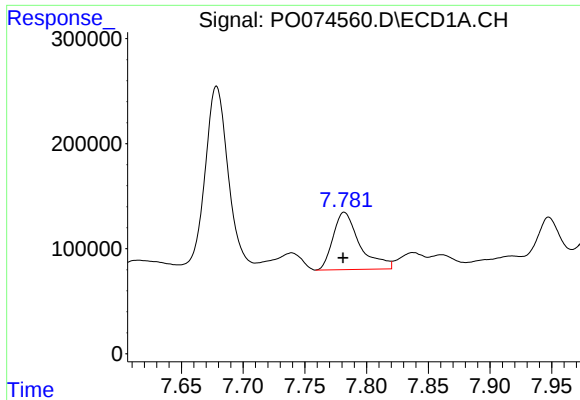


#28 AR-1254-3

R.T.: 7.782 min
Delta R.T.: 0.001 min
Response: 823996
Conc: 117.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-28A


Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:59 AM

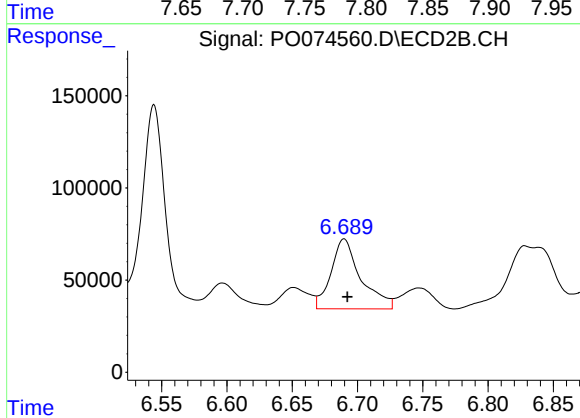


#28 AR-1254-3

R.T.: 6.690 min
Delta R.T.: -0.002 min
Response: 604709
Conc: 123.31 ng/ml

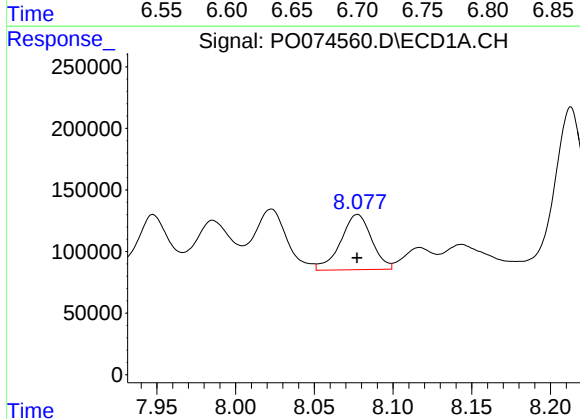


#29 AR-1254-4

R.T.: 8.077 min
Delta R.T.: 0.000 min
Response: 614871
Conc: 101.39 ng/ml

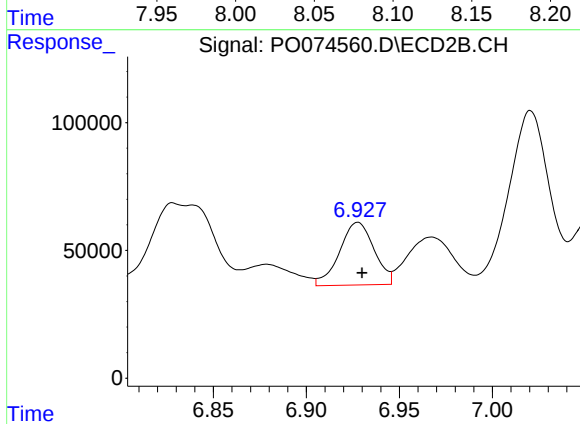

#29 AR-1254-4

R.T.: 6.928 min
Delta R.T.: -0.002 min
Response: 317687
Conc: 91.61 ng/ml

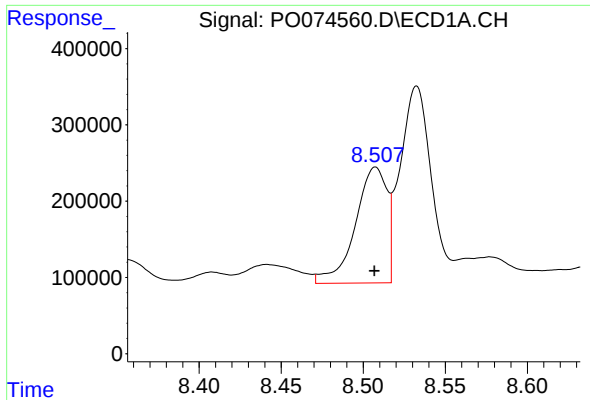


#30 AR-1254-5

R.T.: 8.507 min
Delta R.T.: 0.000 min
Response: 2041024
Conc: 351.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-28A

Manual Integrations
APPROVED

Ankita
1/13/2021 11:27:59 AM

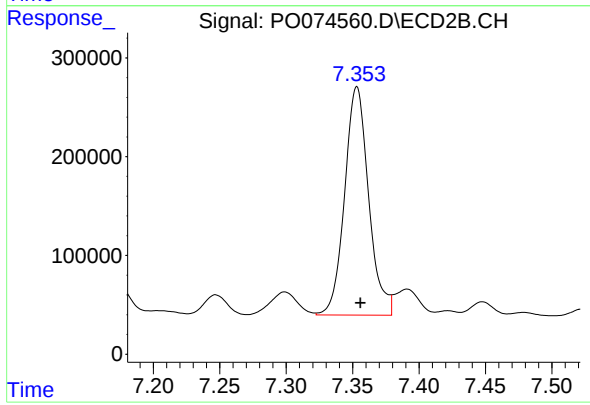

#30 AR-1254-5

R.T.: 7.353 min
Delta R.T.: -0.003 min
Response: 2911577
Conc: 643.31 ng/ml