

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011221\
 Data File : P0074561.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 00:23
 Operator : AJ/MA
 Sample : M1095-19
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-28B

Manual Integrations
 APPROVED

Ankita
 1/13/2021 11:28:01 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 01:10:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.004	1972511	1108026	18.694	19.697
2) SA Decachlor...	10.949	9.256	1393797	747416	13.733	13.613
Target Compounds						
26) L6 AR-1254-1	7.158	6.112	66470	122125	15.113m	33.811m#
27) L6 AR-1254-2	7.397	6.271	560973	301358	82.366	96.696
28) L6 AR-1254-3	7.781	6.687	657966	568187	93.803	115.864
29) L6 AR-1254-4	8.075	6.925	533559	215592	87.978	62.170 #
30) L6 AR-1254-5	8.505	7.351	1720701	2863147	296.216	632.608 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011221\
Data File : PO074561.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 00:23
Operator : AJ/MA
Sample : M1095-19
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-28B


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:01 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 01:10:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

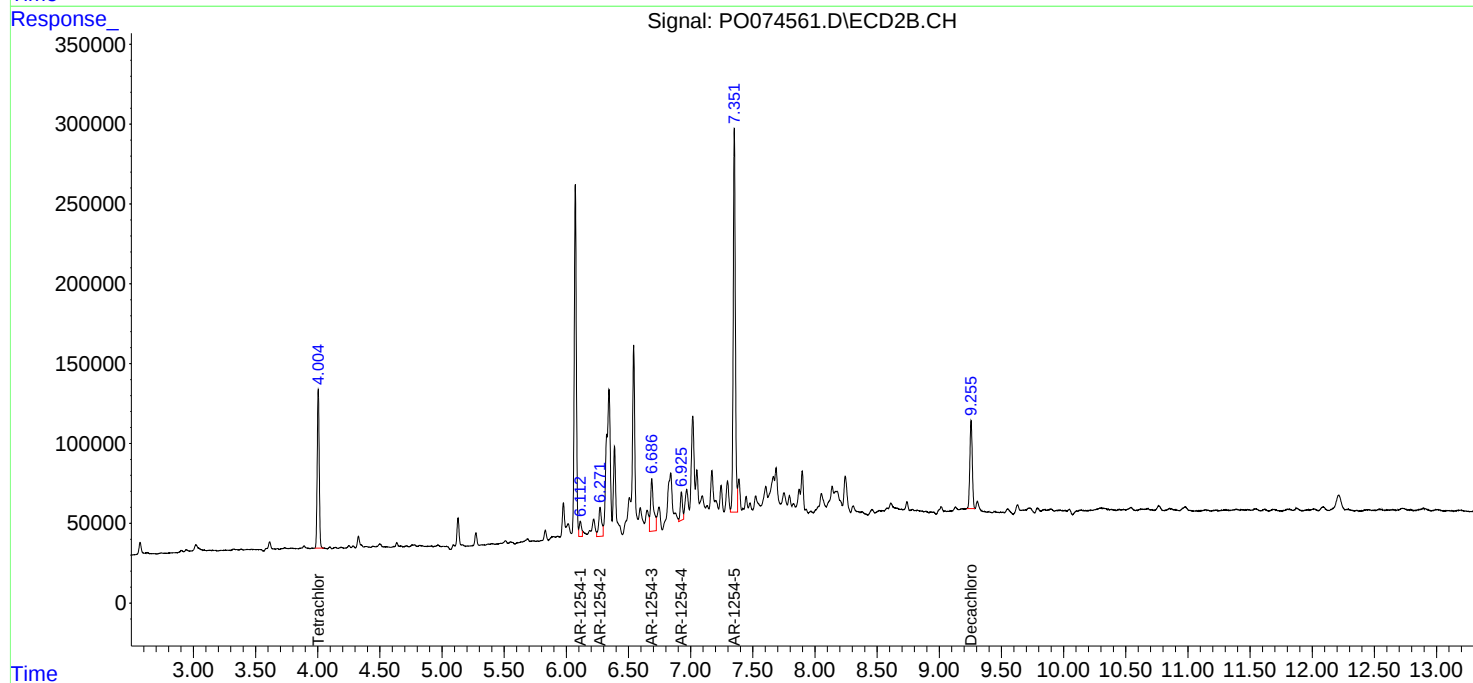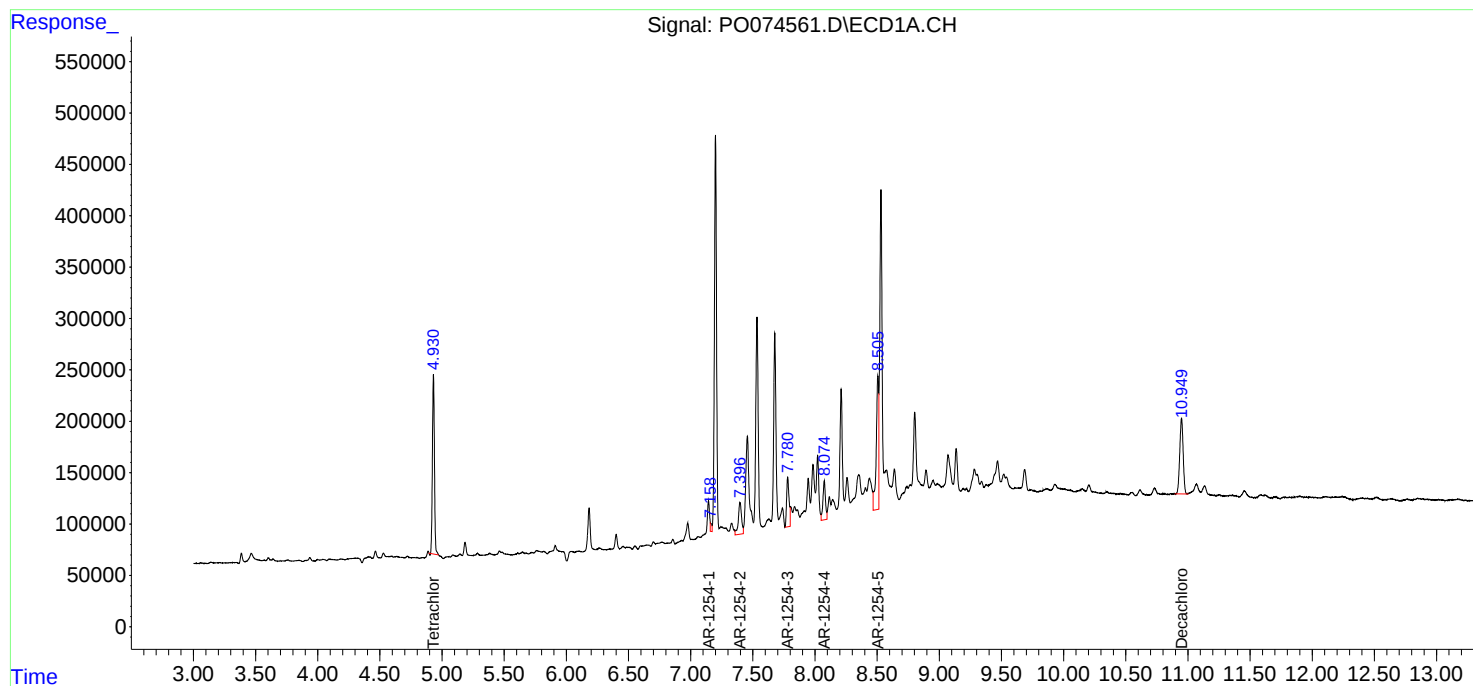

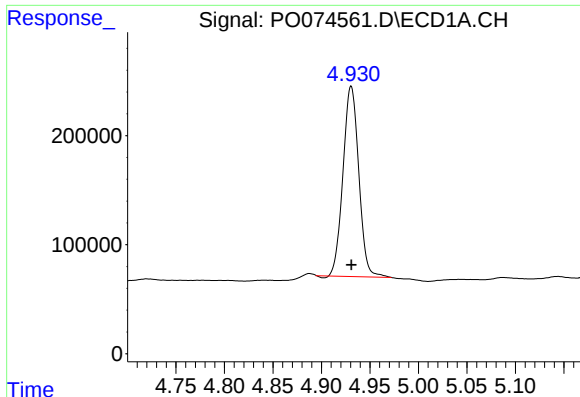


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 1972511
Conc: 18.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-28B


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:01 AM

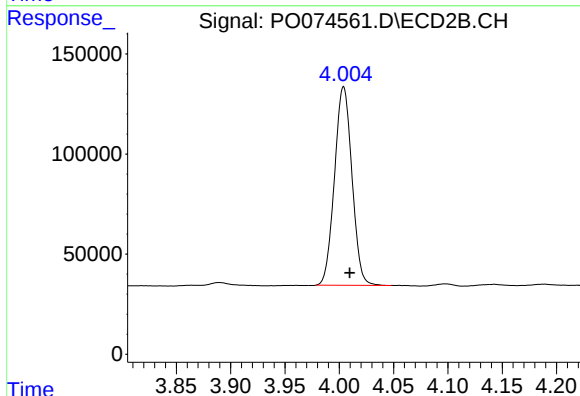


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.006 min
Response: 1108026
Conc: 19.70 ng/ml

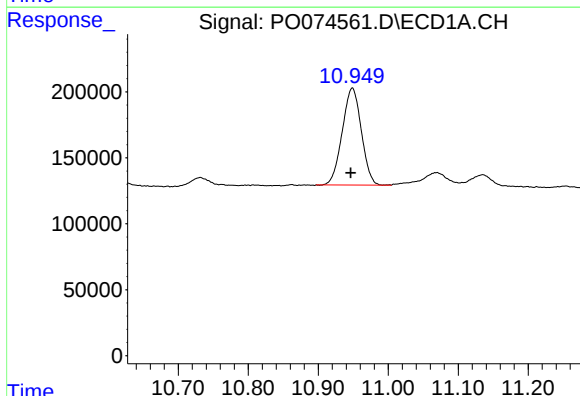


#2 Decachlorobiphenyl

R.T.: 10.949 min
Delta R.T.: 0.002 min
Response: 1393797
Conc: 13.73 ng/ml

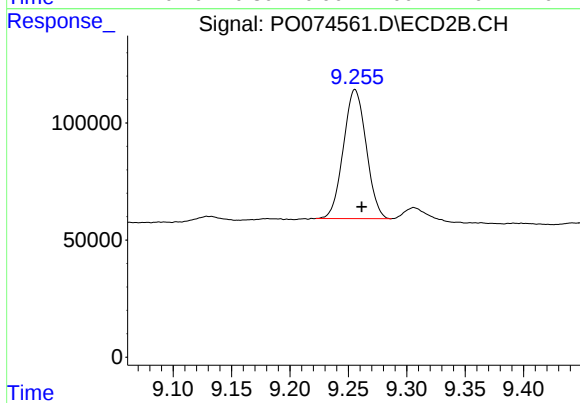

#2 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.006 min
Response: 747416
Conc: 13.61 ng/ml

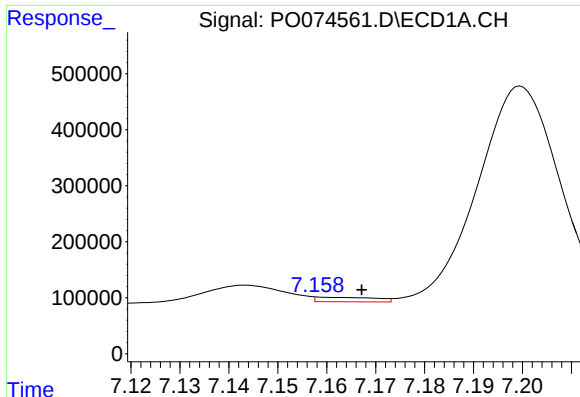


#26 AR-1254-1

R.T.: 7.158 min
Delta R.T.: -0.010 min
Response: 66470
Conc: 15.11 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-28B


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:01 AM

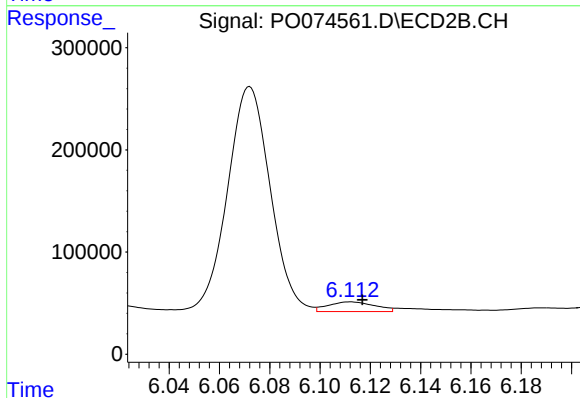


#26 AR-1254-1

R.T.: 6.112 min
Delta R.T.: -0.005 min
Response: 122125
Conc: 33.81 ng/ml m

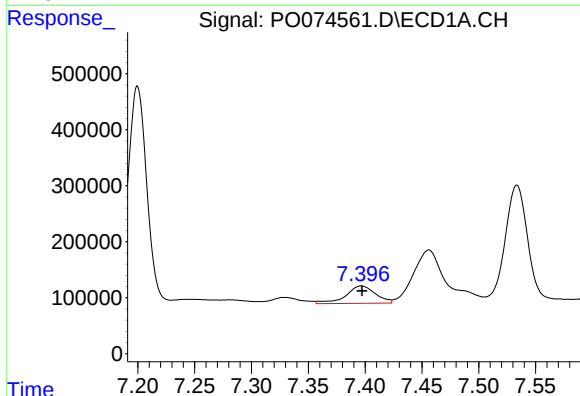


#27 AR-1254-2

R.T.: 7.397 min
Delta R.T.: 0.000 min
Response: 560973
Conc: 82.37 ng/ml

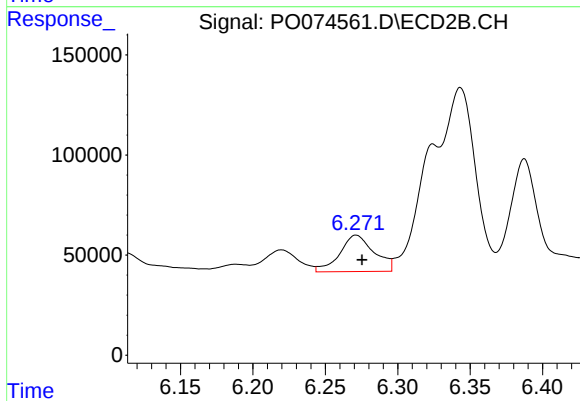

#27 AR-1254-2

R.T.: 6.271 min
Delta R.T.: -0.004 min
Response: 301358
Conc: 96.70 ng/ml

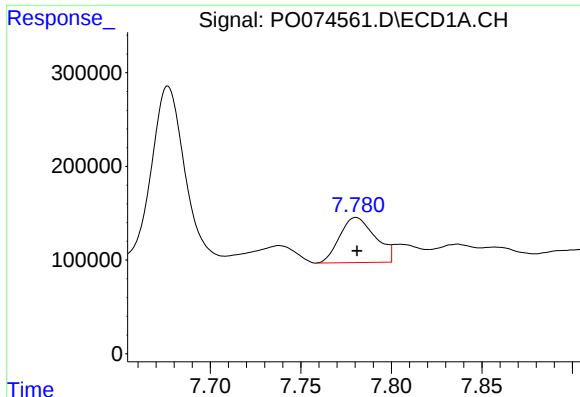


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 657966
Conc: 93.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-28B


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:01 AM

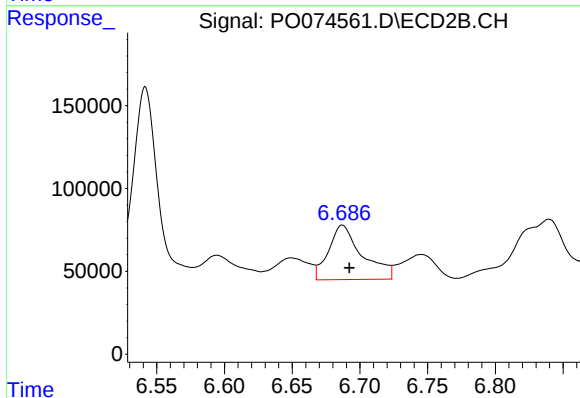


#28 AR-1254-3

R.T.: 6.687 min
Delta R.T.: -0.005 min
Response: 568187
Conc: 115.86 ng/ml

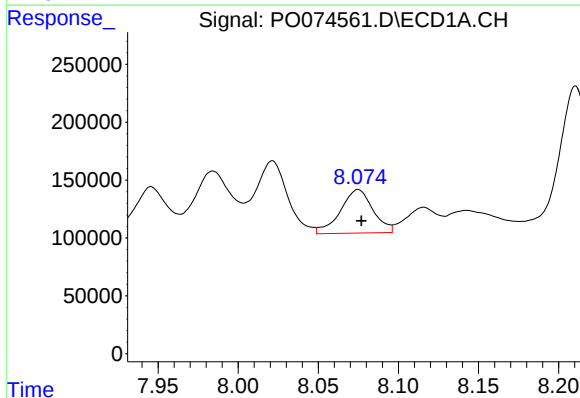


#29 AR-1254-4

R.T.: 8.075 min
Delta R.T.: -0.002 min
Response: 533559
Conc: 87.98 ng/ml

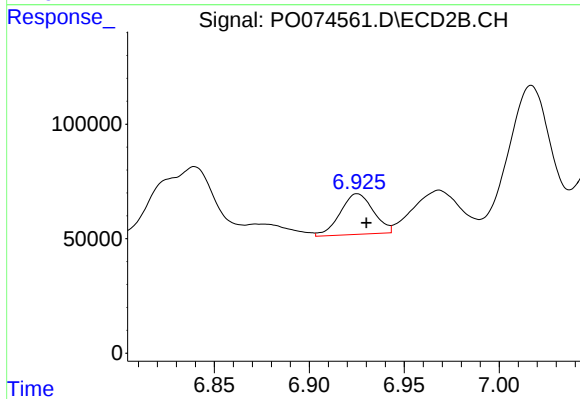

#29 AR-1254-4

R.T.: 6.925 min
Delta R.T.: -0.005 min
Response: 215592
Conc: 62.17 ng/ml

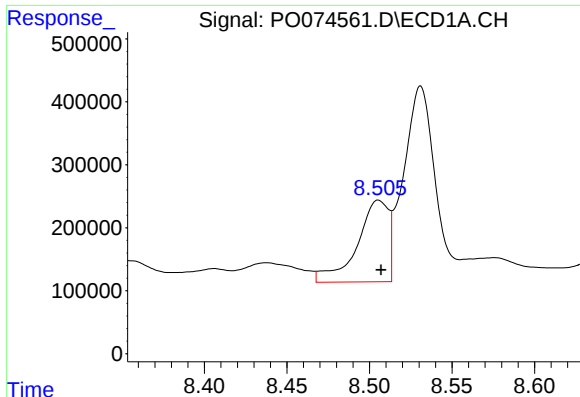


#30 AR-1254-5

R.T.: 8.505 min
Delta R.T.: -0.001 min
Response: 1720701
Conc: 296.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-28B

Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:01 AM

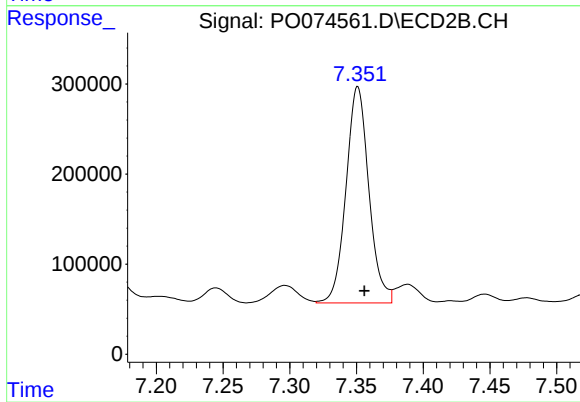

#30 AR-1254-5

R.T.: 7.351 min
Delta R.T.: -0.005 min
Response: 2863147
Conc: 632.61 ng/ml