

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011221\
 Data File : P0074566.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 1:48
 Operator : AJ/MA
 Sample : M1098-09
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 263K-DUP7

Manual Integrations
 APPROVED

Ankita
 1/13/2021 11:28:10 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 02:18:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.931	4.004	2042608	1163225	19.358	20.679
2) SA Decachlor...	10.948	9.257	1318019	809224	12.986	14.739
Target Compounds						
26) L6 AR-1254-1	7.164	6.113	91098	118369	20.713m	32.771 #
27) L6 AR-1254-2	7.396	6.272	626060	264536	91.922	84.881
28) L6 AR-1254-3	7.781	6.688	987348	691486	140.762	141.007
29) L6 AR-1254-4	8.076	6.926	882518	452416	145.518	130.463
30) L6 AR-1254-5	8.505	7.352	2658146	3578943	457.596	790.762 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011221\
Data File : PO074566.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 1:48
Operator : AJ/MA
Sample : M1098-09
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
263K-DUP7


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:10 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 02:18:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

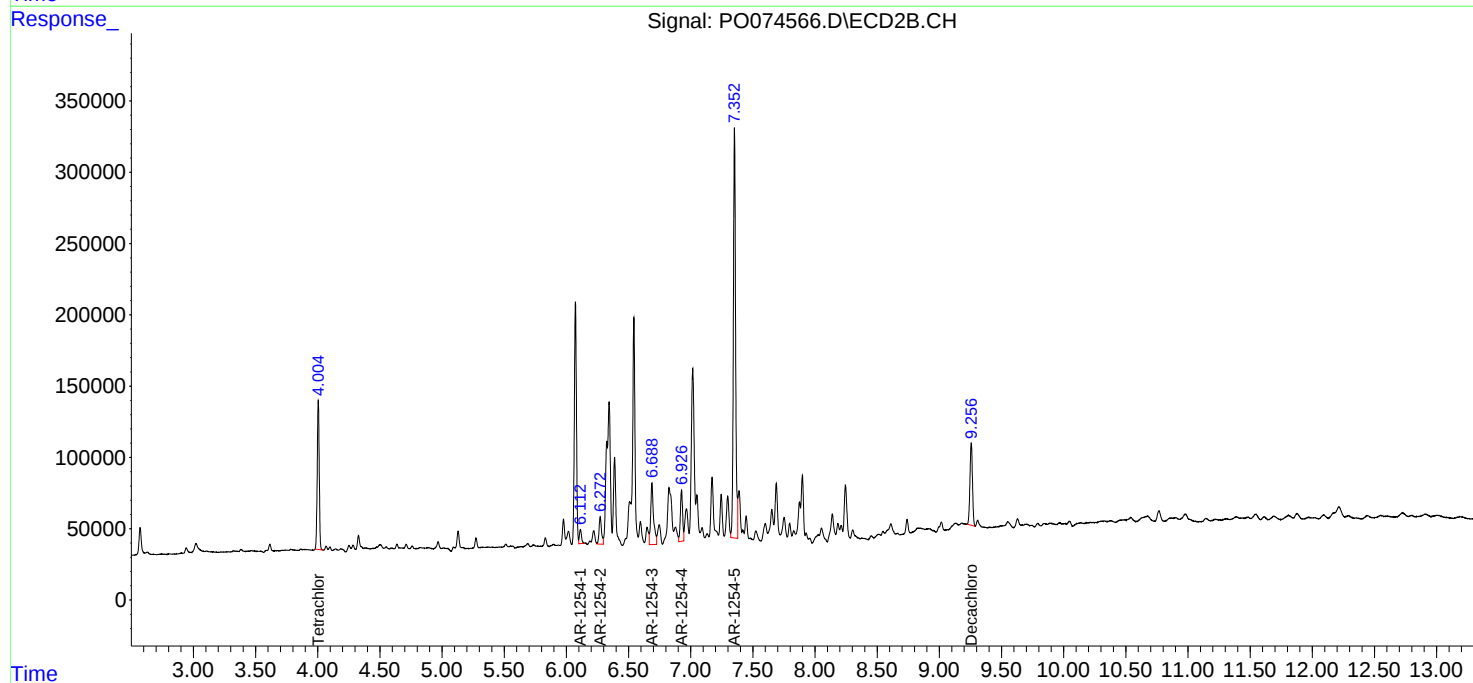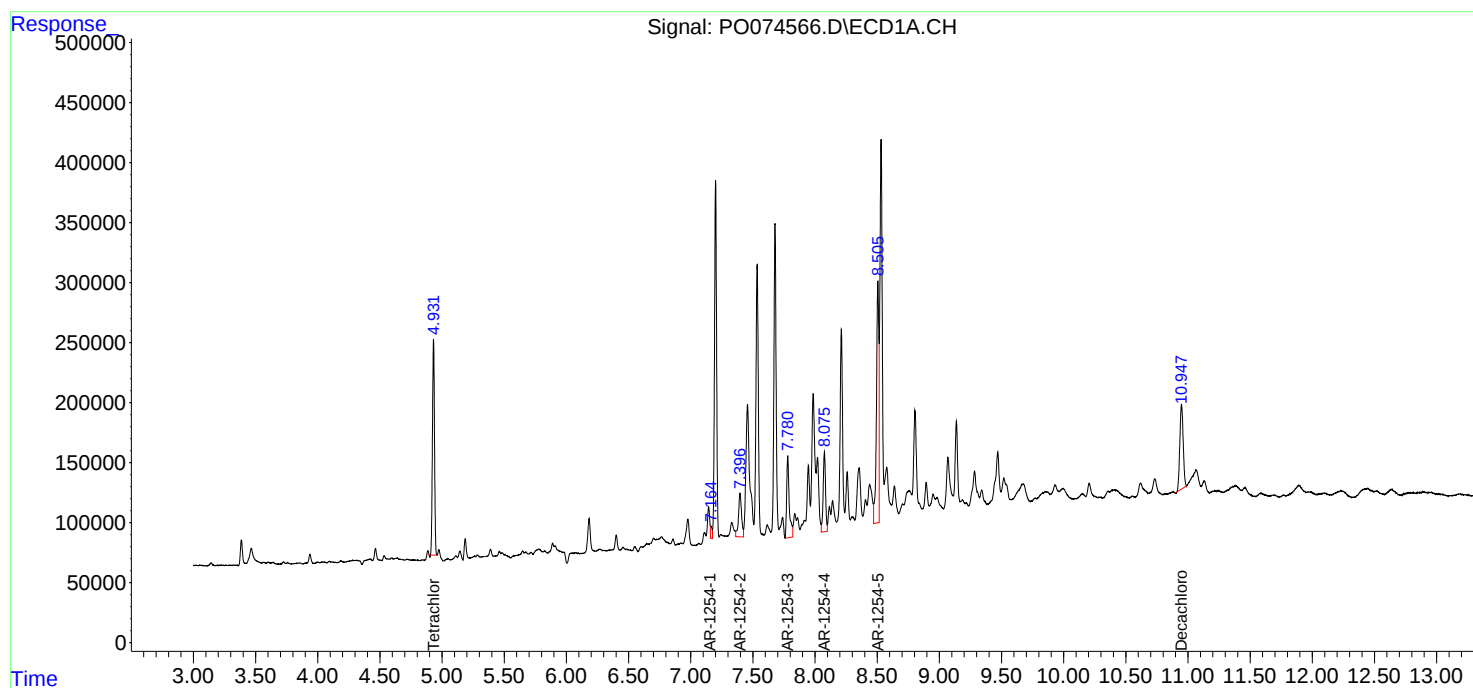

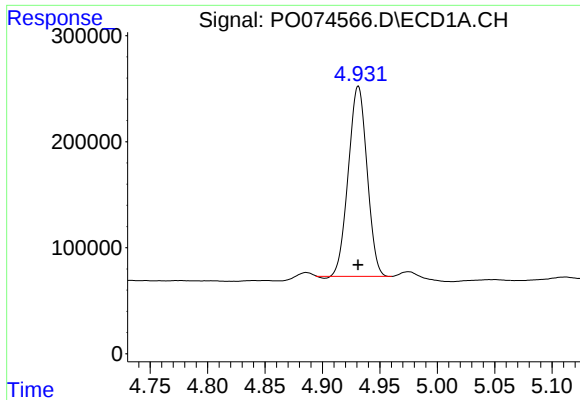


#1 Tetrachloro-m-xylene

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 2042608
Conc: 19.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-DUP7


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:10 AM

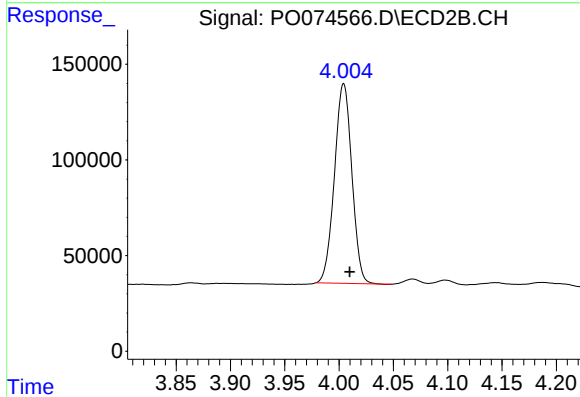


#1 Tetrachloro-m-xylene

R.T.: 4.004 min
Delta R.T.: -0.005 min
Response: 1163225
Conc: 20.68 ng/ml

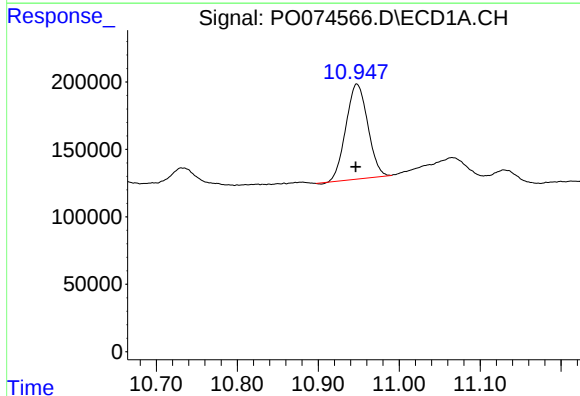


#2 Decachlorobiphenyl

R.T.: 10.948 min
Delta R.T.: 0.001 min
Response: 1318019
Conc: 12.99 ng/ml

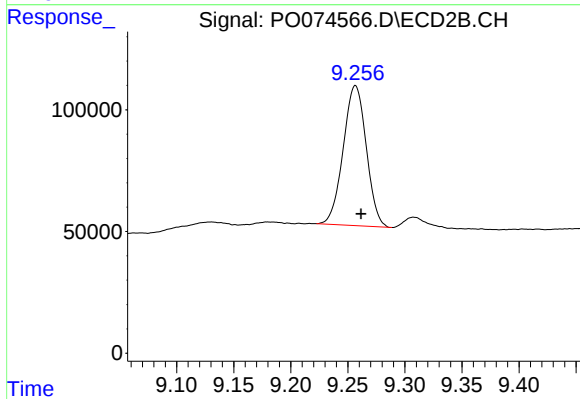

#2 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.005 min
Response: 809224
Conc: 14.74 ng/ml

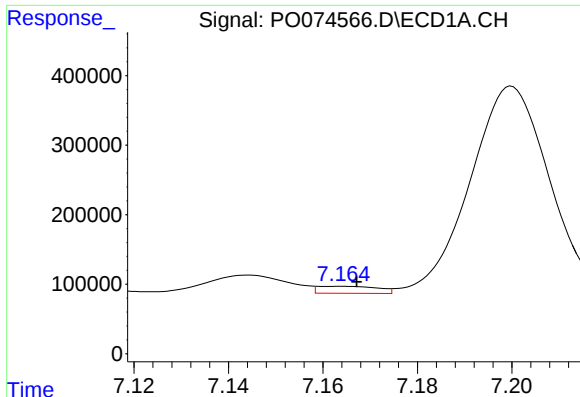


#26 AR-1254-1

R.T.: 7.164 min
Delta R.T.: -0.003 min
Response: 91098
Conc: 20.71 ng/ml m

Instrument :
ECD_O
ClientSampleId :
263K-DUP7


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:10 AM

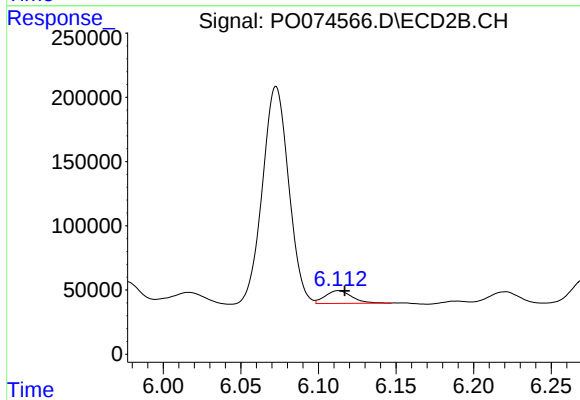


#26 AR-1254-1

R.T.: 6.113 min
Delta R.T.: -0.004 min
Response: 118369
Conc: 32.77 ng/ml

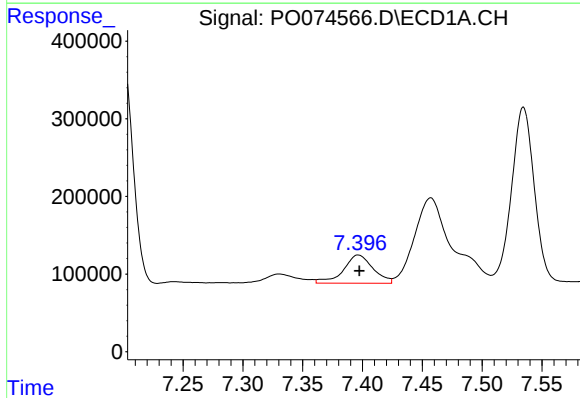


#27 AR-1254-2

R.T.: 7.396 min
Delta R.T.: 0.000 min
Response: 626060
Conc: 91.92 ng/ml

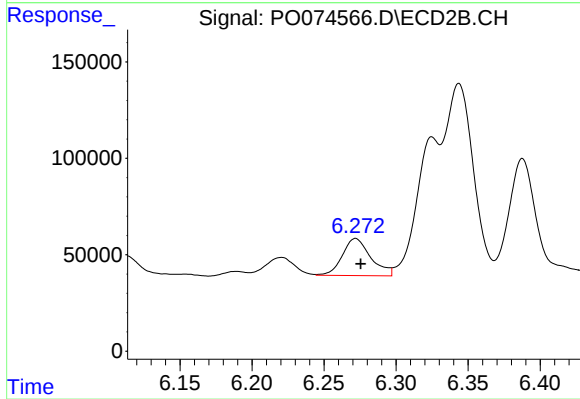

#27 AR-1254-2

R.T.: 6.272 min
Delta R.T.: -0.003 min
Response: 264536
Conc: 84.88 ng/ml

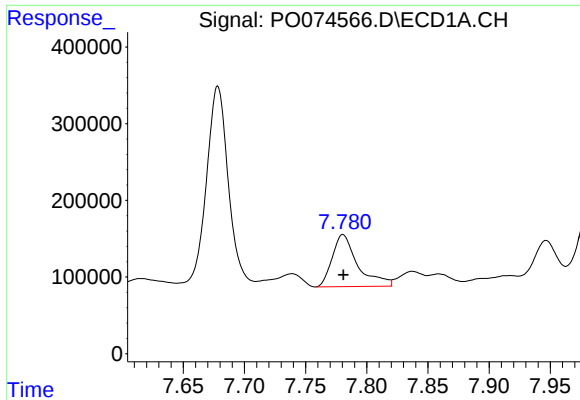


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 987348
Conc: 140.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-DUP7


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:10 AM

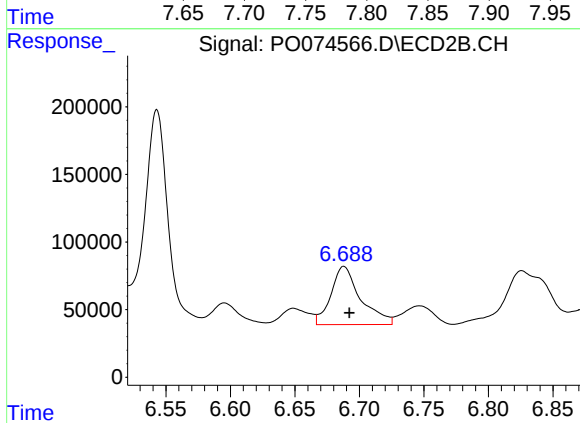


#28 AR-1254-3

R.T.: 6.688 min
Delta R.T.: -0.004 min
Response: 691486
Conc: 141.01 ng/ml

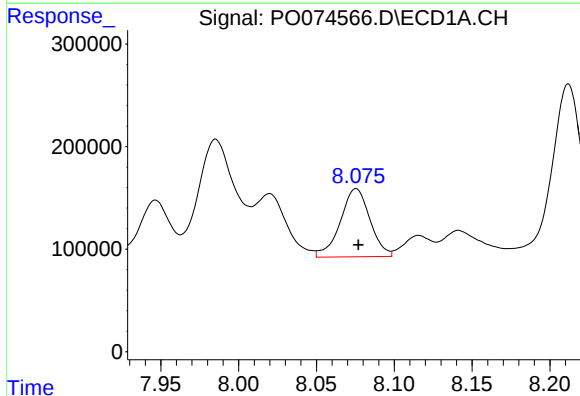


#29 AR-1254-4

R.T.: 8.076 min
Delta R.T.: -0.002 min
Response: 882518
Conc: 145.52 ng/ml

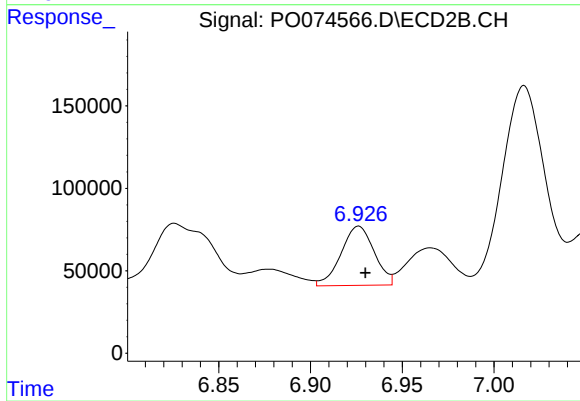

#29 AR-1254-4

R.T.: 6.926 min
Delta R.T.: -0.004 min
Response: 452416
Conc: 130.46 ng/ml

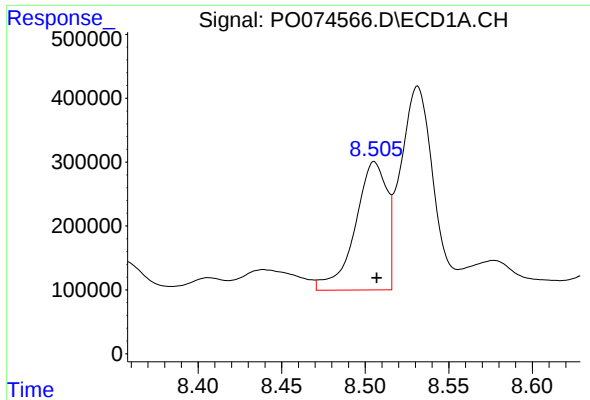


#30 AR-1254-5

R.T.: 8.505 min
Delta R.T.: -0.001 min
Response: 2658146
Conc: 457.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
263K-DUP7

Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:10 AM

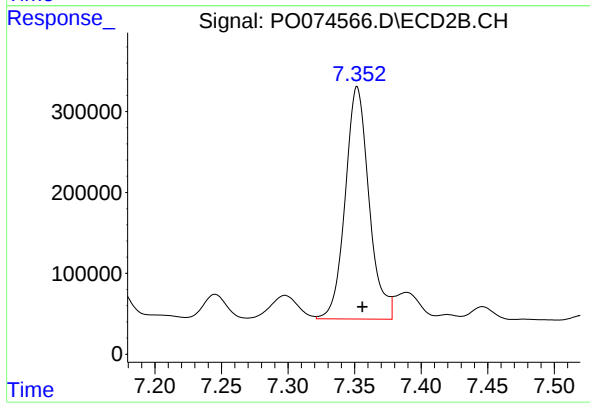

#30 AR-1254-5

R.T.: 7.352 min
Delta R.T.: -0.004 min
Response: 3578943
Conc: 790.76 ng/ml