

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011221\
 Data File : P0074567.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Jan 2021 2:06
 Operator : AJ/MA
 Sample : M1084-01DL 5X
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S1-01-BDL

Manual Integrations
 APPROVED

Ankita
 1/13/2021 11:28:12 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 03:45:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jan 12 06:02:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.933	4.006	440355	275730	4.173	4.902
2) SA Decachlor...	10.950	9.258	270508	186960	2.665	3.405 #
Target Compounds						
26) L6 AR-1254-1	7.169	6.115	702236	500621	159.667m	138.599
27) L6 AR-1254-2	7.398	6.274	1564664	748157	229.734	240.060
28) L6 AR-1254-3	7.781	6.690	1873942	1345143	267.159	274.299
29) L6 AR-1254-4	8.078	6.928	1891093	1040896	311.821	300.162
30) L6 AR-1254-5	8.507	7.354	3214443	3439169	553.362	759.879 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011221\
Data File : PO074567.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Jan 2021 2:06
Operator : AJ/MA
Sample : M1084-01DL 5X
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S1-01-BDL


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:12 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 03:45:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jan 12 06:02:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

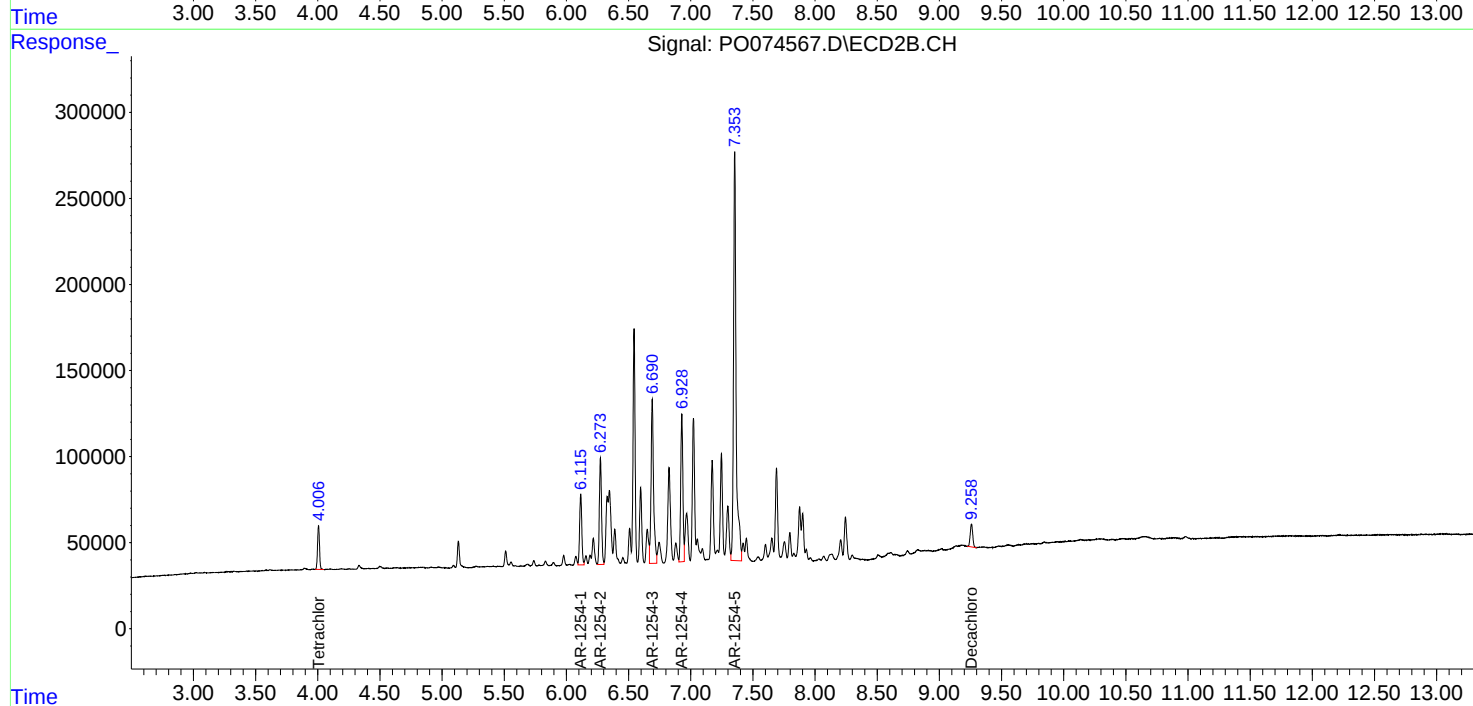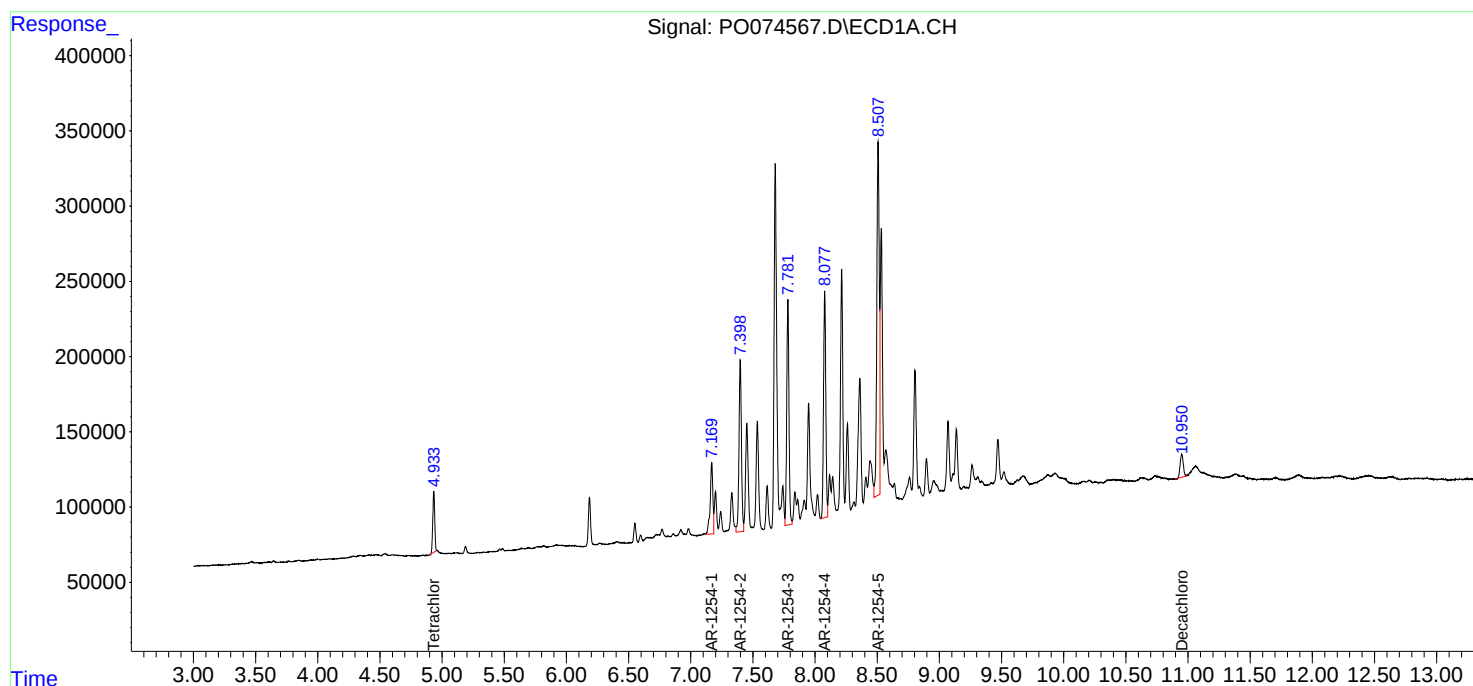

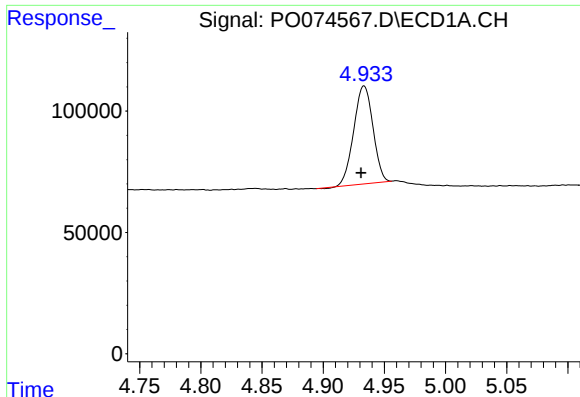


#1 Tetrachloro-m-xylene

R.T.: 4.933 min
Delta R.T.: 0.002 min
Response: 440355
Conc: 4.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-01-BDL


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:12 AM

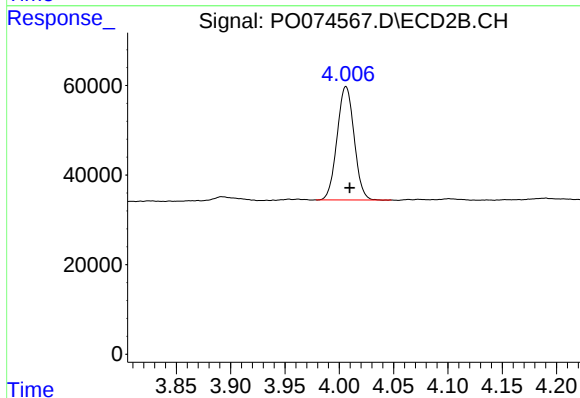


#1 Tetrachloro-m-xylene

R.T.: 4.006 min
Delta R.T.: -0.004 min
Response: 275730
Conc: 4.90 ng/ml

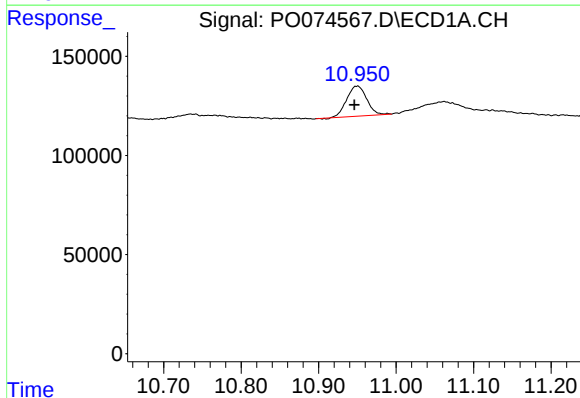


#2 Decachlorobiphenyl

R.T.: 10.950 min
Delta R.T.: 0.004 min
Response: 270508
Conc: 2.67 ng/ml

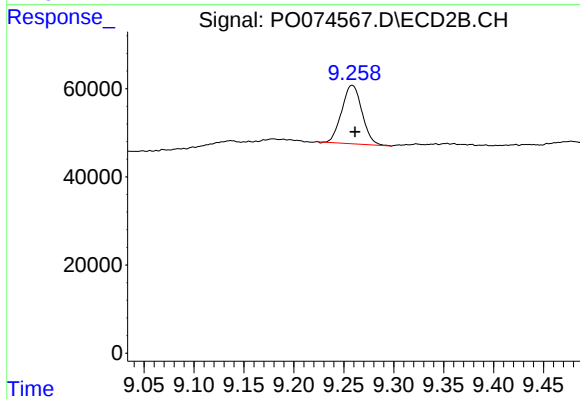

#2 Decachlorobiphenyl

R.T.: 9.258 min
Delta R.T.: -0.003 min
Response: 186960
Conc: 3.41 ng/ml

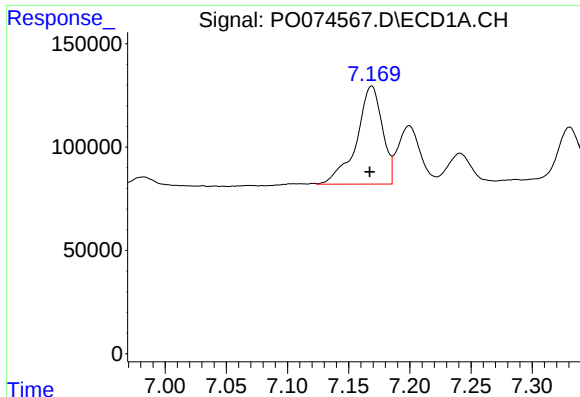


#26 AR-1254-1

R.T.: 7.169 min
Delta R.T.: 0.001 min
Response: 702236
Conc: 159.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S1-01-BDL


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:12 AM

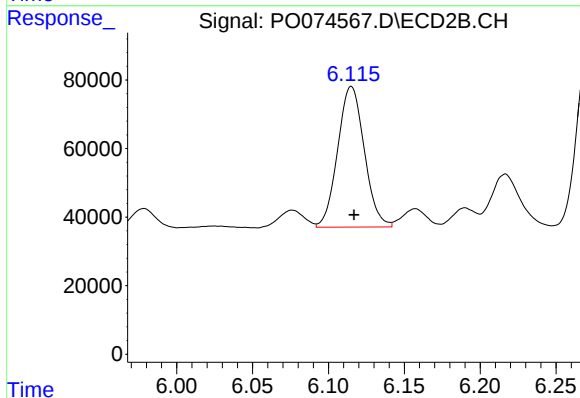


#26 AR-1254-1

R.T.: 6.115 min
Delta R.T.: -0.002 min
Response: 500621
Conc: 138.60 ng/ml

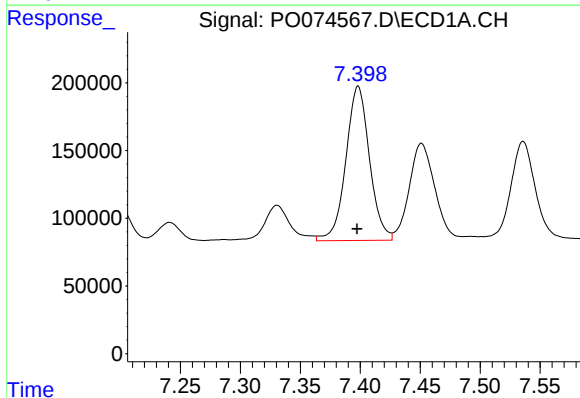


#27 AR-1254-2

R.T.: 7.398 min
Delta R.T.: 0.000 min
Response: 1564664
Conc: 229.73 ng/ml

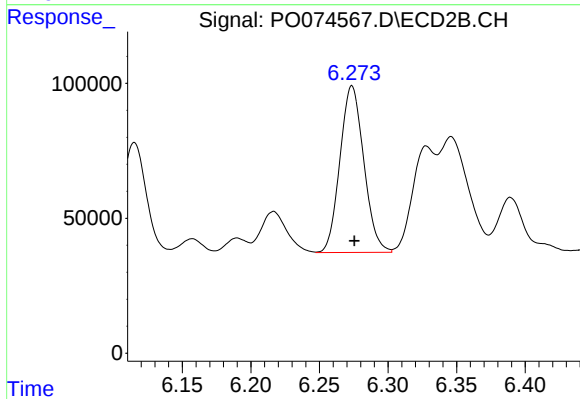

#27 AR-1254-2

R.T.: 6.274 min
Delta R.T.: -0.002 min
Response: 748157
Conc: 240.06 ng/ml

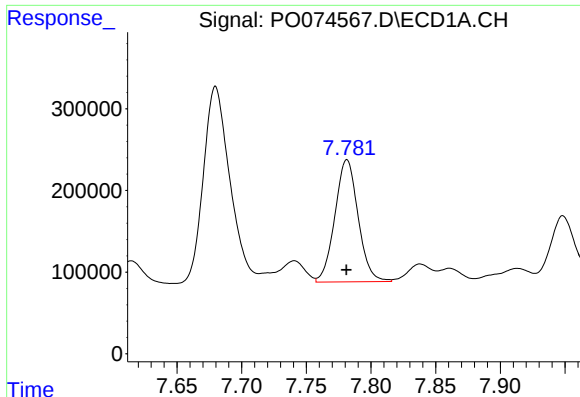


#28 AR-1254-3

R.T.: 7.781 min
Delta R.T.: 0.000 min
Response: 1873942
Conc: 267.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-01-BDL


Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:12 AM

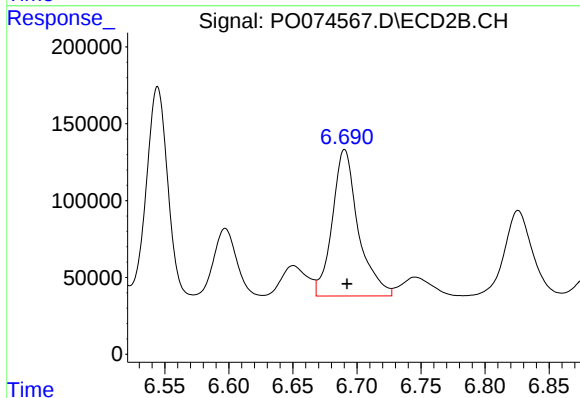


#28 AR-1254-3

R.T.: 6.690 min
Delta R.T.: -0.002 min
Response: 1345143
Conc: 274.30 ng/ml

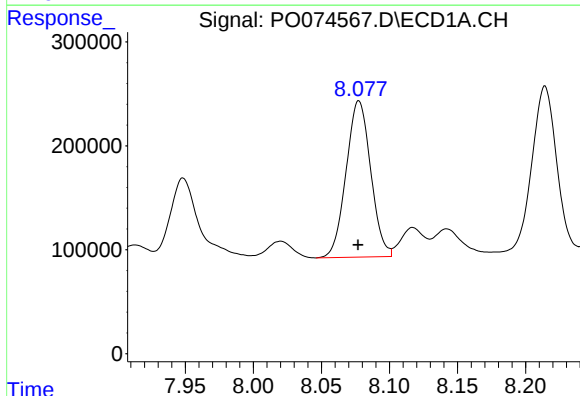


#29 AR-1254-4

R.T.: 8.078 min
Delta R.T.: 0.000 min
Response: 1891093
Conc: 311.82 ng/ml

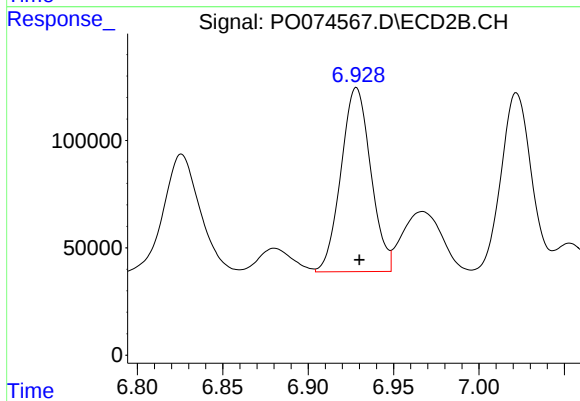

#29 AR-1254-4

R.T.: 6.928 min
Delta R.T.: -0.002 min
Response: 1040896
Conc: 300.16 ng/ml

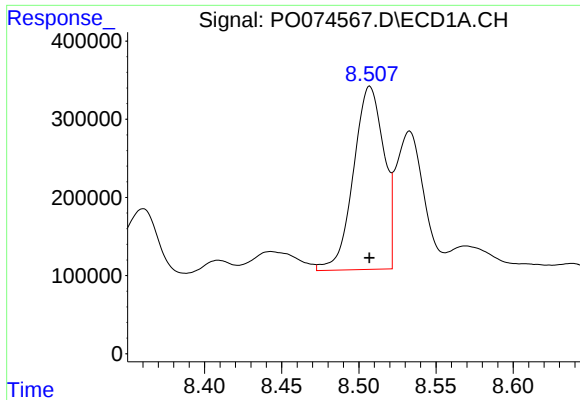


#30 AR-1254-5

R.T.: 8.507 min
Delta R.T.: 0.000 min
Response: 3214443
Conc: 553.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-01-BDL

Manual Integrations
APPROVED

Ankita
1/13/2021 11:28:12 AM

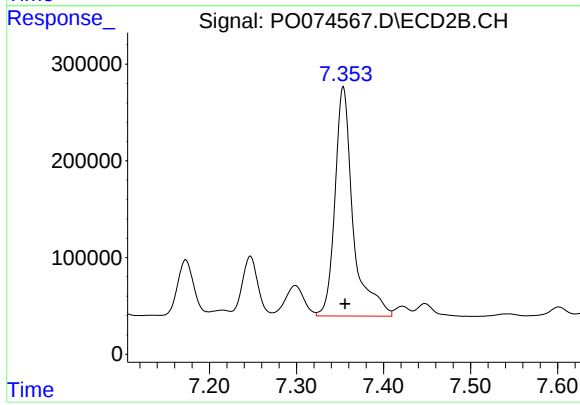

#30 AR-1254-5

R.T.: 7.354 min
Delta R.T.: -0.002 min
Response: 3439169
Conc: 759.88 ng/ml