

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011223\
 Data File : P0092002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2023 20:58
 Operator : YP/AJ
 Sample : 01102-12 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KZA4310-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 01/13/2023
 Supervised By :Ankita Jodhani 01/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 04:54:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011023.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jan 11 04:41:00 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.446	3.648	4045360	2711703	1.450m	1.953 #
2) SA Decachlor...	10.360	8.703	4052731	2331264	2.070m	2.629 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011223\
Data File : PO092002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2023 20:58
Operator : YP/AJ
Sample : 01102-12 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KZA4310-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/13/2023
Supervised By :Ankita Jodhani 01/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 04:54:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011023.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jan 11 04:41:00 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

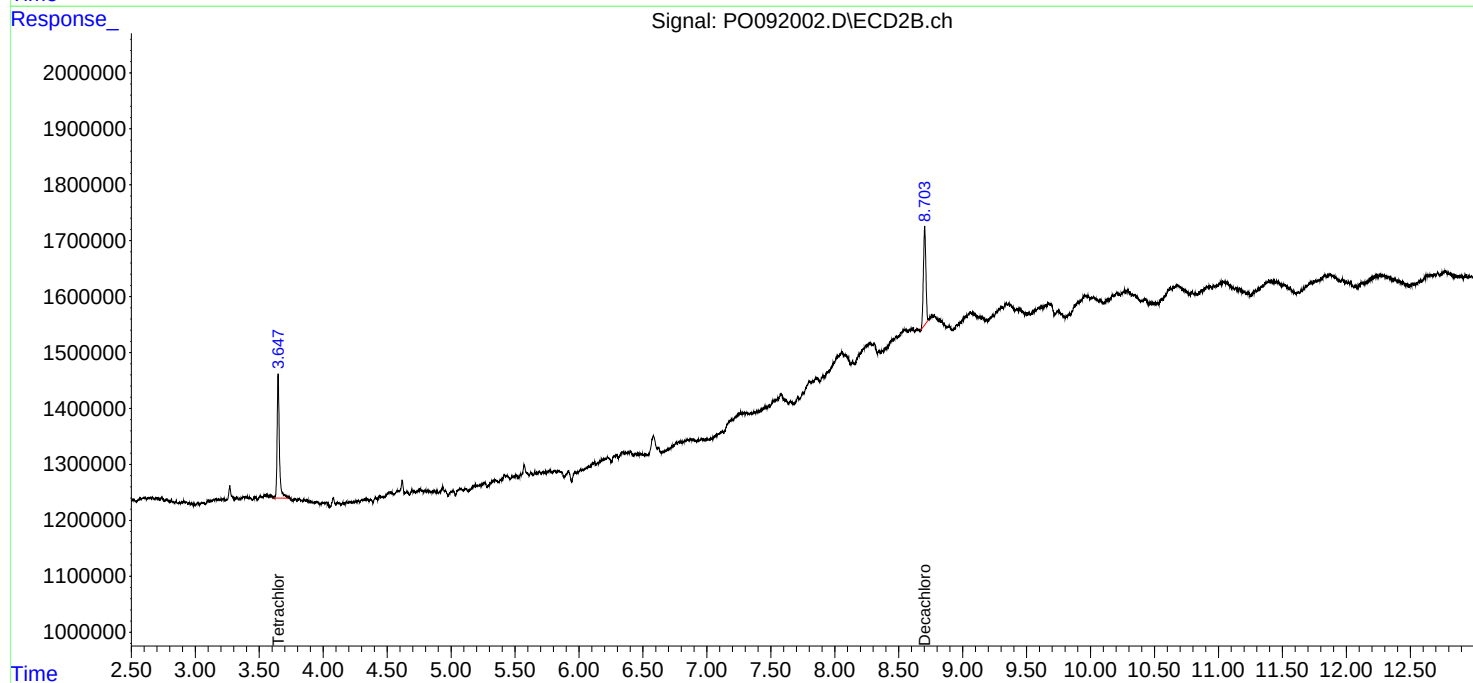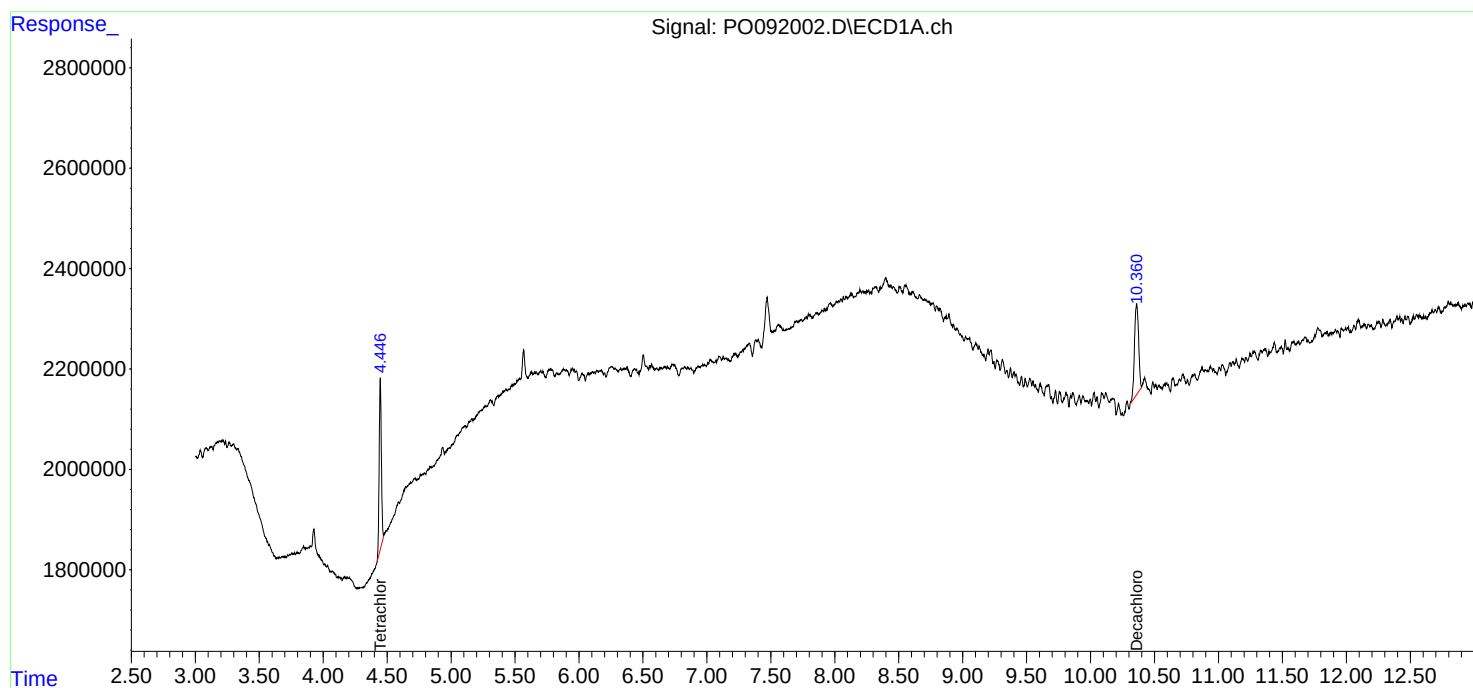

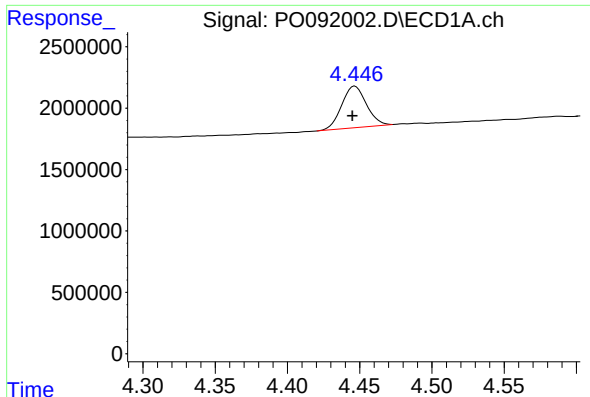


#1 Tetrachloro-m-xylene

R.T.: 4.446 min
Delta R.T.: 0.000 min
Response: 4045360
Conc: 1.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
KZA4310-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 01/13/2023
Supervised By :Ankita Jodhani 01/13/2023

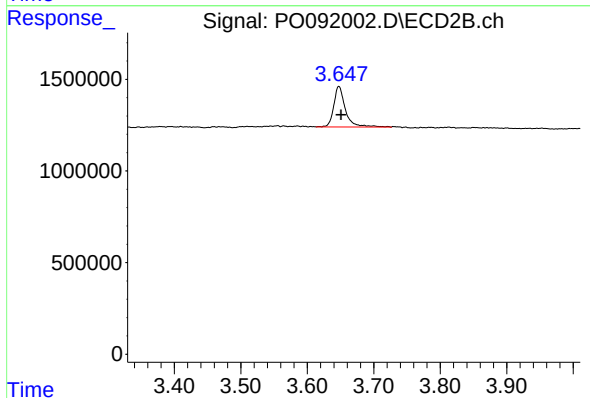


#1 Tetrachloro-m-xylene

R.T.: 3.648 min
Delta R.T.: -0.003 min
Response: 2711703
Conc: 1.95 ng/ml

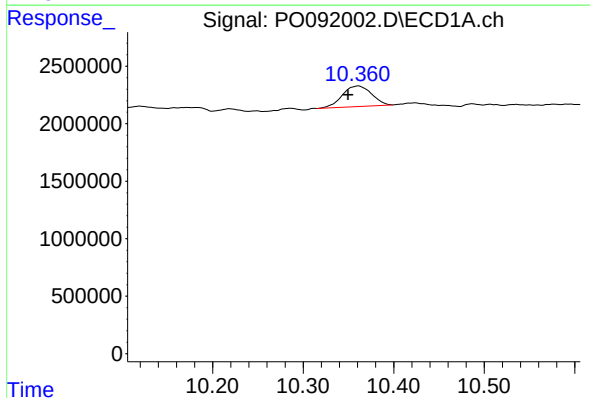

#2 Decachlorobiphenyl

R.T.: 10.360 min
Delta R.T.: 0.011 min
Response: 4052731
Conc: 2.07 ng/ml m

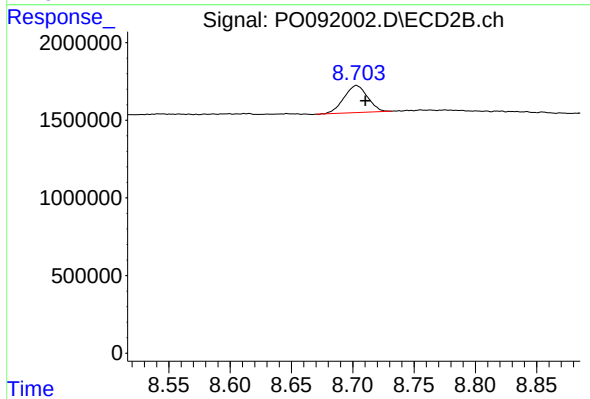

#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: -0.007 min
Response: 2331264
Conc: 2.63 ng/ml