

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011224\
 Data File : P0101131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2024 13:08
 Operator : YP/AJ
 Sample : P1111-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DRYER-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 23:02:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 11 11:52:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.341	3.637	100.7E6	64020665	24.854	24.285
2) SA Decachlor...	10.079	8.690	69931337	50531610	35.407	30.597m
Target Compounds						
26) L6 AR-1254-1	6.366	5.541	104.5E6	103.6E6	870.497	849.961
27) L6 AR-1254-2	6.586	5.689	224.4E6	135.2E6	1315.075	1266.411
28) L6 AR-1254-3	6.953	6.098	306.4E6	264.6E6	1917.441	1679.789
29) L6 AR-1254-4	7.240	6.327	294.8E6	222.3E6	2967.269	2671.865
30) L6 AR-1254-5	7.661	6.748	502.2E6	492.8E6	4213.177	3670.699



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011224\
Data File : PO101131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2024 13:08
Operator : YP/AJ
Sample : P1111-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DRYER-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 23:02:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011024.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 11 11:52:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

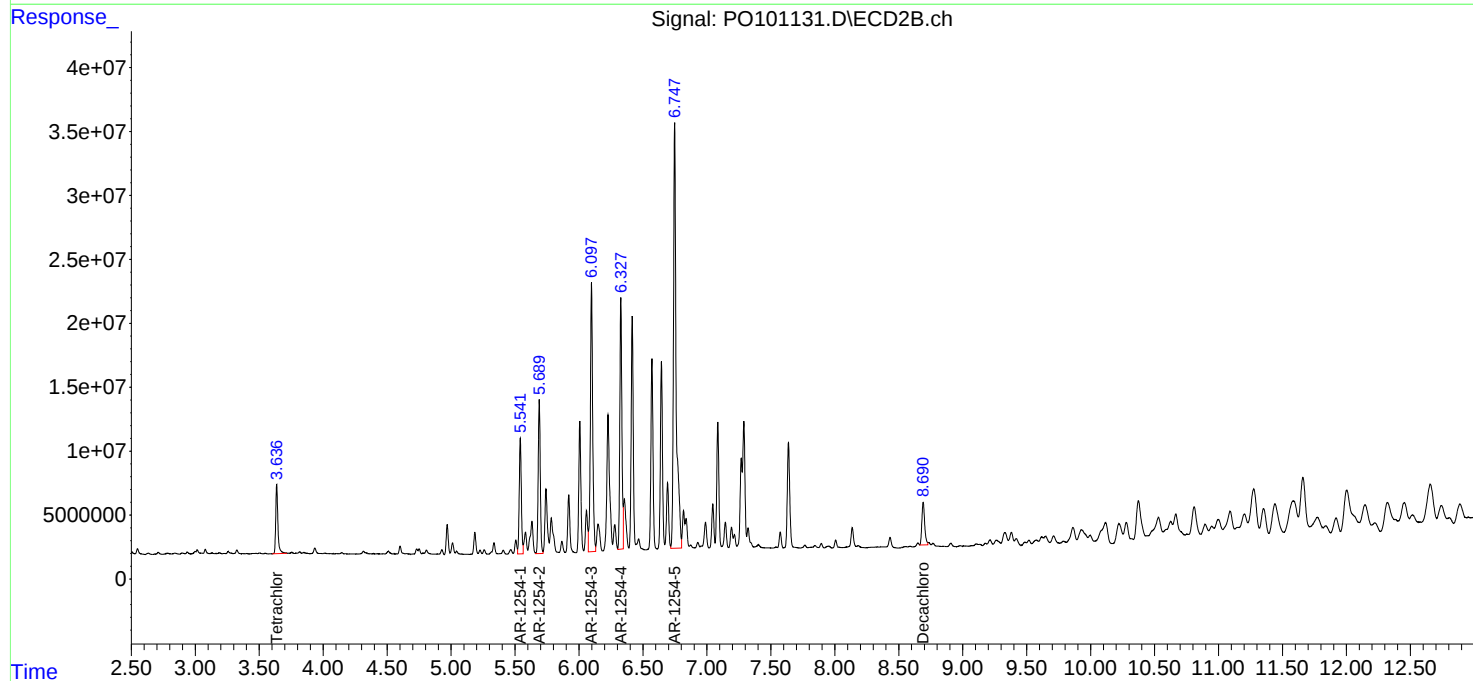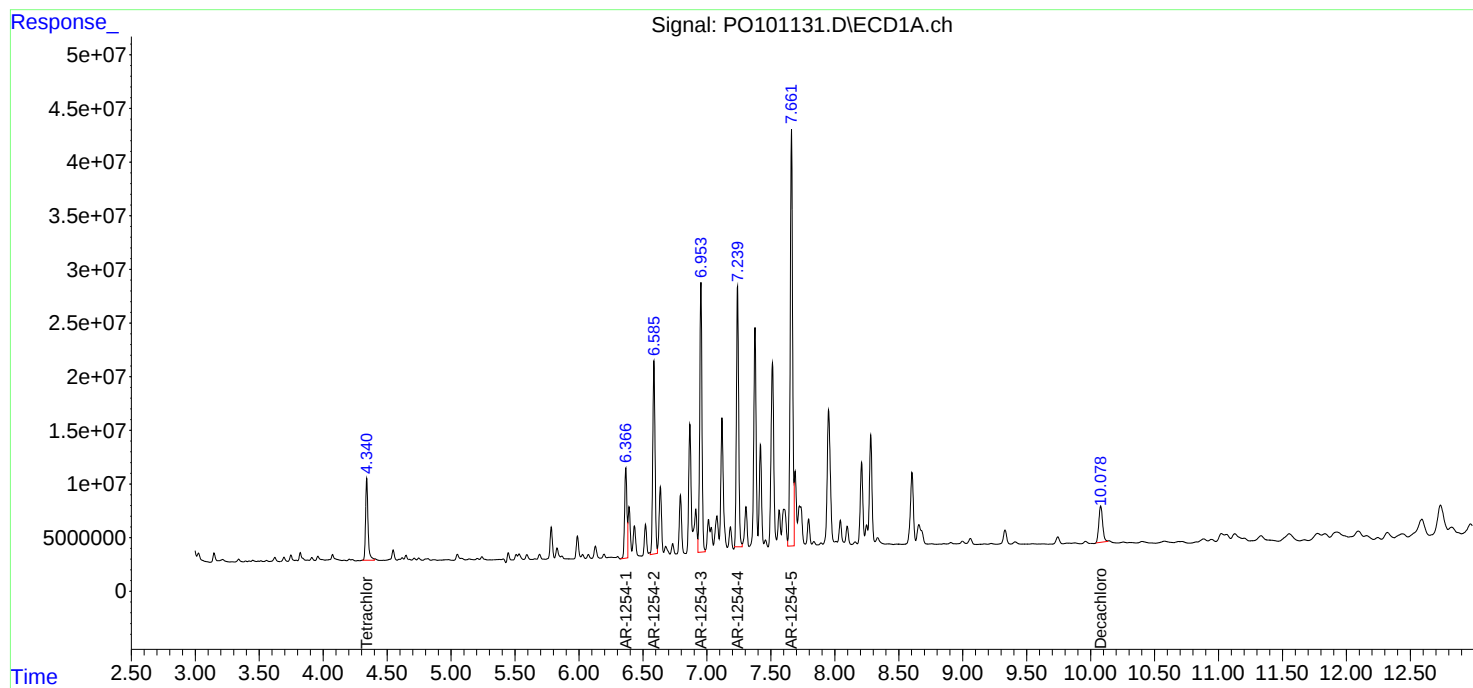


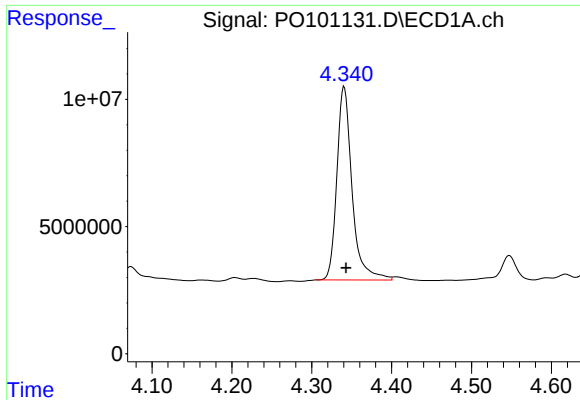

#1 Tetrachloro-m-xylene


R.T.: 4.341 min
Delta R.T.: -0.002 min
Response: 100672949
Conc: 24.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-1

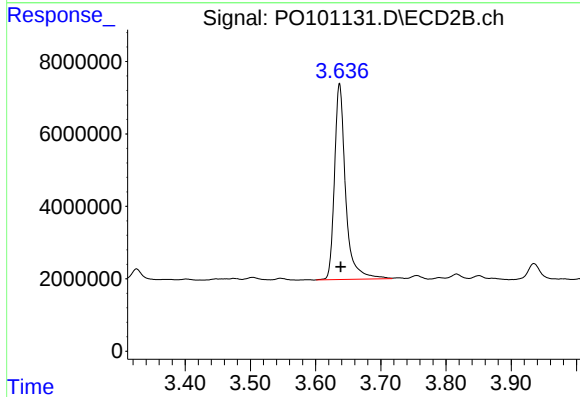


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.002 min
Response: 64020665
Conc: 24.29 ng/ml

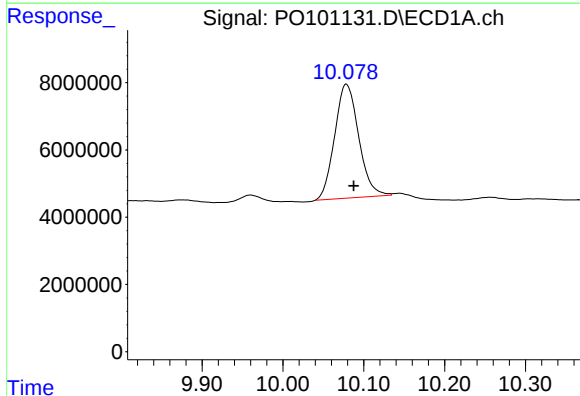


#2 Decachlorobiphenyl

R.T.: 10.079 min
Delta R.T.: -0.009 min
Response: 69931337
Conc: 35.41 ng/ml

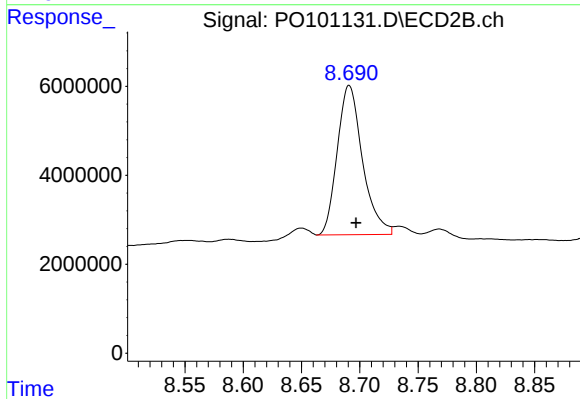

#2 Decachlorobiphenyl


R.T.: 8.690 min
Delta R.T.: -0.006 min
Response: 50531610
Conc: 30.60 ng/ml m

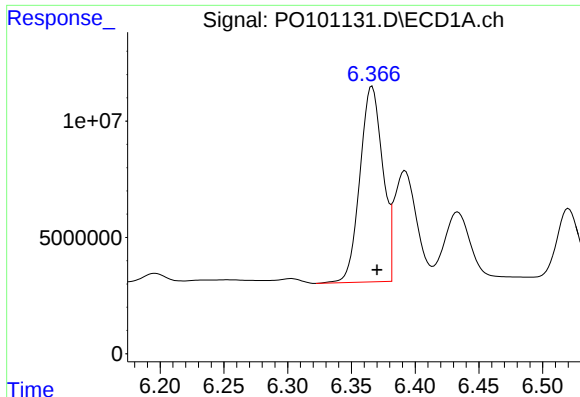

#26 AR-1254-1


R.T.: 6.366 min
Delta R.T.: -0.004 min
Response: 104484820
Conc: 870.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-1

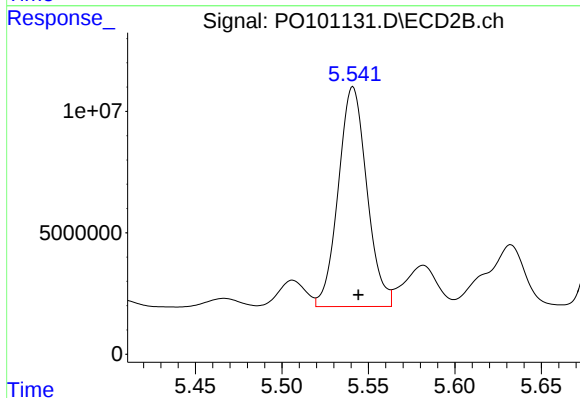


#26 AR-1254-1

R.T.: 5.541 min
Delta R.T.: -0.003 min
Response: 103631462
Conc: 849.96 ng/ml

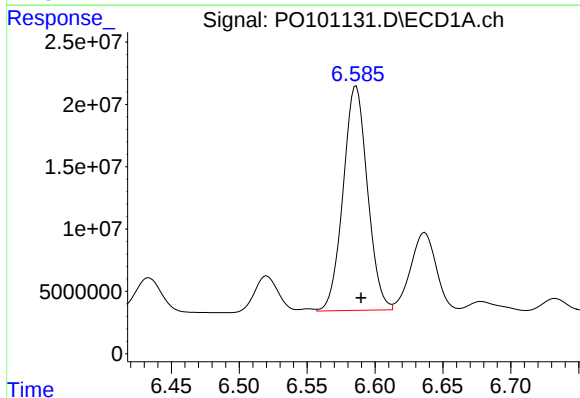


#27 AR-1254-2

R.T.: 6.586 min
Delta R.T.: -0.004 min
Response: 224437280
Conc: 1315.07 ng/ml

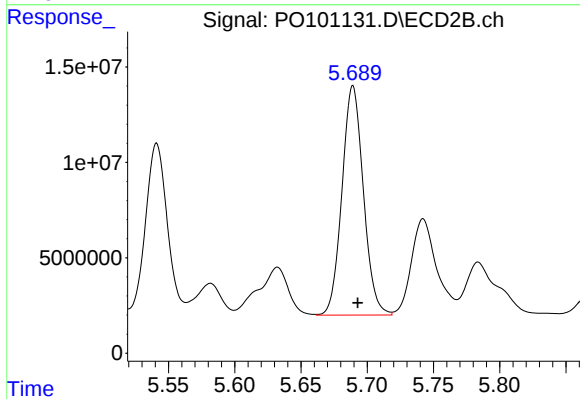

#27 AR-1254-2


R.T.: 5.689 min
Delta R.T.: -0.004 min
Response: 135214312
Conc: 1266.41 ng/ml

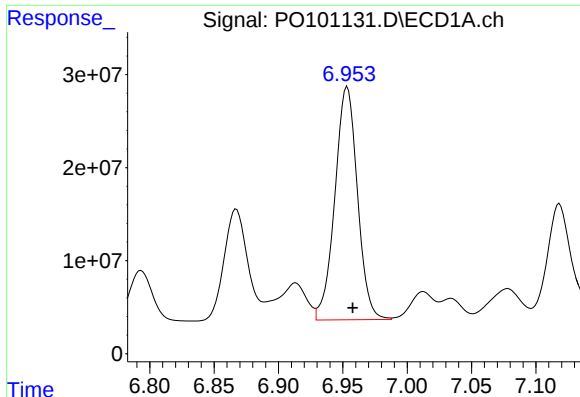

#28 AR-1254-3


R.T.: 6.953 min
Delta R.T.: -0.004 min
Response: 306373914
Conc: 1917.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-1

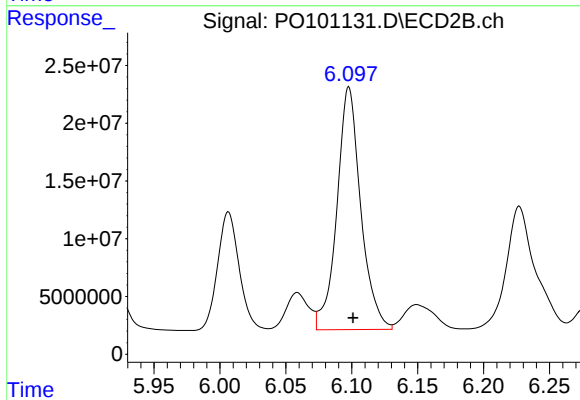


#28 AR-1254-3

R.T.: 6.098 min
Delta R.T.: -0.003 min
Response: 264616863
Conc: 1679.79 ng/ml

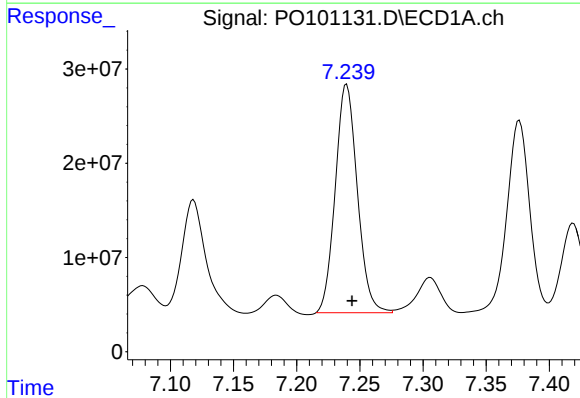


#29 AR-1254-4

R.T.: 7.240 min
Delta R.T.: -0.004 min
Response: 294848994
Conc: 2967.27 ng/ml

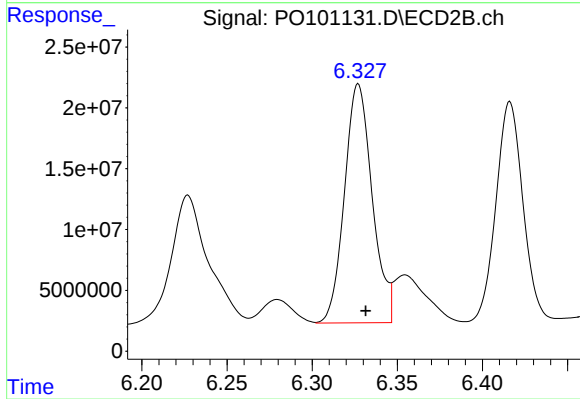

#29 AR-1254-4


R.T.: 6.327 min
Delta R.T.: -0.004 min
Response: 222342872
Conc: 2671.86 ng/ml

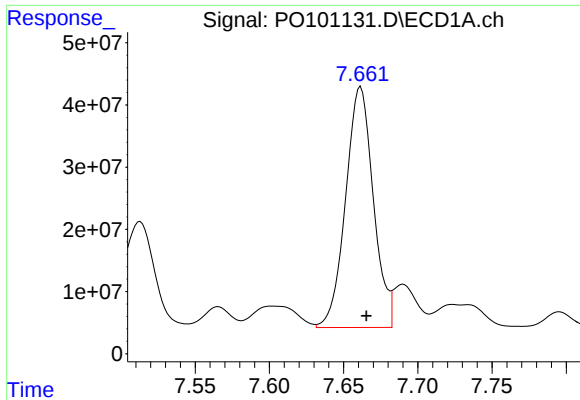

#30 AR-1254-5

R.T.: 7.661 min
Delta R.T.: -0.004 min
Response: 502225144
Conc: 4213.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-1

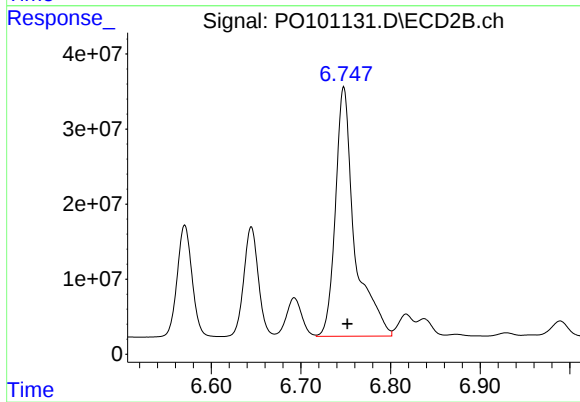

#30 AR-1254-5

R.T.: 6.748 min
Delta R.T.: -0.004 min
Response: 492788897
Conc: 3670.70 ng/ml