

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011224\
 Data File : P0101148.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2024 17:52
 Operator : YP/AJ
 Sample : P1111-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DRYER-13

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 23:09:23 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 11 11:52:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.340	3.637	80127992	60845870	19.782m	23.081
2)	SA Decachlor...	10.080	8.691	60777861	48671054	30.773	29.471
Target Compounds							
26)	L6 AR-1254-1	6.366	5.541	2679192	3021881	22.321	24.785
27)	L6 AR-1254-2	6.586	5.690	5819309	3401628	34.098	31.859
28)	L6 AR-1254-3	6.954	6.097	5103760	5194486	31.942	32.975
29)	L6 AR-1254-4	7.239	6.327	5726399	4169161	57.629m	50.100
30)	L6 AR-1254-5	7.660	6.747	10314034	9432600	86.525	70.262



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011224\
Data File : PO101148.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2024 17:52
Operator : YP/AJ
Sample : P1111-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DRYER-13

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 23:09:23 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011024.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 11 11:52:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

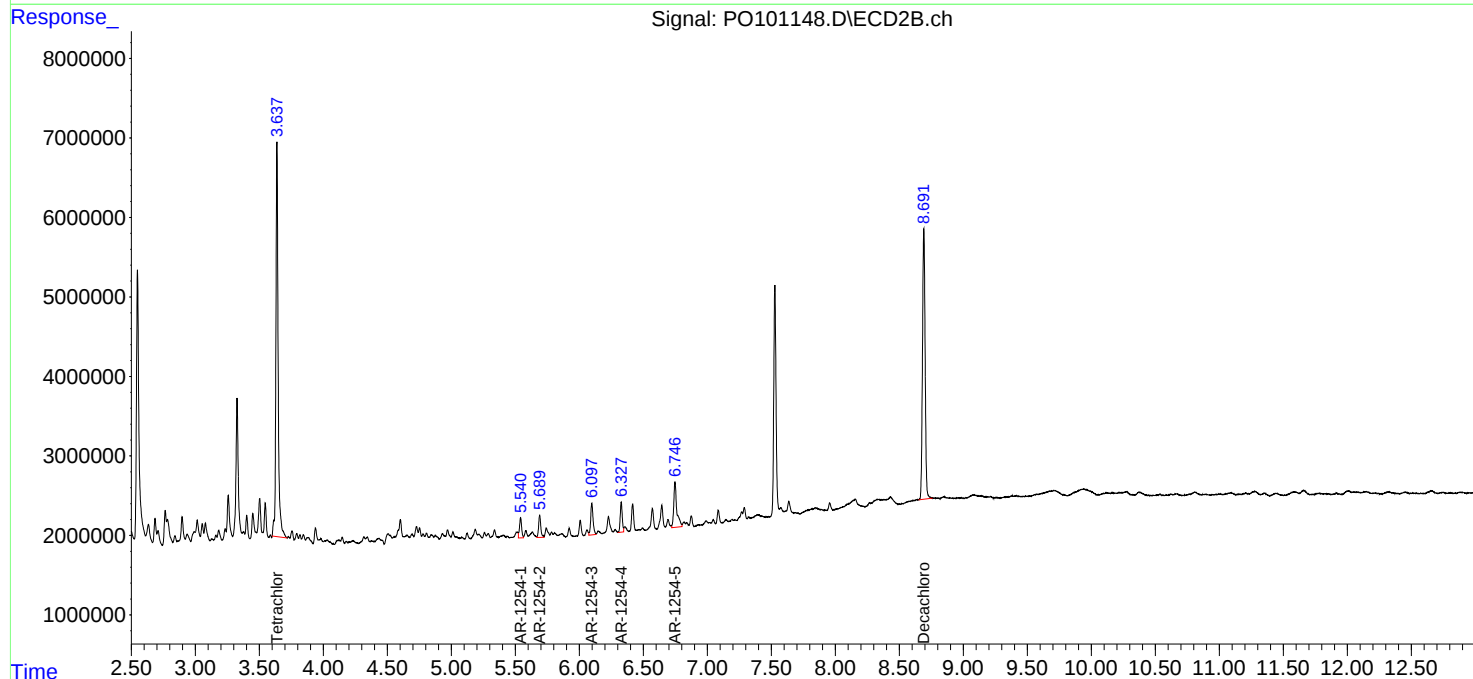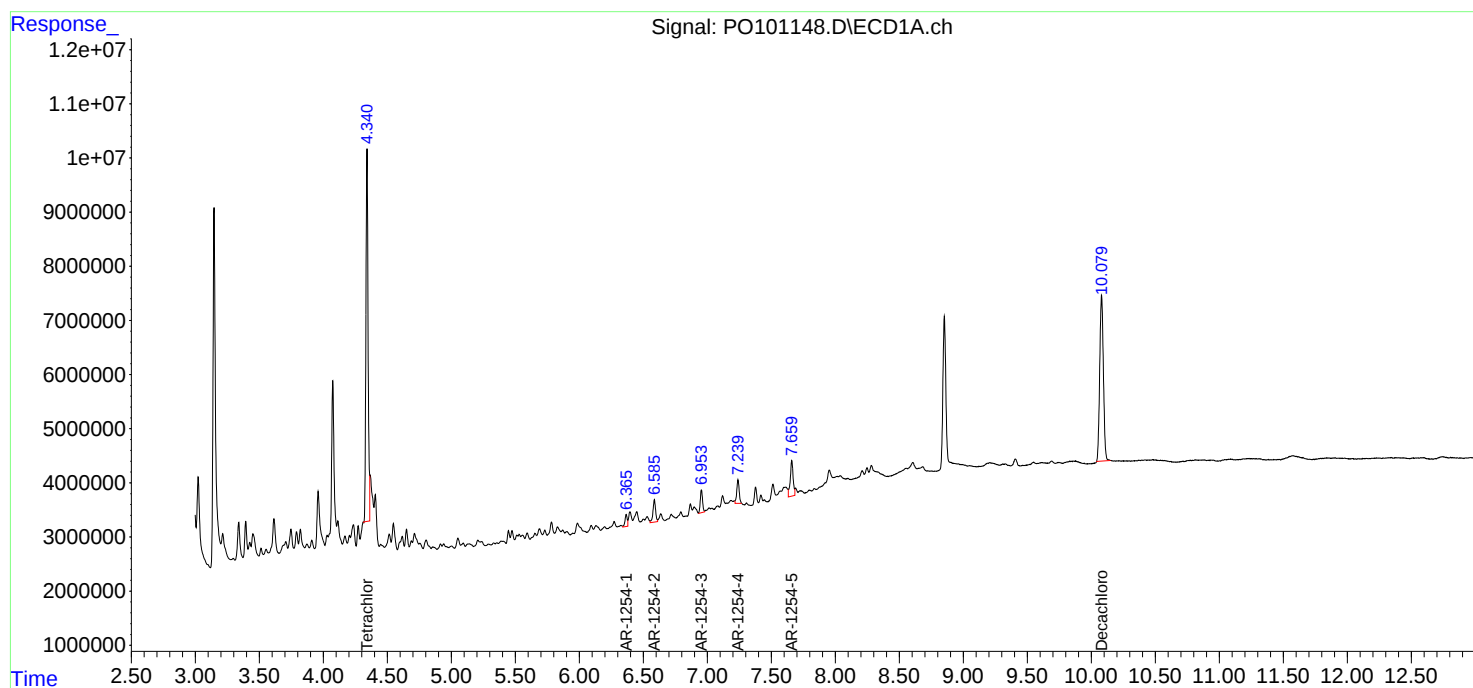


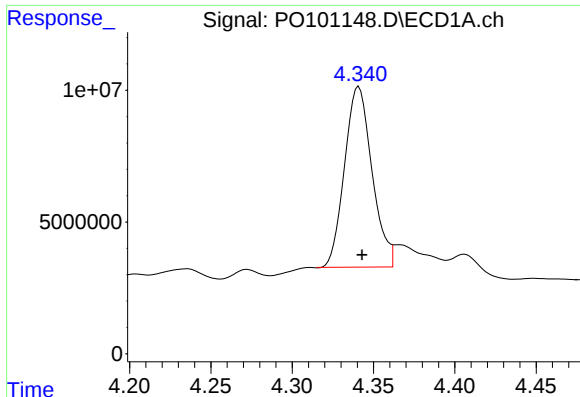

#1 Tetrachloro-m-xylene


R.T.: 4.340 min
Delta R.T.: -0.003 min
Response: 80127992
Conc: 19.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-13

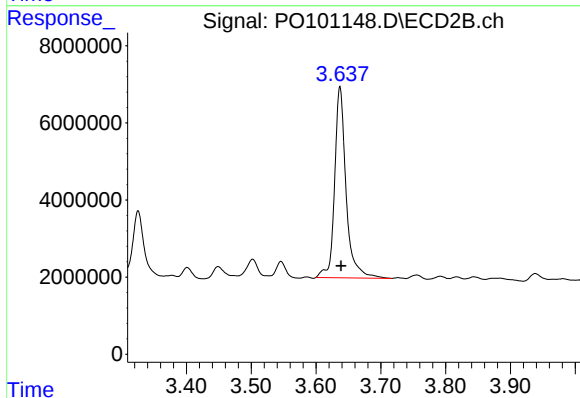


#1 Tetrachloro-m-xylene

R.T.: 3.637 min
Delta R.T.: -0.001 min
Response: 60845870
Conc: 23.08 ng/ml

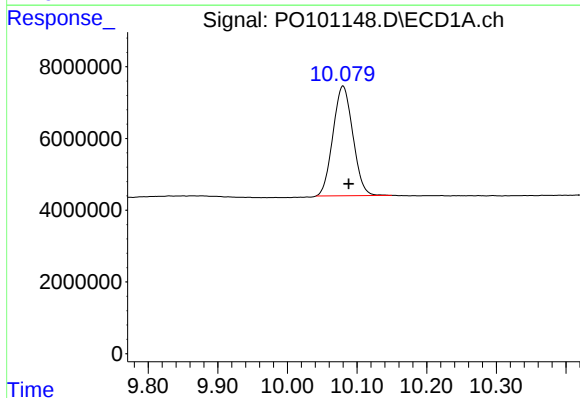


#2 Decachlorobiphenyl

R.T.: 10.080 min
Delta R.T.: -0.008 min
Response: 60777861
Conc: 30.77 ng/ml

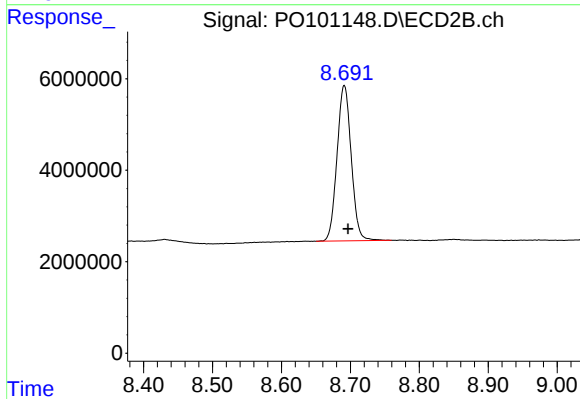

#2 Decachlorobiphenyl


R.T.: 8.691 min
Delta R.T.: -0.005 min
Response: 48671054
Conc: 29.47 ng/ml

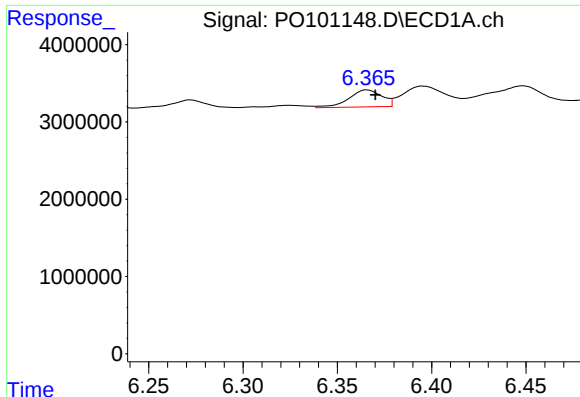

#26 AR-1254-1


R.T.: 6.366 min
Delta R.T.: -0.004 min
Response: 2679192
Conc: 22.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-13

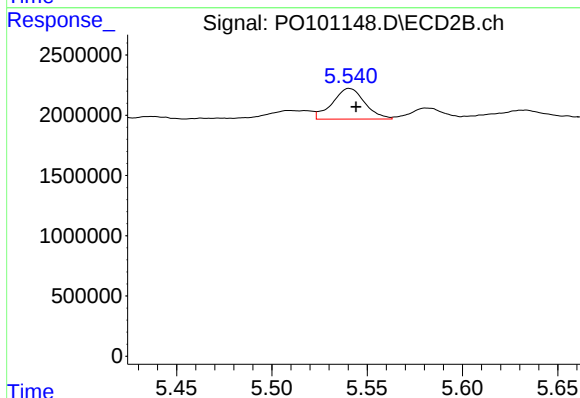


#26 AR-1254-1

R.T.: 5.541 min
Delta R.T.: -0.003 min
Response: 3021881
Conc: 24.78 ng/ml

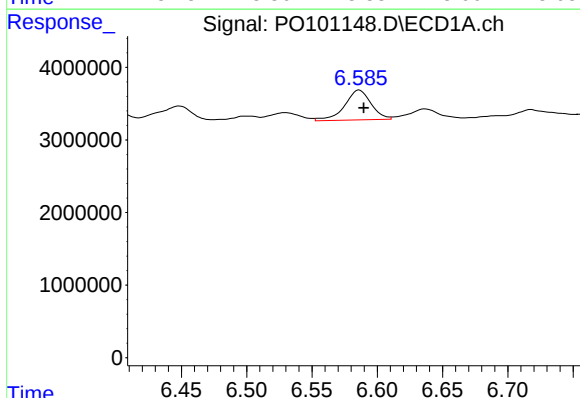


#27 AR-1254-2

R.T.: 6.586 min
Delta R.T.: -0.004 min
Response: 5819309
Conc: 34.10 ng/ml

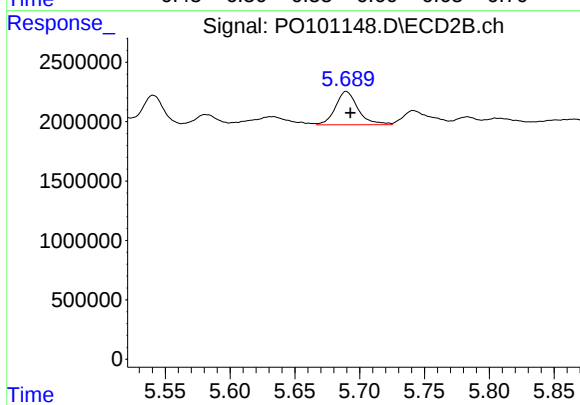

#27 AR-1254-2


R.T.: 5.690 min
Delta R.T.: -0.003 min
Response: 3401628
Conc: 31.86 ng/ml

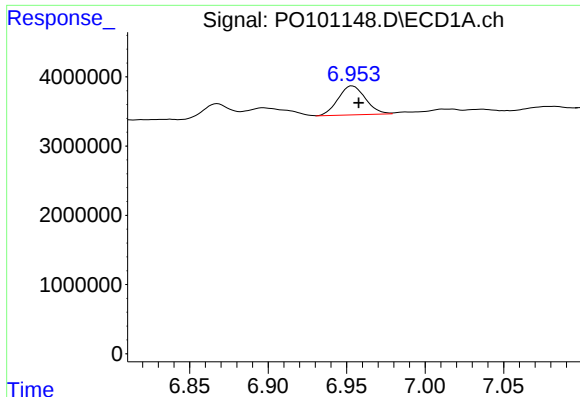

#28 AR-1254-3


R.T.: 6.954 min
Delta R.T.: -0.004 min
Response: 5103760
Conc: 31.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-13

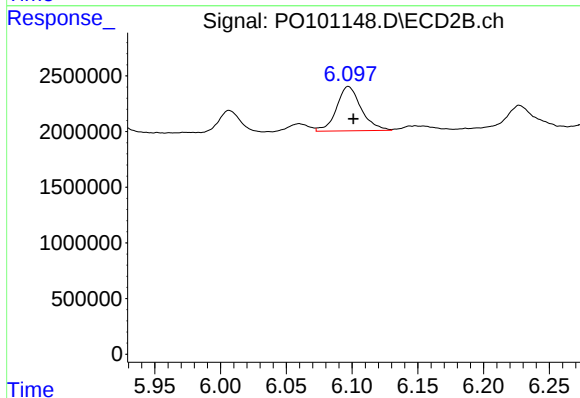


#28 AR-1254-3

R.T.: 6.097 min
Delta R.T.: -0.004 min
Response: 5194486
Conc: 32.97 ng/ml

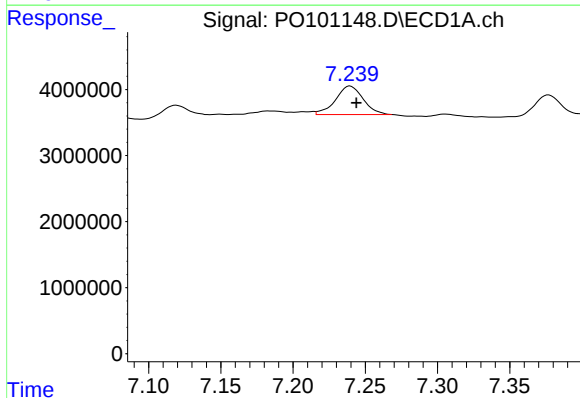


#29 AR-1254-4

R.T.: 7.239 min
Delta R.T.: -0.005 min
Response: 5726399
Conc: 57.63 ng/ml m

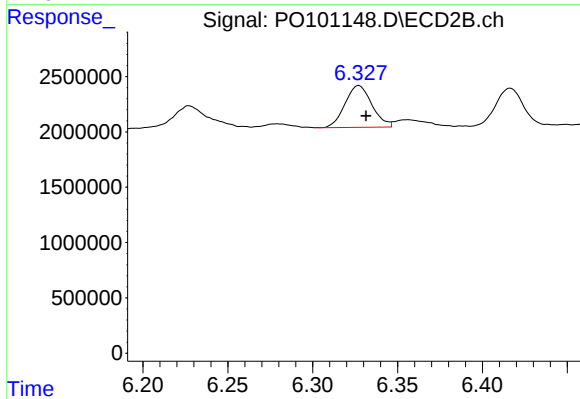

#29 AR-1254-4


R.T.: 6.327 min
Delta R.T.: -0.004 min
Response: 4169161
Conc: 50.10 ng/ml

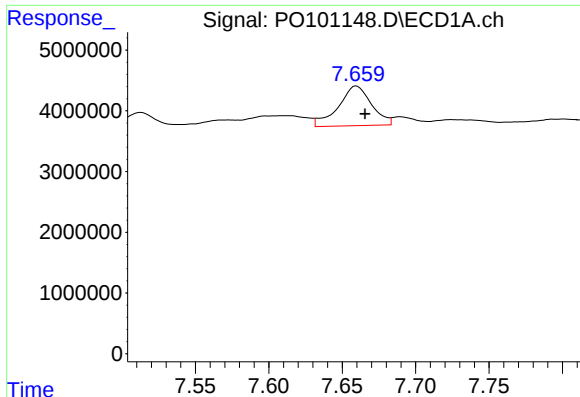

#30 AR-1254-5

R.T.: 7.660 min
Delta R.T.: -0.006 min
Response: 10314034
Conc: 86.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-13

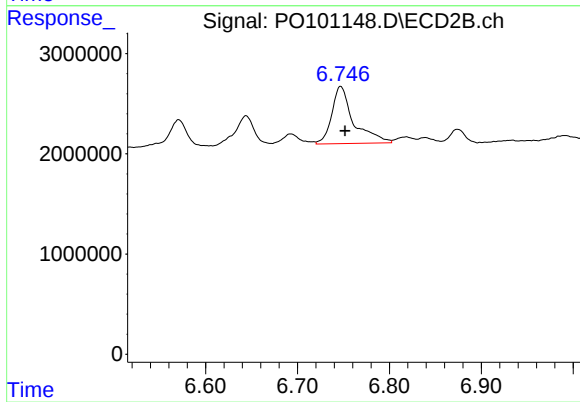

#30 AR-1254-5

R.T.: 6.747 min
Delta R.T.: -0.005 min
Response: 9432600
Conc: 70.26 ng/ml