

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0011224\
 Data File : P0101150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Jan 2024 18:26
 Operator : YP/AJ
 Sample : P1111-01DL 5X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DRYER-IDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 12 23:10:15 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0011024.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jan 11 11:52:38 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.340	3.636	20864940	13547185	5.151	5.139
2) SA Decachlor...	10.080	8.692	13652275	10366023	6.912	6.277
Target Compounds						
26) L6 AR-1254-1	6.367	5.541	22620011	24602103	188.455	201.781
27) L6 AR-1254-2	6.586	5.690	48259237	31976652	282.772	299.492
28) L6 AR-1254-3	6.954	6.098	62404857	58906586	390.561	373.939
29) L6 AR-1254-4	7.240	6.328	58151071	47717591	585.214	573.416
30) L6 AR-1254-5	7.662	6.748	98813546	104.8E6	828.949	780.726



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO011224\
Data File : PO101150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Jan 2024 18:26
Operator : YP/AJ
Sample : P1111-01DL 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DRYER-1DL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 12 23:10:15 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO011024.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jan 11 11:52:38 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

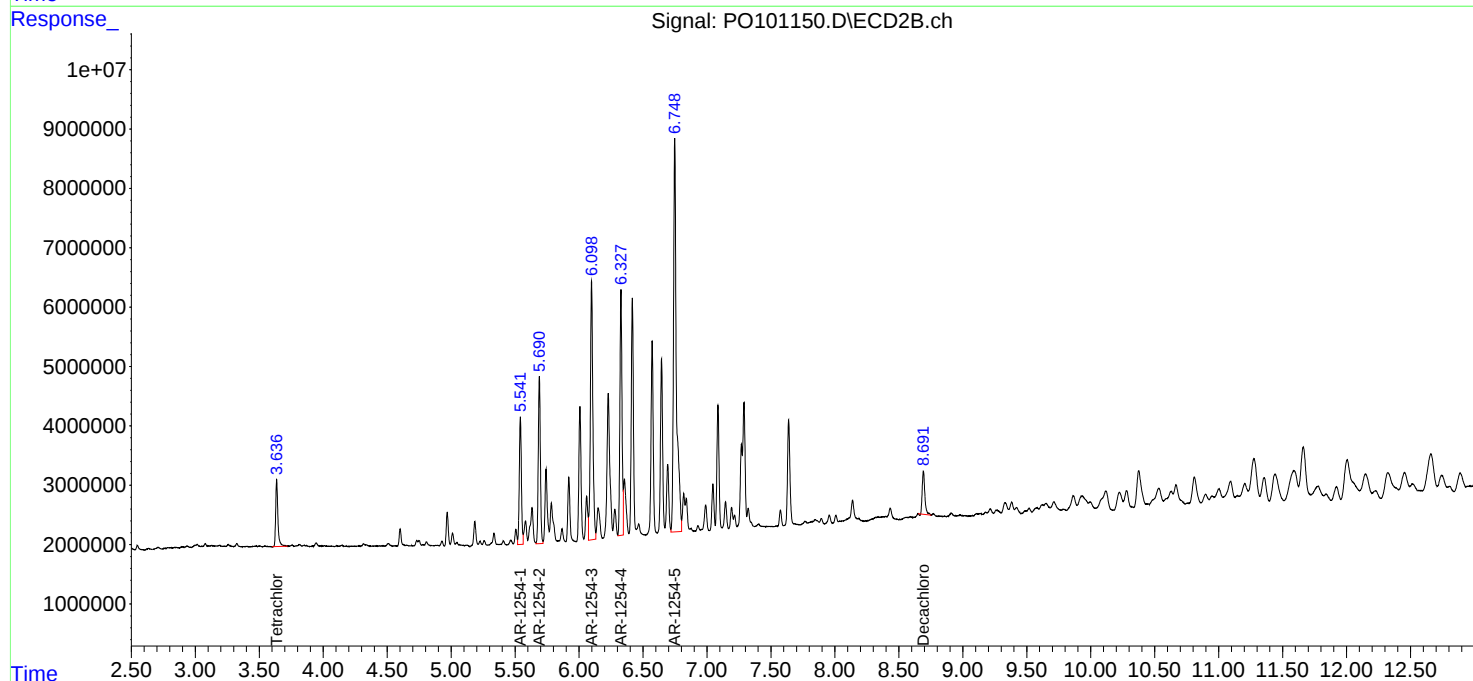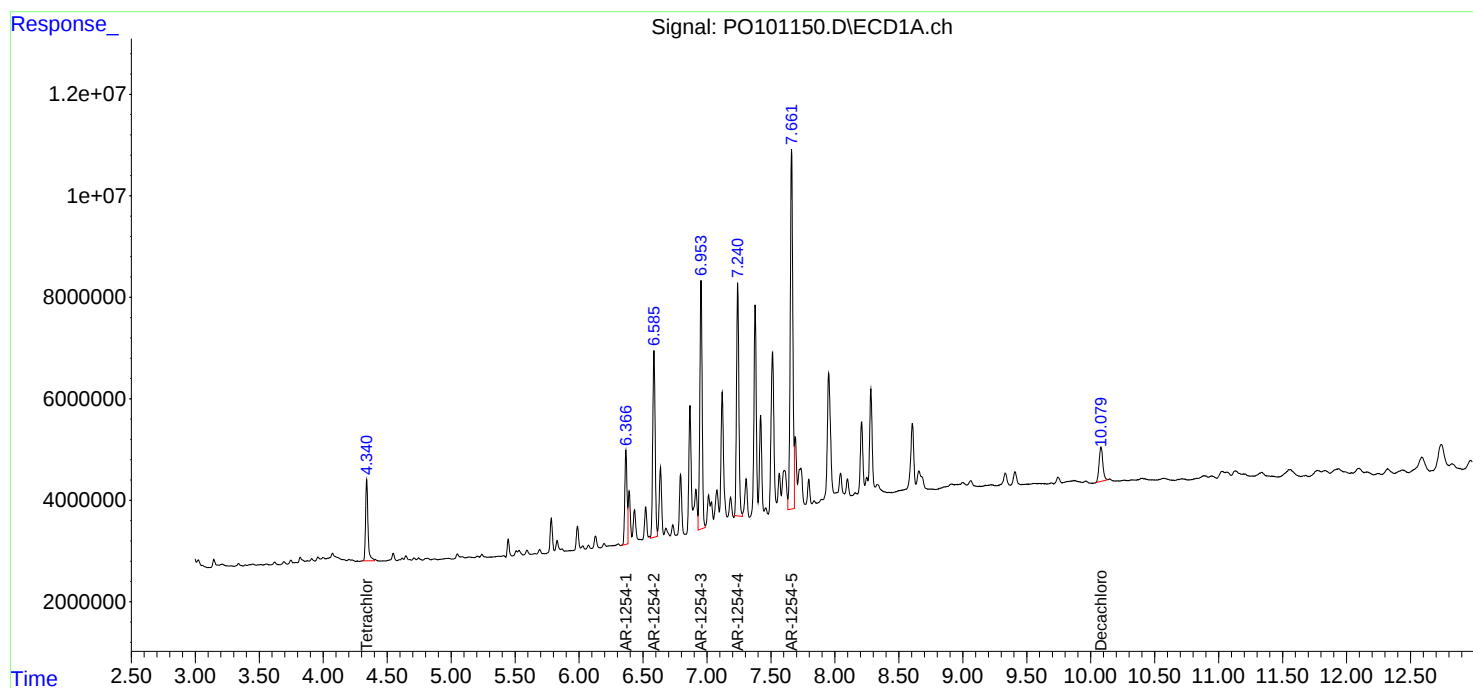


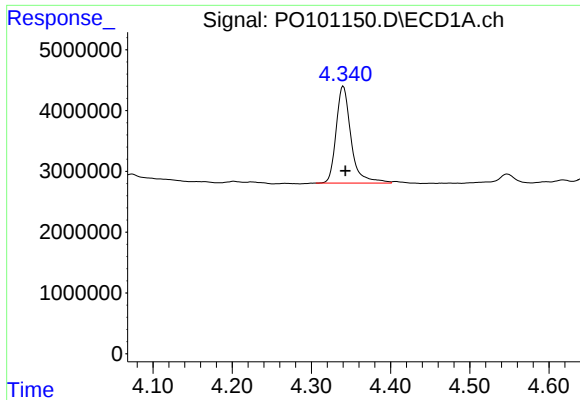

#1 Tetrachloro-m-xylene


R.T.: 4.340 min
Delta R.T.: -0.003 min
Response: 20864940
Conc: 5.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-1DL

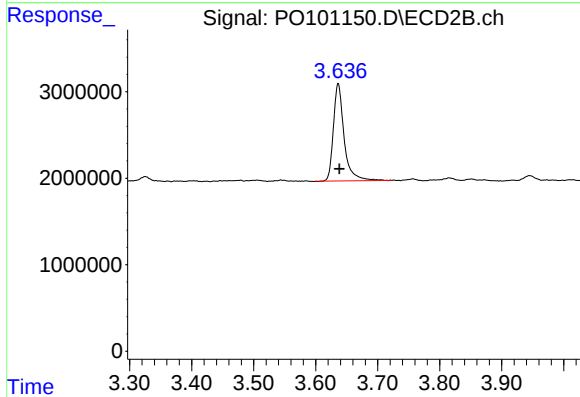


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.002 min
Response: 13547185
Conc: 5.14 ng/ml

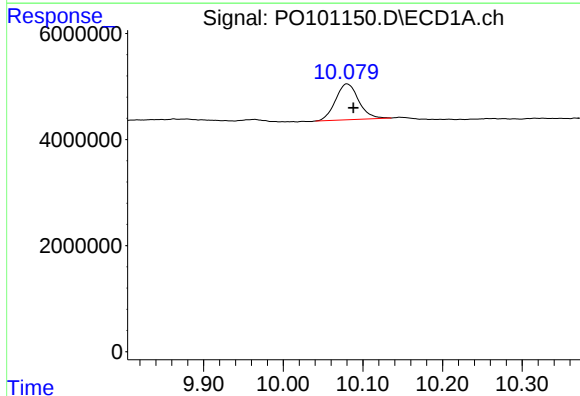


#2 Decachlorobiphenyl

R.T.: 10.080 min
Delta R.T.: -0.008 min
Response: 13652275
Conc: 6.91 ng/ml

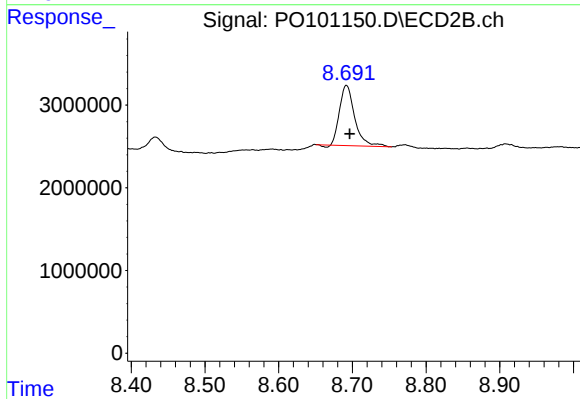

#2 Decachlorobiphenyl


R.T.: 8.692 min
Delta R.T.: -0.005 min
Response: 10366023
Conc: 6.28 ng/ml

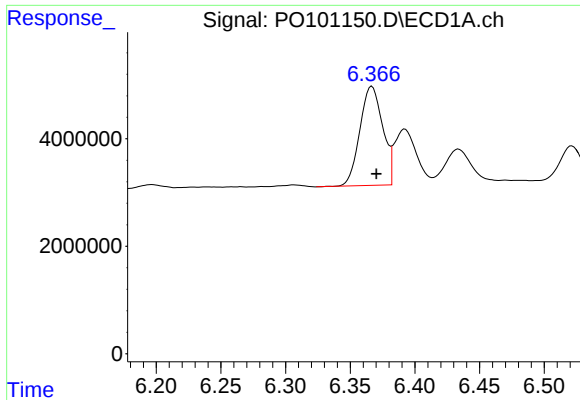

#26 AR-1254-1


R.T.: 6.367 min
Delta R.T.: -0.003 min
Response: 22620011
Conc: 188.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-1DL

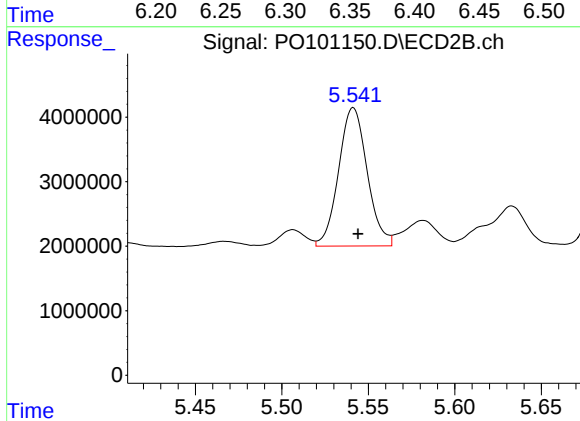


#26 AR-1254-1

R.T.: 5.541 min
Delta R.T.: -0.003 min
Response: 24602103
Conc: 201.78 ng/ml

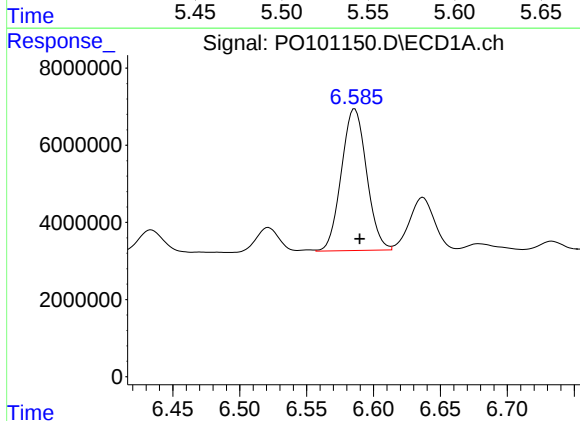


#27 AR-1254-2

R.T.: 6.586 min
Delta R.T.: -0.004 min
Response: 48259237
Conc: 282.77 ng/ml

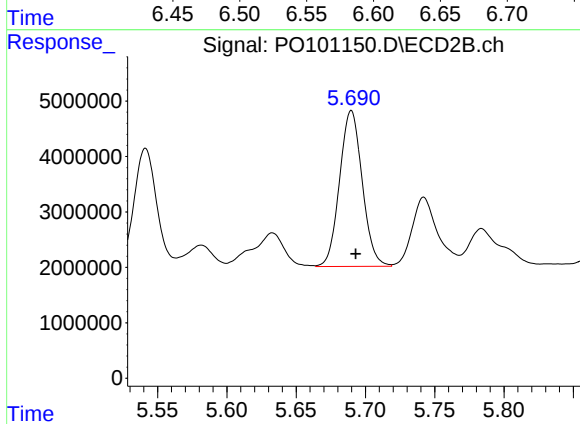

#27 AR-1254-2


R.T.: 5.690 min
Delta R.T.: -0.003 min
Response: 31976652
Conc: 299.49 ng/ml

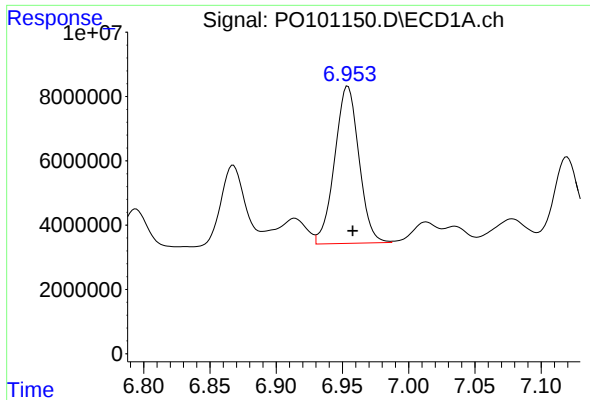

#28 AR-1254-3


R.T.: 6.954 min
Delta R.T.: -0.004 min
Response: 62404857
Conc: 390.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-1DL

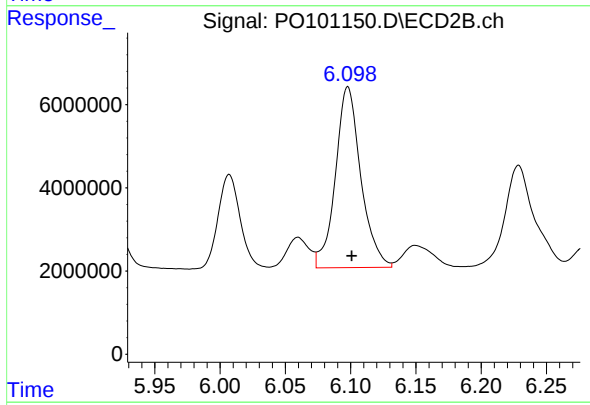


#28 AR-1254-3

R.T.: 6.098 min
Delta R.T.: -0.003 min
Response: 58906586
Conc: 373.94 ng/ml

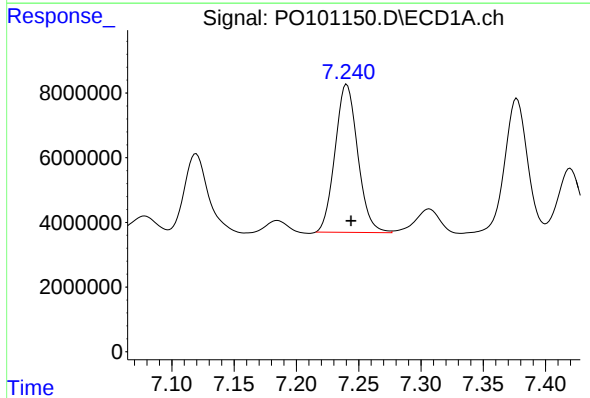


#29 AR-1254-4

R.T.: 7.240 min
Delta R.T.: -0.003 min
Response: 58151071
Conc: 585.21 ng/ml

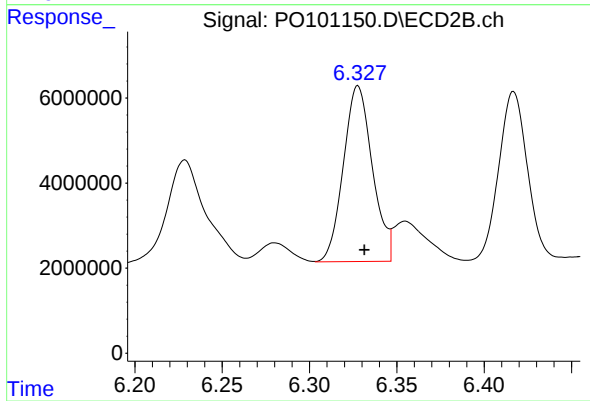

#29 AR-1254-4


R.T.: 6.328 min
Delta R.T.: -0.004 min
Response: 47717591
Conc: 573.42 ng/ml

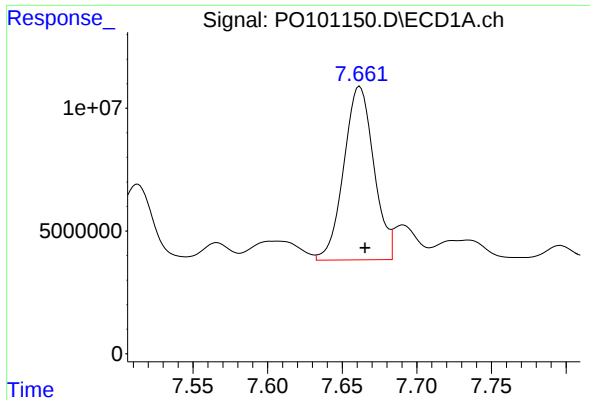

#30 AR-1254-5

R.T.: 7.662 min
Delta R.T.: -0.004 min
Response: 98813546
Conc: 828.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRYER-1DL

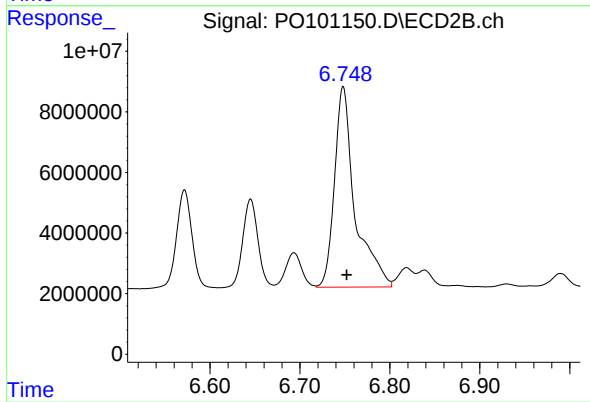

#30 AR-1254-5

R.T.: 6.748 min
Delta R.T.: -0.004 min
Response: 104812007
Conc: 780.73 ng/ml